
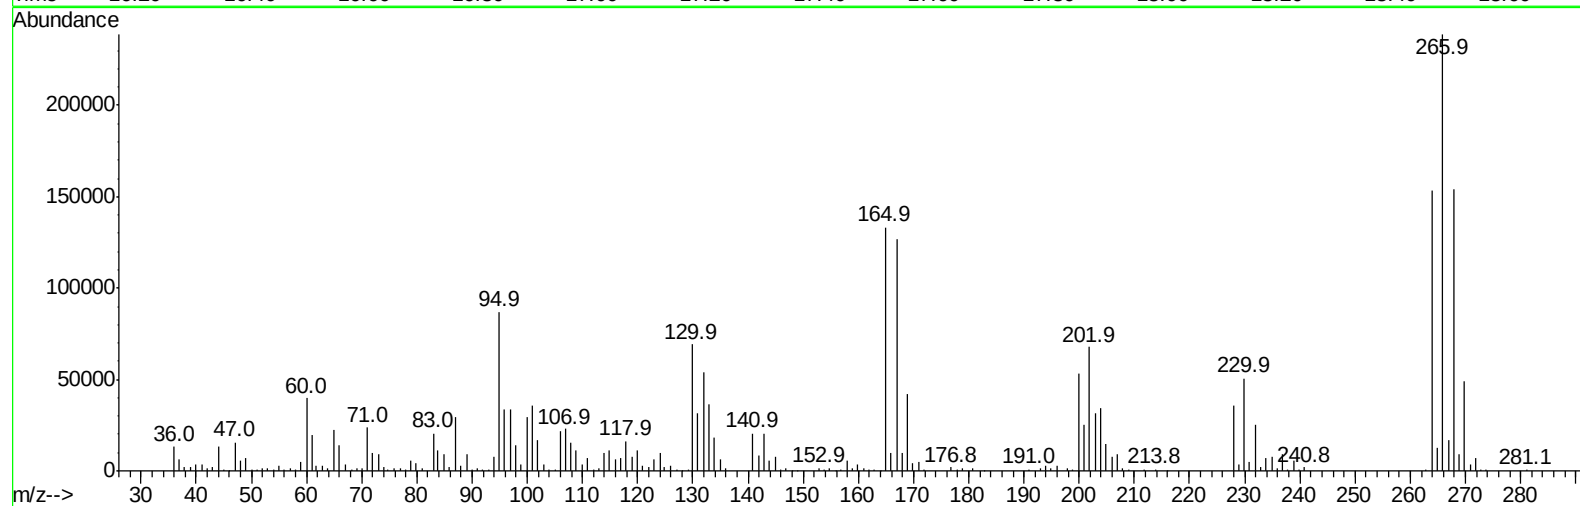


Data Path : U:\HPCHEM1\BNA N\Data\BN020118\
Data File : BN000001.D
Acq On : 01 Feb 2018 14:33
Operator :
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 05:05:49 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 19:48:39 2018
Response via : Initial Calibration

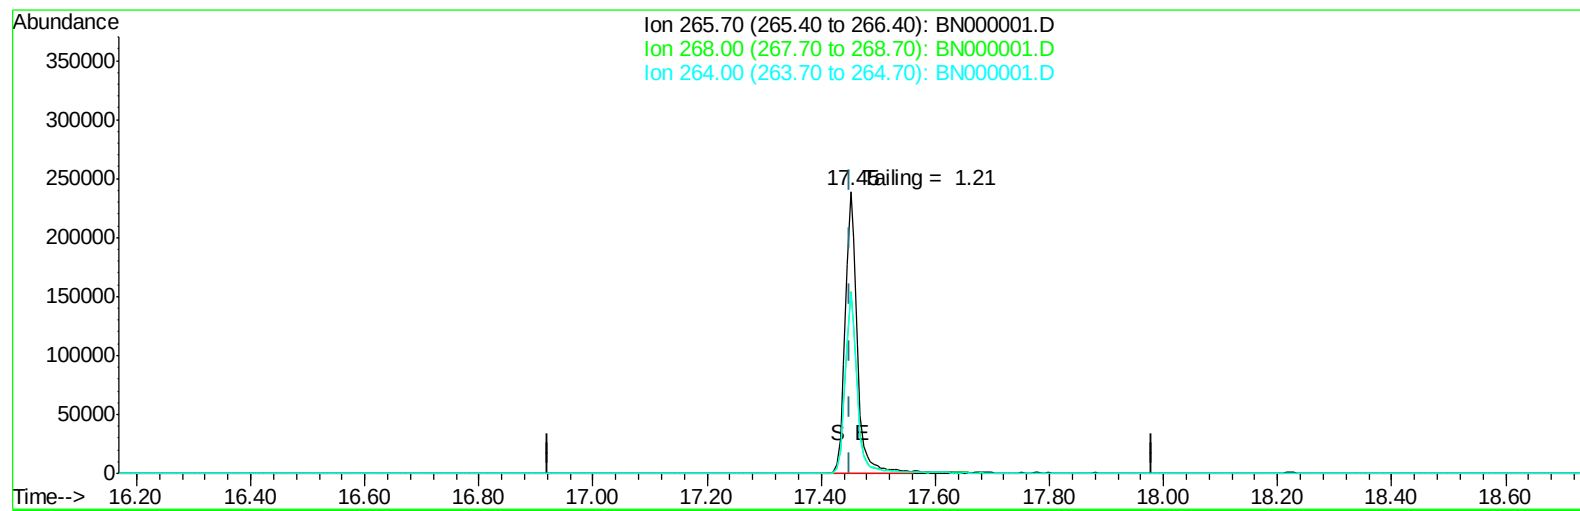

TIC: BN000001.D

(69) Pentachlorophenol (C)



17.451min (-0.000) 22588.74ng

response 355725

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.41
264.00	62.00	64.30
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA N\Data\BN020118\
Data File : BN000001.D
Acq On : 01 Feb 2018 14:33
Operator :
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 05:05:49 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 19:48:39 2018
Response via : Initial Calibration

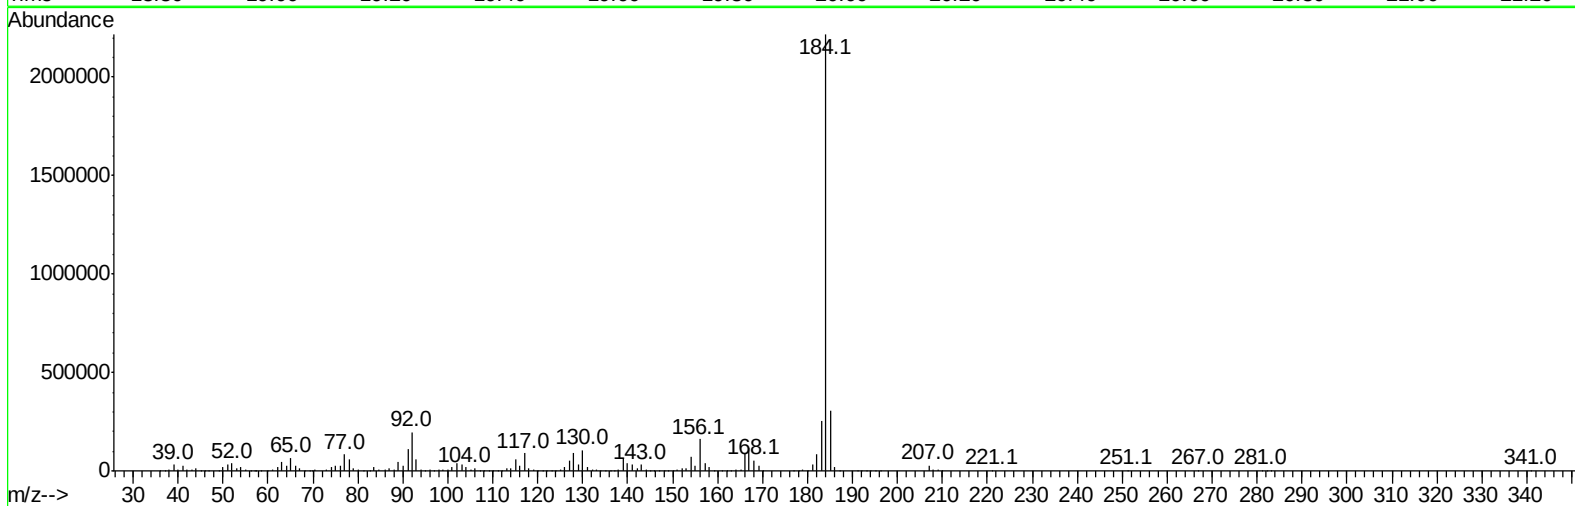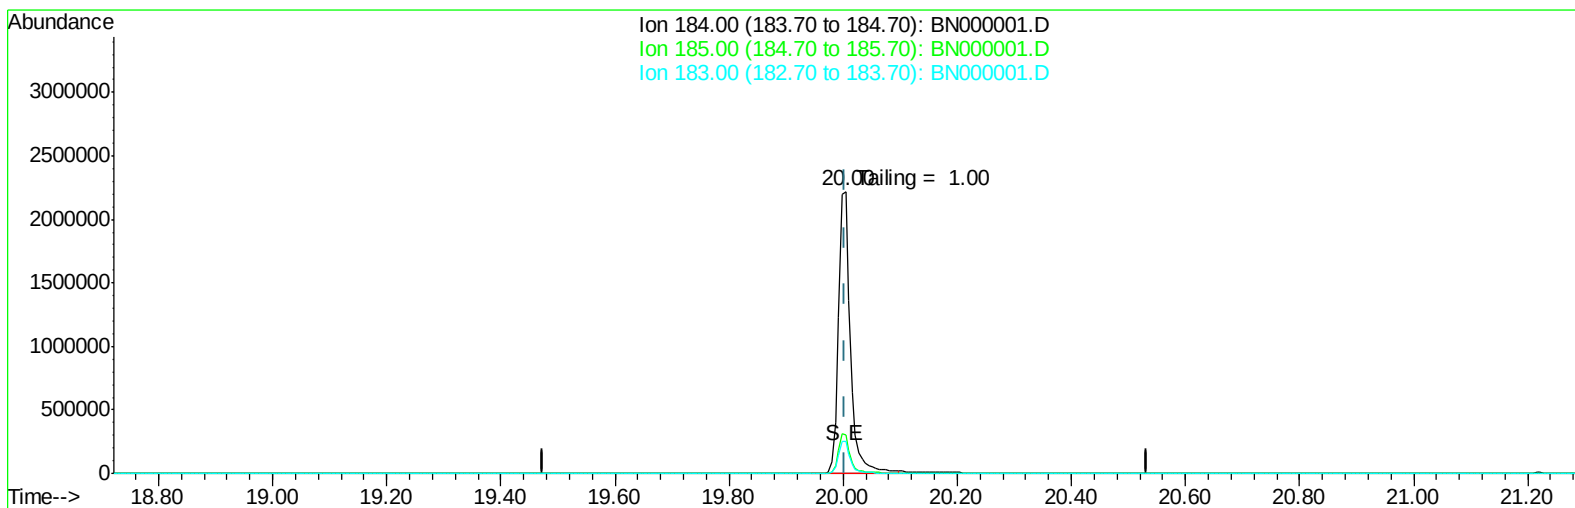

TIC: BN000001.D

(76) Benzidine

20.004min (-0.000) 0.00ng

response 3271688

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.82
183.00	13.30	11.57
0.00	0.00	0.00