


Data Path : Z:\HPCHEM1\BNA N\Data\BN020118\
 Data File : BN000001.D
 Acq On : 01 Feb 2018 14:33
 Operator :
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 06 15:24:10 2018

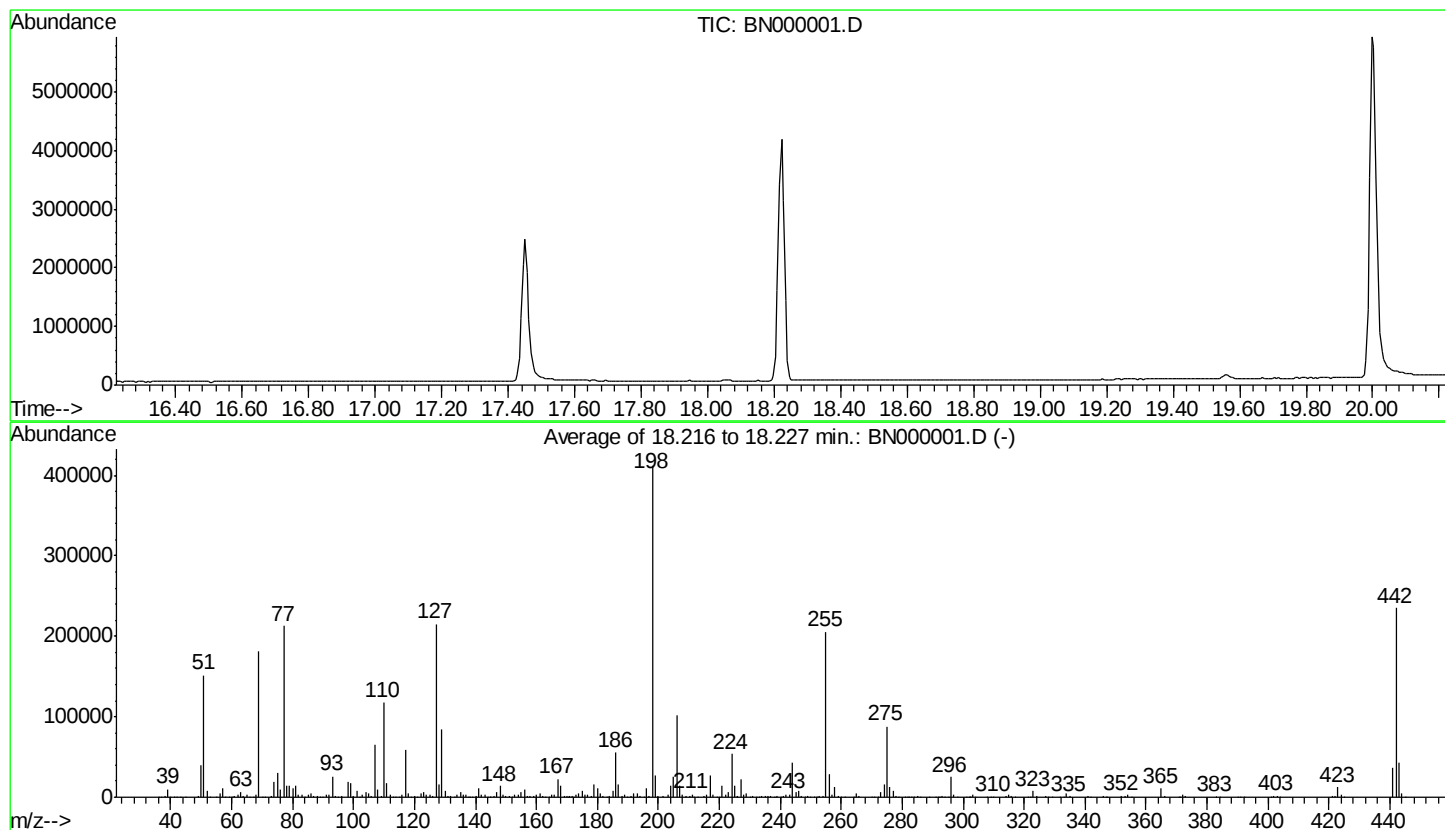

AutoFind: Scans 2589, 2590, 2591; Background Corrected with Scan 2582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	151628	PASS
68	69	0.00	2	1.7	3036	PASS
69	198	0.00	100	44.0	181176	PASS
70	69	0.00	2	0.4	692	PASS
127	198	10	80	52.2	214954	PASS
197	198	0.00	2	0.5	2131	PASS
198	198	100	100	100.0	412032	PASS
199	198	5	9	6.7	27656	PASS
275	198	10	60	21.4	87970	PASS
365	198	1	100	2.5	10431	PASS
441	443	0.01	100	83.6	36165	PASS
442	198	50	100	57.0	234986	PASS
443	442	15	24	18.4	43282	PASS