
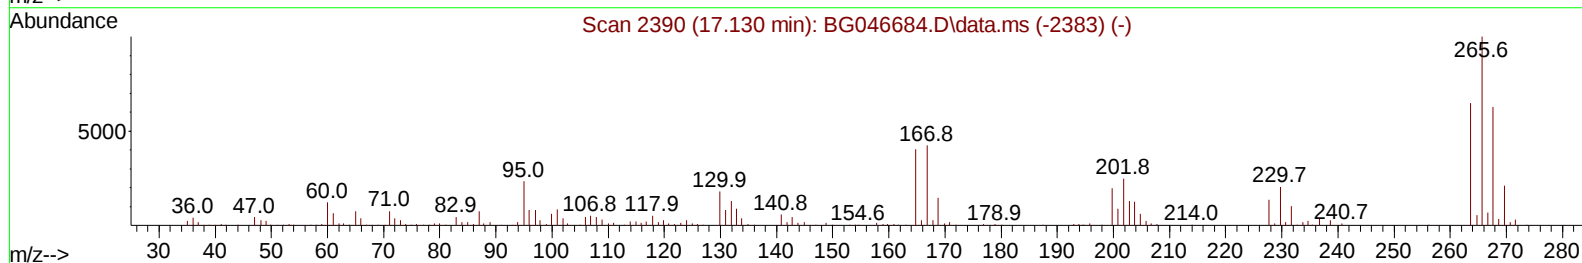
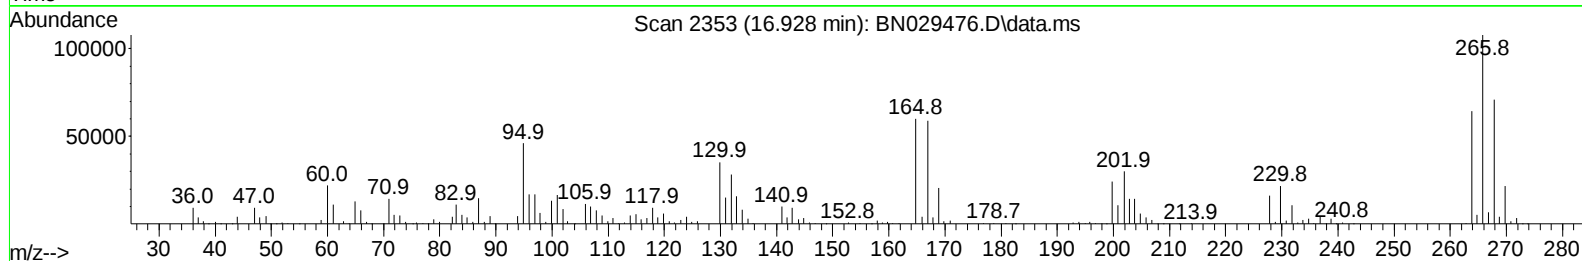


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020124\
Data File : BN029476.D
Acq On : 01 Feb 2024 08:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 02 02:35:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 02 02:35:20 2024
Response via : Initial Calibration

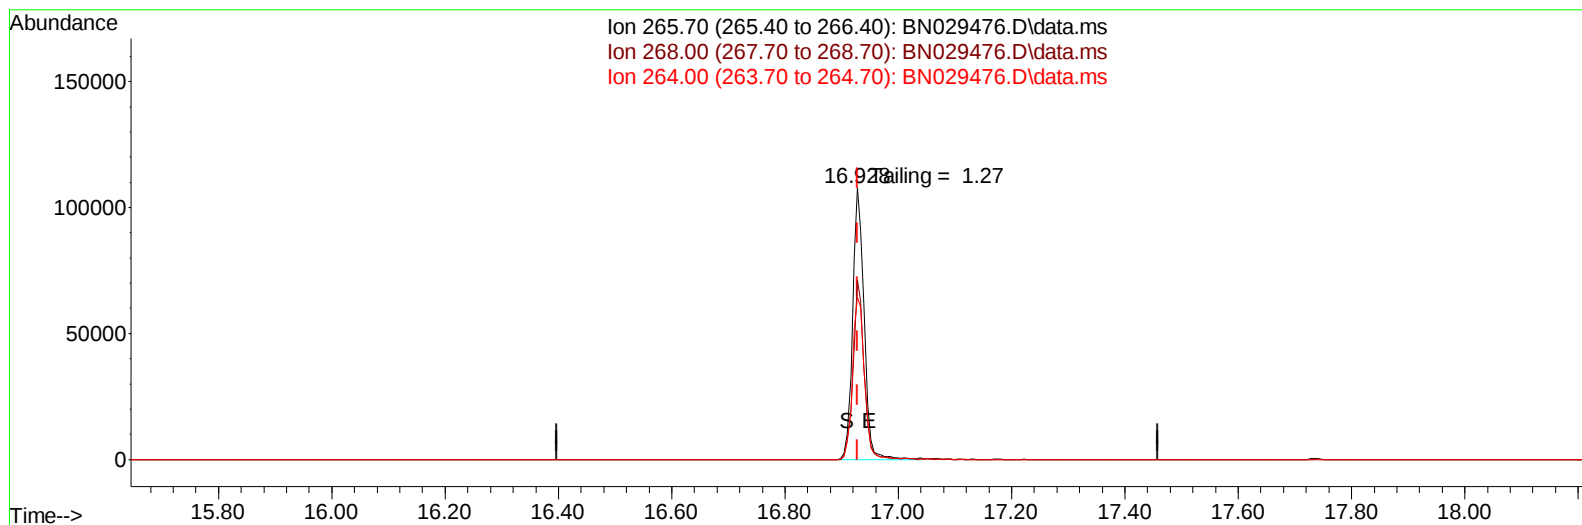




TIC: BN029476.D\data.ms

(70) Pentachlorophenol (C)**16.928min (0.000) 17034.58 ng****response 151864**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.85
264.00	61.60	59.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020124\
Data File : BN029476.D
Acq On : 01 Feb 2024 08:36
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Feb 02 02:35:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 02 02:35:20 2024
Response via : Initial Calibration

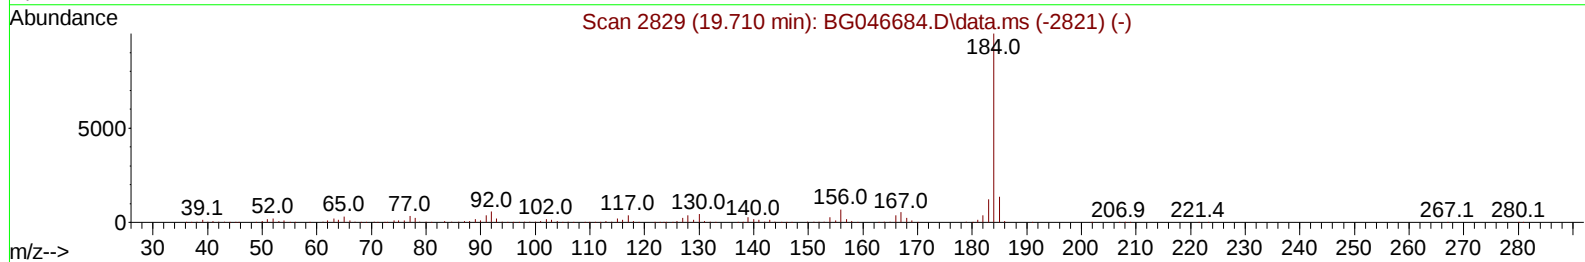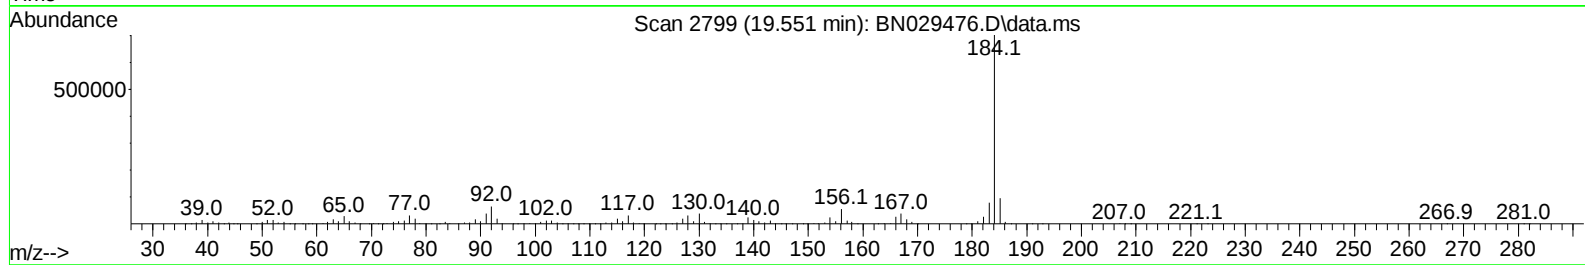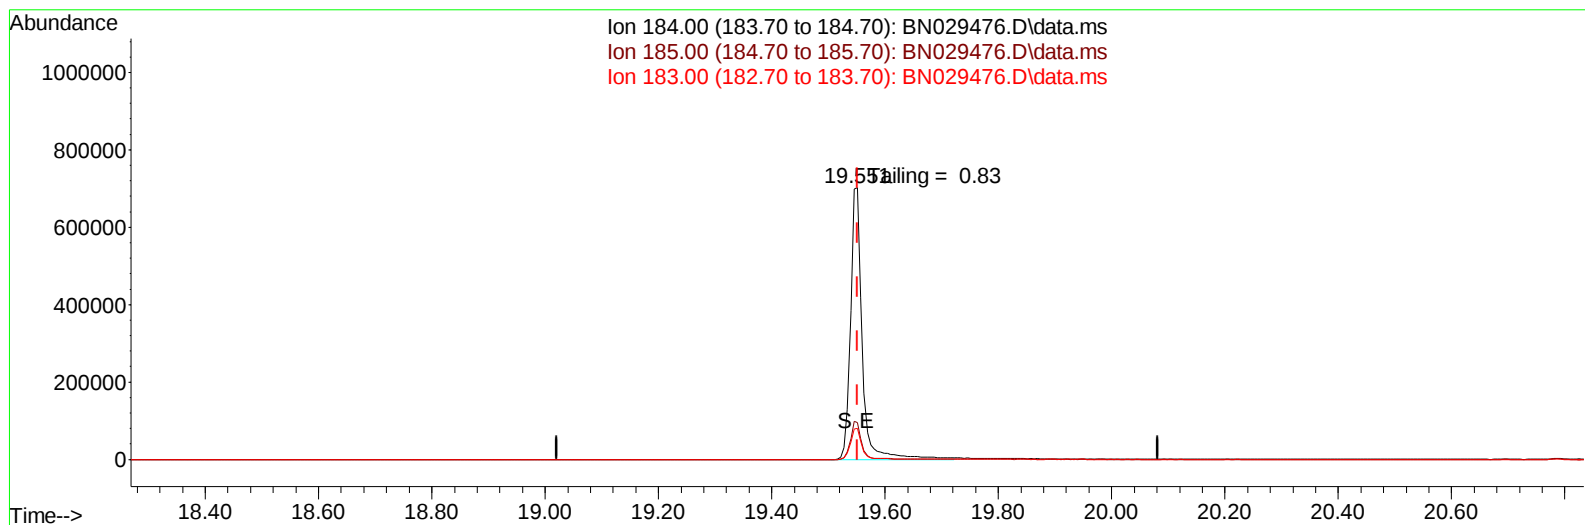

TIC: BN029476.D\data.ms

(77) Benzidine

19.551min (0.000) 0.00 ng

response 1011195

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.59
183.00	13.20	11.36
0.00	0.00	0.00