
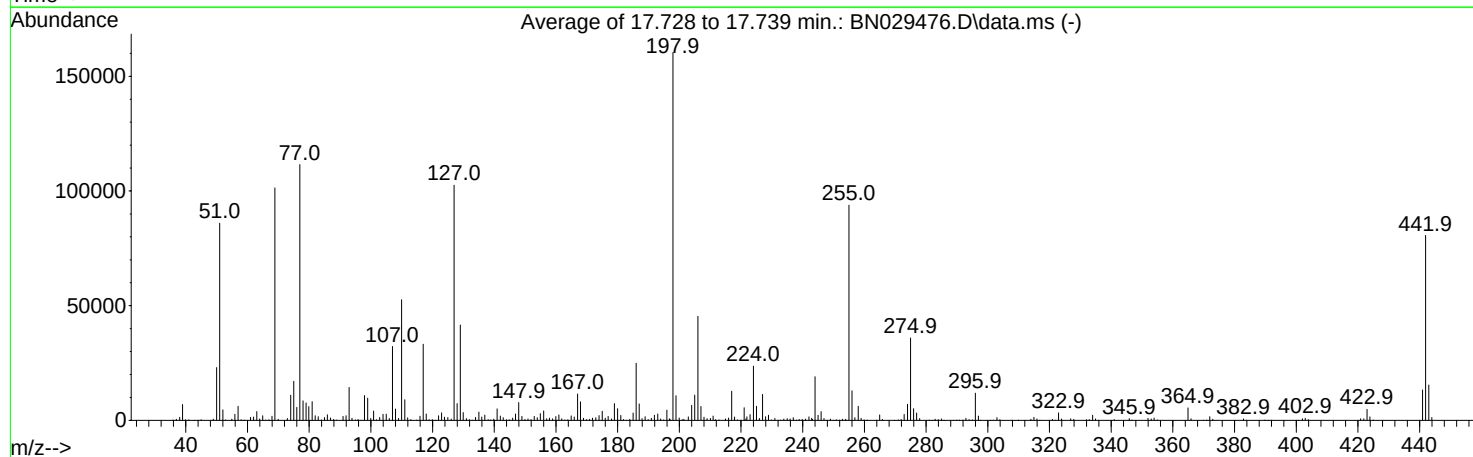


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020124\
Data File : BN029476.D
Acq On : 01 Feb 2024 08:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 01:51:59 2024

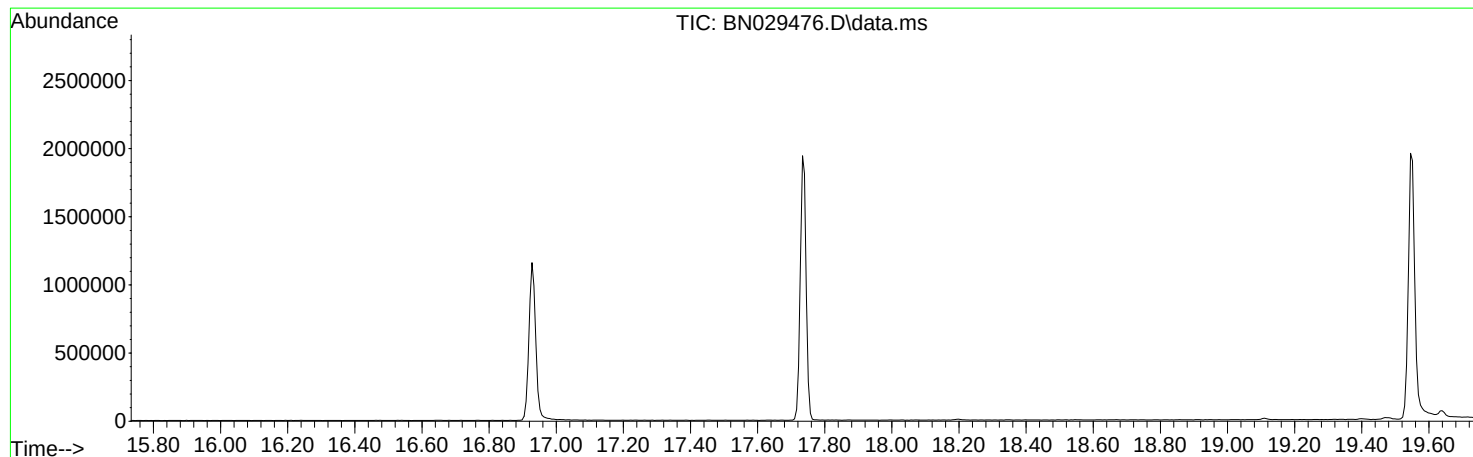




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.6	85925	PASS
68	69	0.00	2	1.8	1841	PASS
69	198	0.00	100	63.2	101376	PASS
70	69	0.00	2	0.5	484	PASS
127	198	10	80	64.0	102563	PASS
197	198	0.00	2	0.4	685	PASS
198	198	100	100	100.0	160379	PASS
199	198	5	9	6.7	10715	PASS
275	198	10	60	22.4	35957	PASS
365	198	1	100	3.4	5421	PASS
441	198	0.01	100	8.2	13225	PASS
442	442	50	100	100.0	80637	PASS
443	442	15	24	19.1	15412	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020124\
Data File : BN029476.D
Acq On : 01 Feb 2024 08:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 02 02:35:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 02 02:35:20 2024
Response via : Initial Calibration

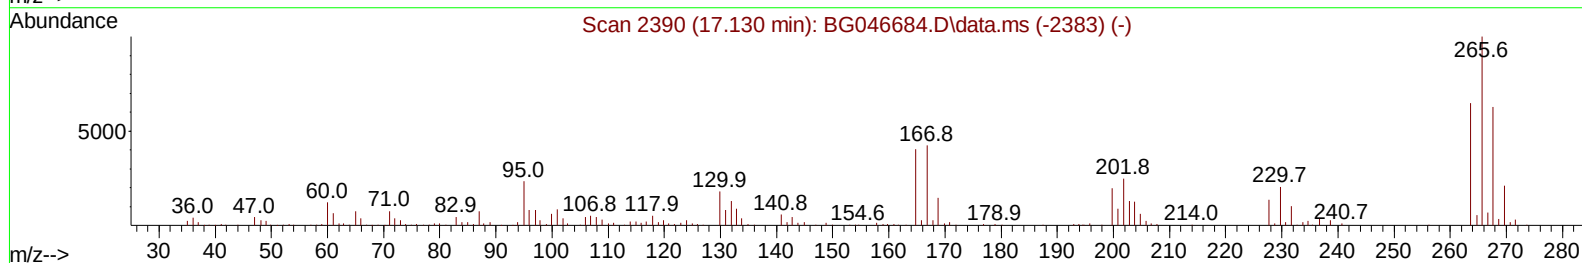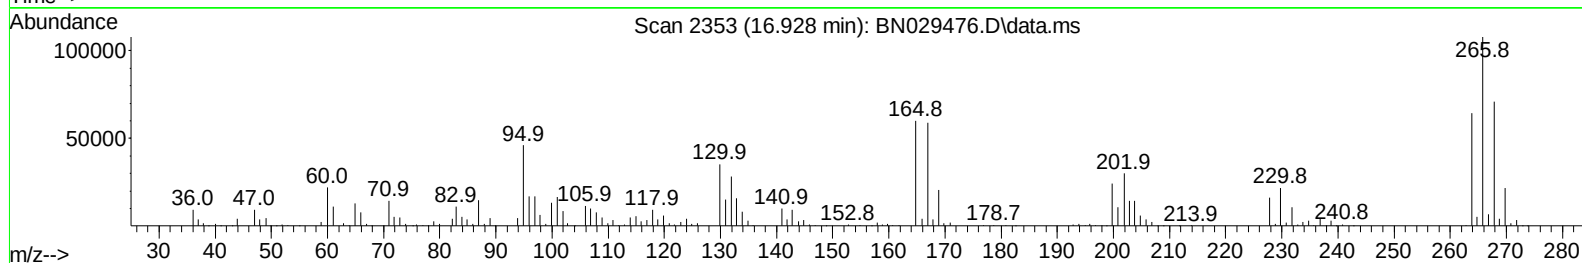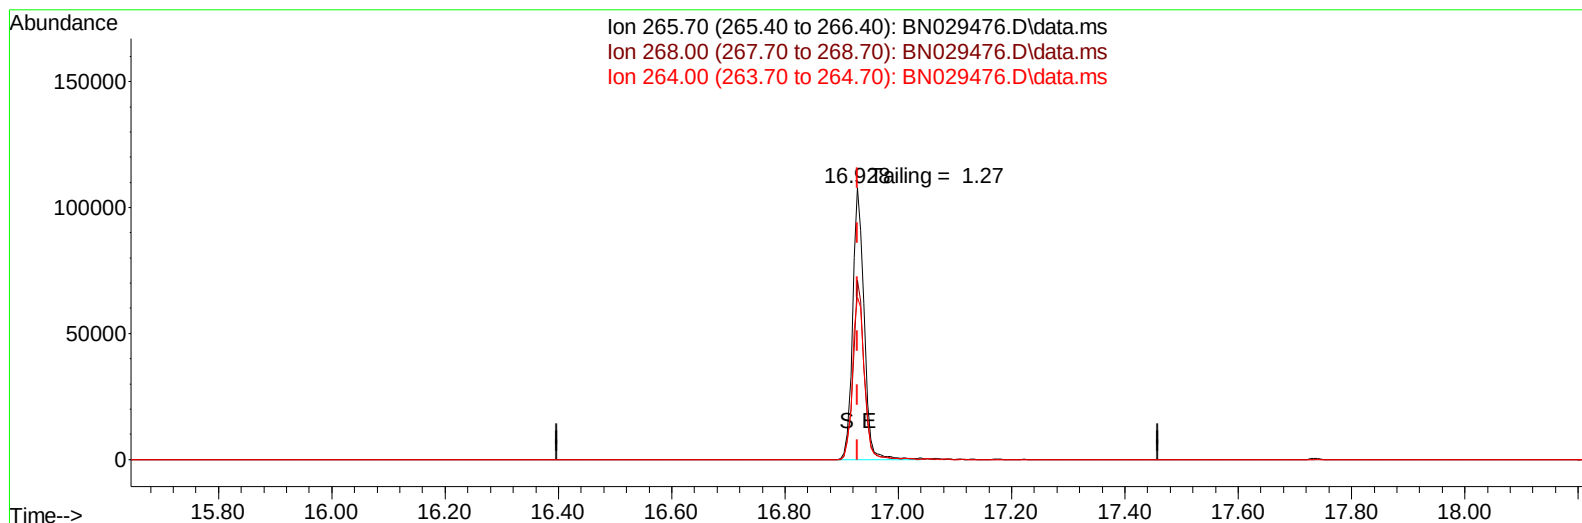

TIC: BN029476.D\data.ms

(70) Pentachlorophenol (C)

16.928min (0.000) 17034.58 ng




response 151864

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.85
264.00	61.60	59.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020124\
Data File : BN029476.D
Acq On : 01 Feb 2024 08:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 02 02:35:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 02 02:35:20 2024
Response via : Initial Calibration

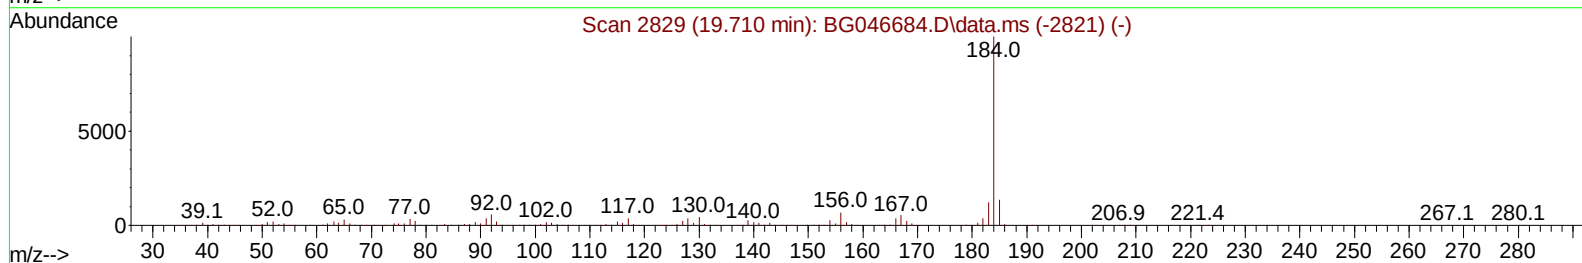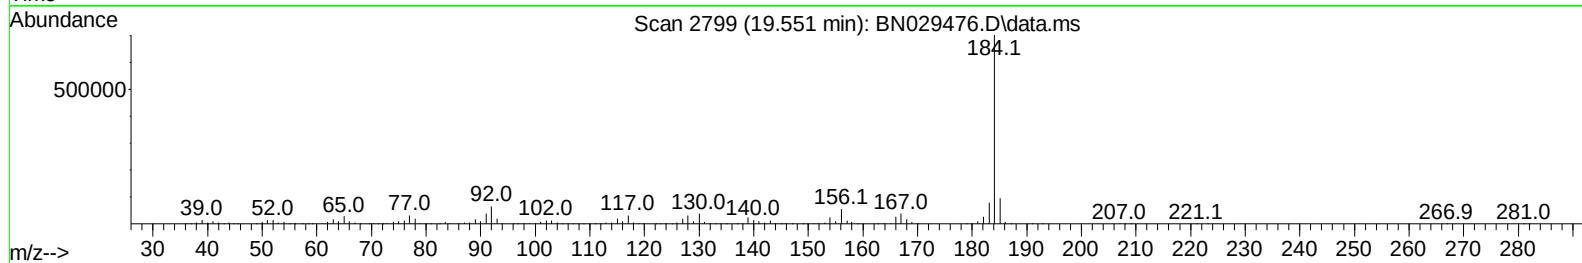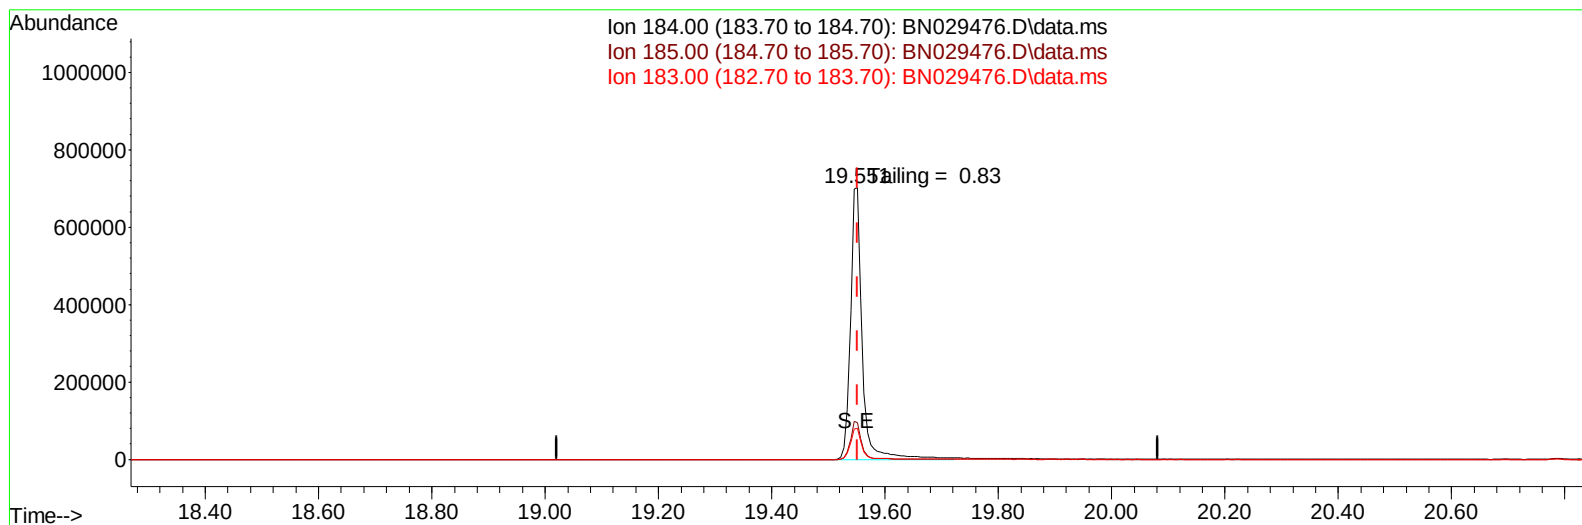

TIC: BN029476.D\data.ms

(77) Benzidine

19.551min (0.000) 0.00 ng

response 1011195

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.59
183.00	13.20	11.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/1/2024	BNA_N	<u>BN029476.D</u>
Compound Name	Response	Retention Time
DDT	488447	20.786
DDD	5366	20.348
DDE	0	19.828
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5366	493813	1.09

Instrument :
BNA_N
ClientSampleId :
DFTPP