

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
 Data File : BN018549.D
 Acq On : 02 Feb 2022 14:53
 Operator : CG/JU
 Sample : PB142347BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK347

Quant Time: Feb 02 17:15:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 02 14:08:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	441	0.400	ng/ul	0.00
4) Naphthalene-d8	10.733	136	1586	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.558	164	886	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.293	188	1695	0.400	ng/ul #	0.00
17) Chrysene-d12	21.464	240	1267	0.400	ng/ul #	0.00
23) Perylene-d12	23.861	264	1324	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.294	96	2797	5.524	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.317	152	678	0.314	ng/ul	0.00
18) Fluoranthene-d10	19.314	212	1434	0.396	ng/ul	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.943	266	32	0.101	ng/ul	89
20) Pyrene	19.681	202	210	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.709	252	491	0.105	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
Data File : BN018549.D
Acq On : 02 Feb 2022 14:53
Operator : CG/JU
Sample : PB142347BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK347


Quant Time: Feb 02 17:15:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:08:46 2022
Response via : Initial Calibration

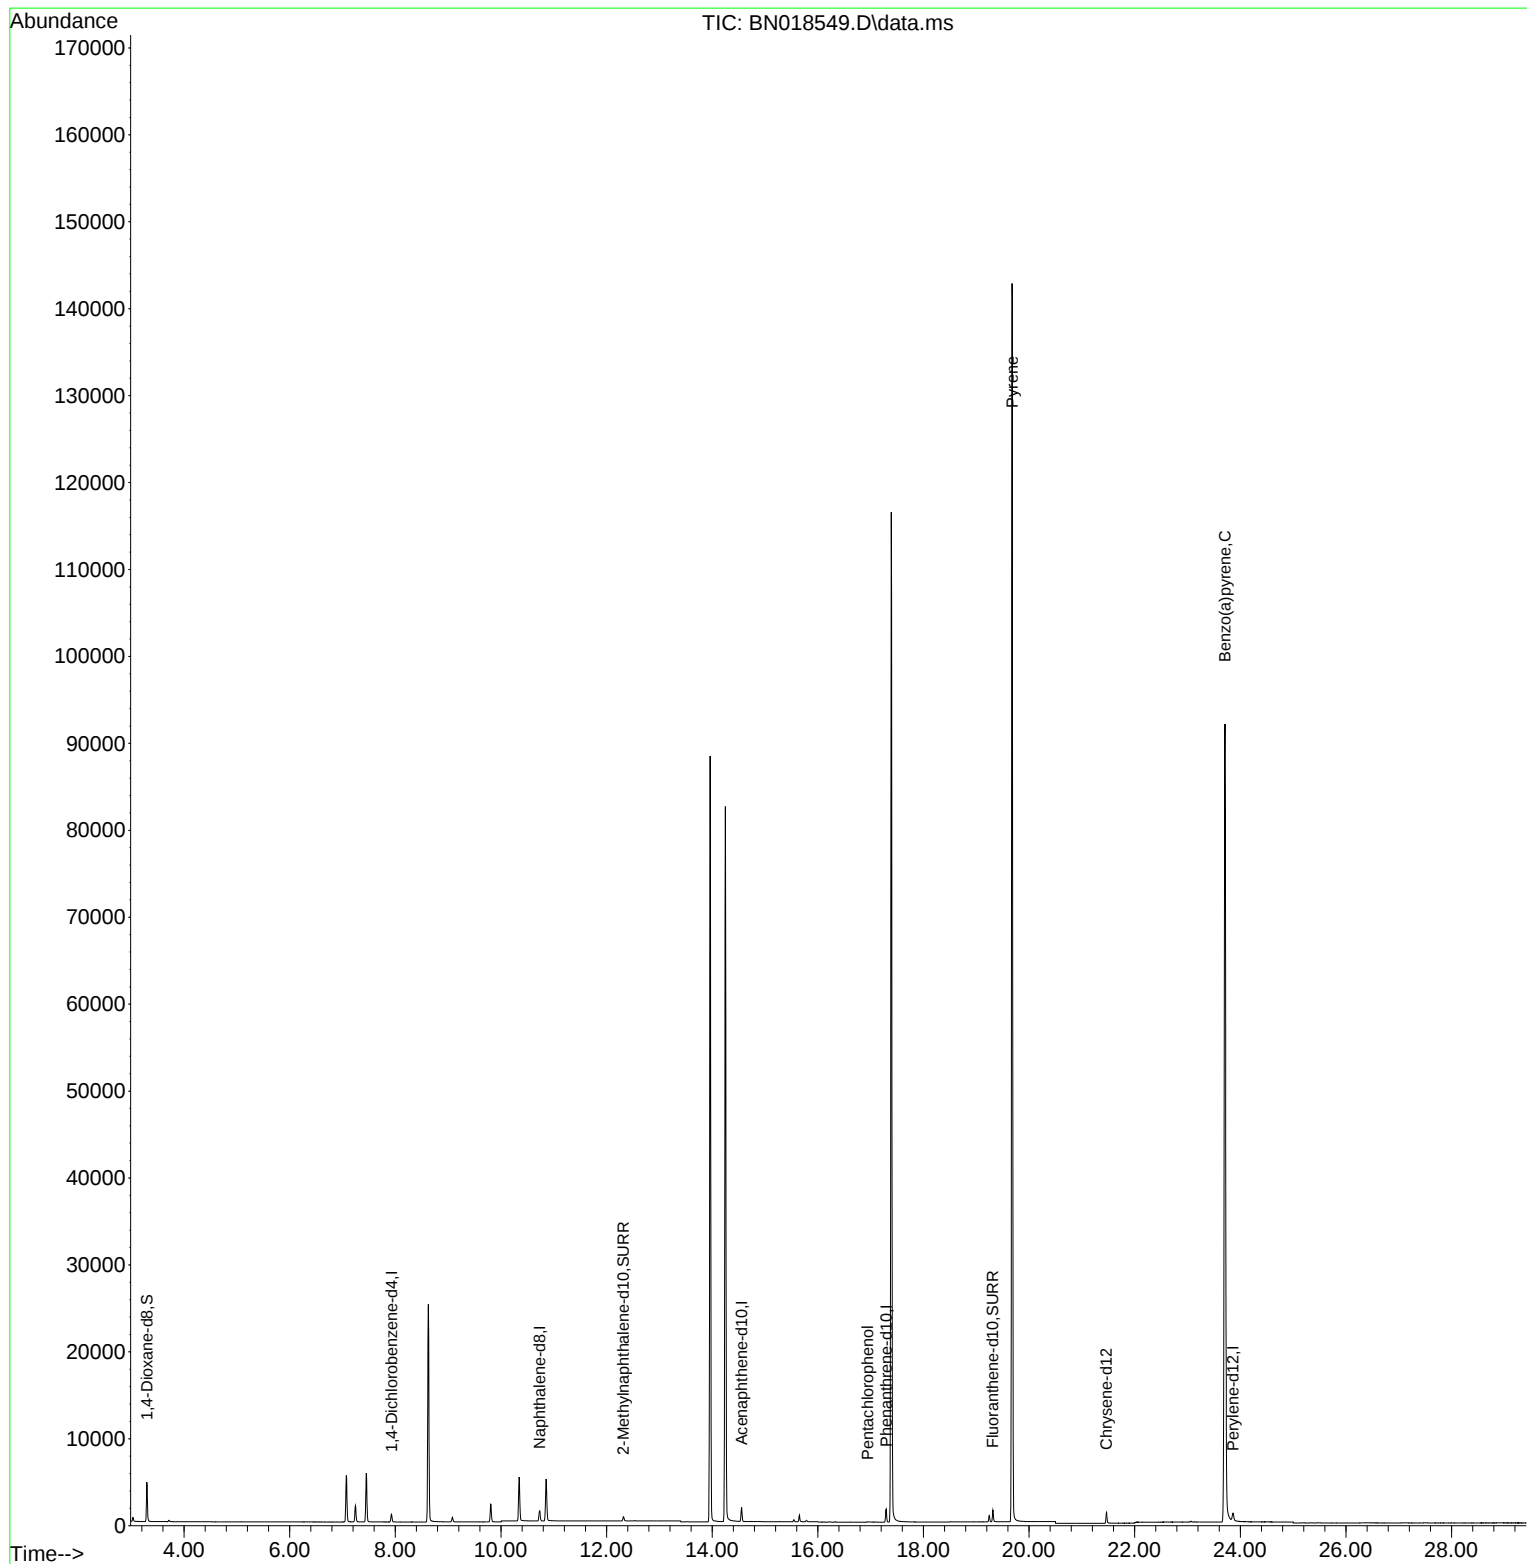

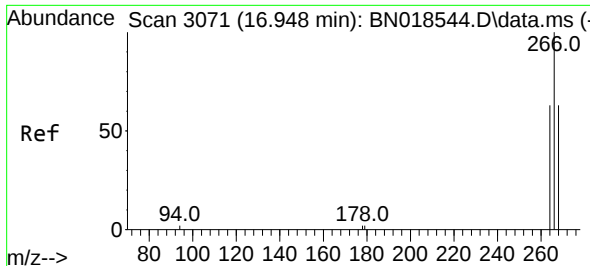




#14
 Pentachlorophenol
 Concen: 0.101 ng/ul
 RT: 16.943 min Scan# 3070
 Delta R.T. -0.005 min
 Lab File: BN018549.D
 Acq: 02 Feb 2022 14:53

Instrument :
 BNA_N
 ClientSampleId :
 SBLK347

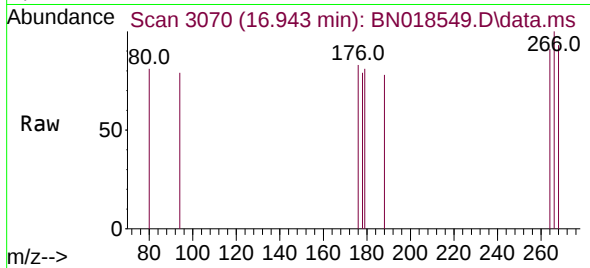

Tgt Ion:266 Resp: 32




Ion	Ratio	Lower	Upper
266	100		
264	68.8	49.9	74.9
268	75.0	51.7	77.5

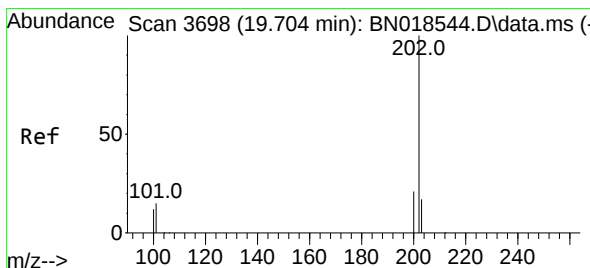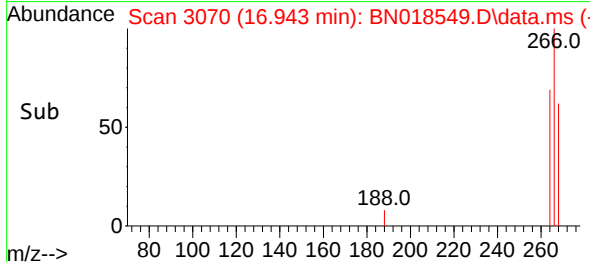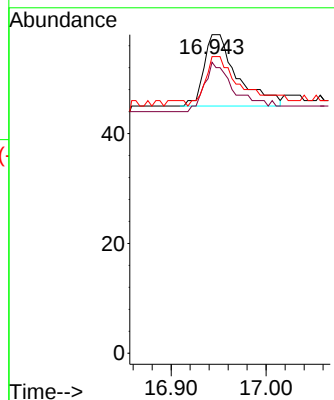


#20
 Pyrene
 Concen: 0.041 ng/ul
 RT: 19.681 min Scan# 3693
 Delta R.T. -0.024 min
 Lab File: BN018549.D
 Acq: 02 Feb 2022 14:53

Tgt Ion:202 Resp: 210

Ion	Ratio	Lower	Upper
202	100		
101	136.8	9.0	13.4#
100	836.8	7.0	10.4#

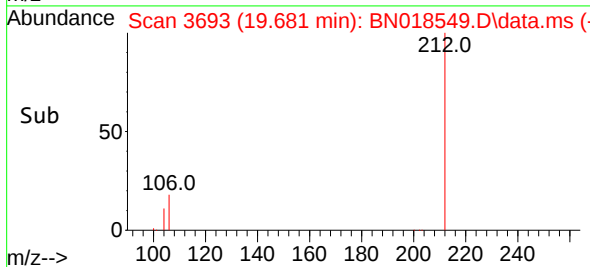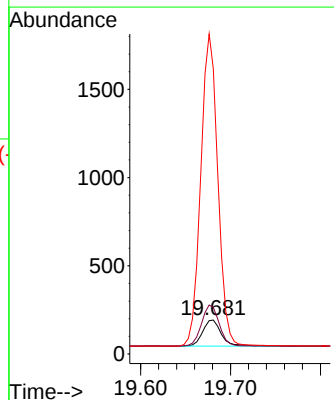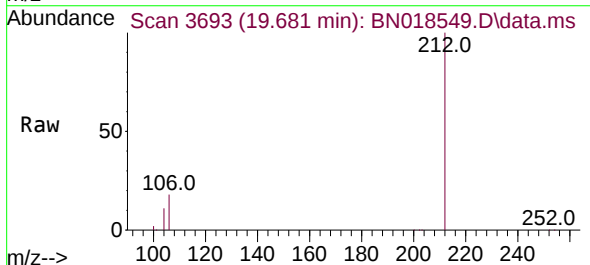

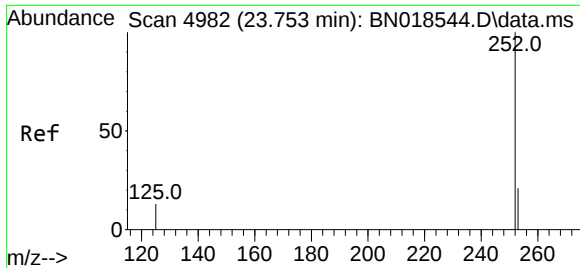

#26

Benzo(a)pyrene

Concen: 0.105 ng/ul

RT: 23.709 min Scan# 49

Delta R.T. -0.044 min

Lab File: BN018549.D


Acq: 02 Feb 2022 14:53

Instrument :

BNA_N

ClientSampleId :

SBLK347

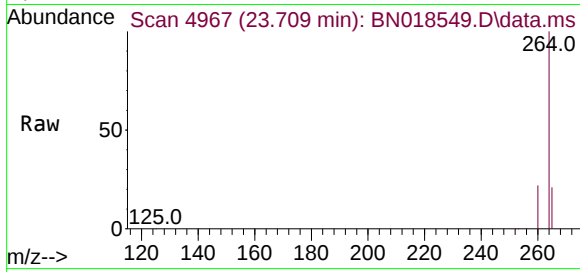

Tgt Ion:252 Resp: 491

Ion Ratio Lower Upper

252 100

253 48.1 18.9 28.3#

125 39.3 8.2 12.2#

