

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
 Data File : BN018550.D
 Acq On : 02 Feb 2022 15:28
 Operator : CG/JU
 Sample : PB142349BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK349

Quant Time: Feb 02 17:15:55 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 02 14:08:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	401	0.400	ng/ul	0.00
4) Naphthalene-d8	10.733	136	1437	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.558	164	807	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.294	188	1543	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.465	240	1171	0.400	ng/ul	# 0.00
23) Perylene-d12	23.859	264	1264	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.295	96	2818	6.120	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.323	152	694	0.354	ng/ul	0.00
18) Fluoranthene-d10	19.314	212	1453	0.434	ng/ul	0.00
Target Compounds						
					Qvalue	
14) Pentachlorophenol	16.948	266	27	0.094	ng/ul	96
20) Pyrene	19.681	202	214	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.707	252	499	0.111	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
Data File : BN018550.D
Acq On : 02 Feb 2022 15:28
Operator : CG/JU
Sample : PB142349BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK349


Quant Time: Feb 02 17:15:55 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:08:46 2022
Response via : Initial Calibration

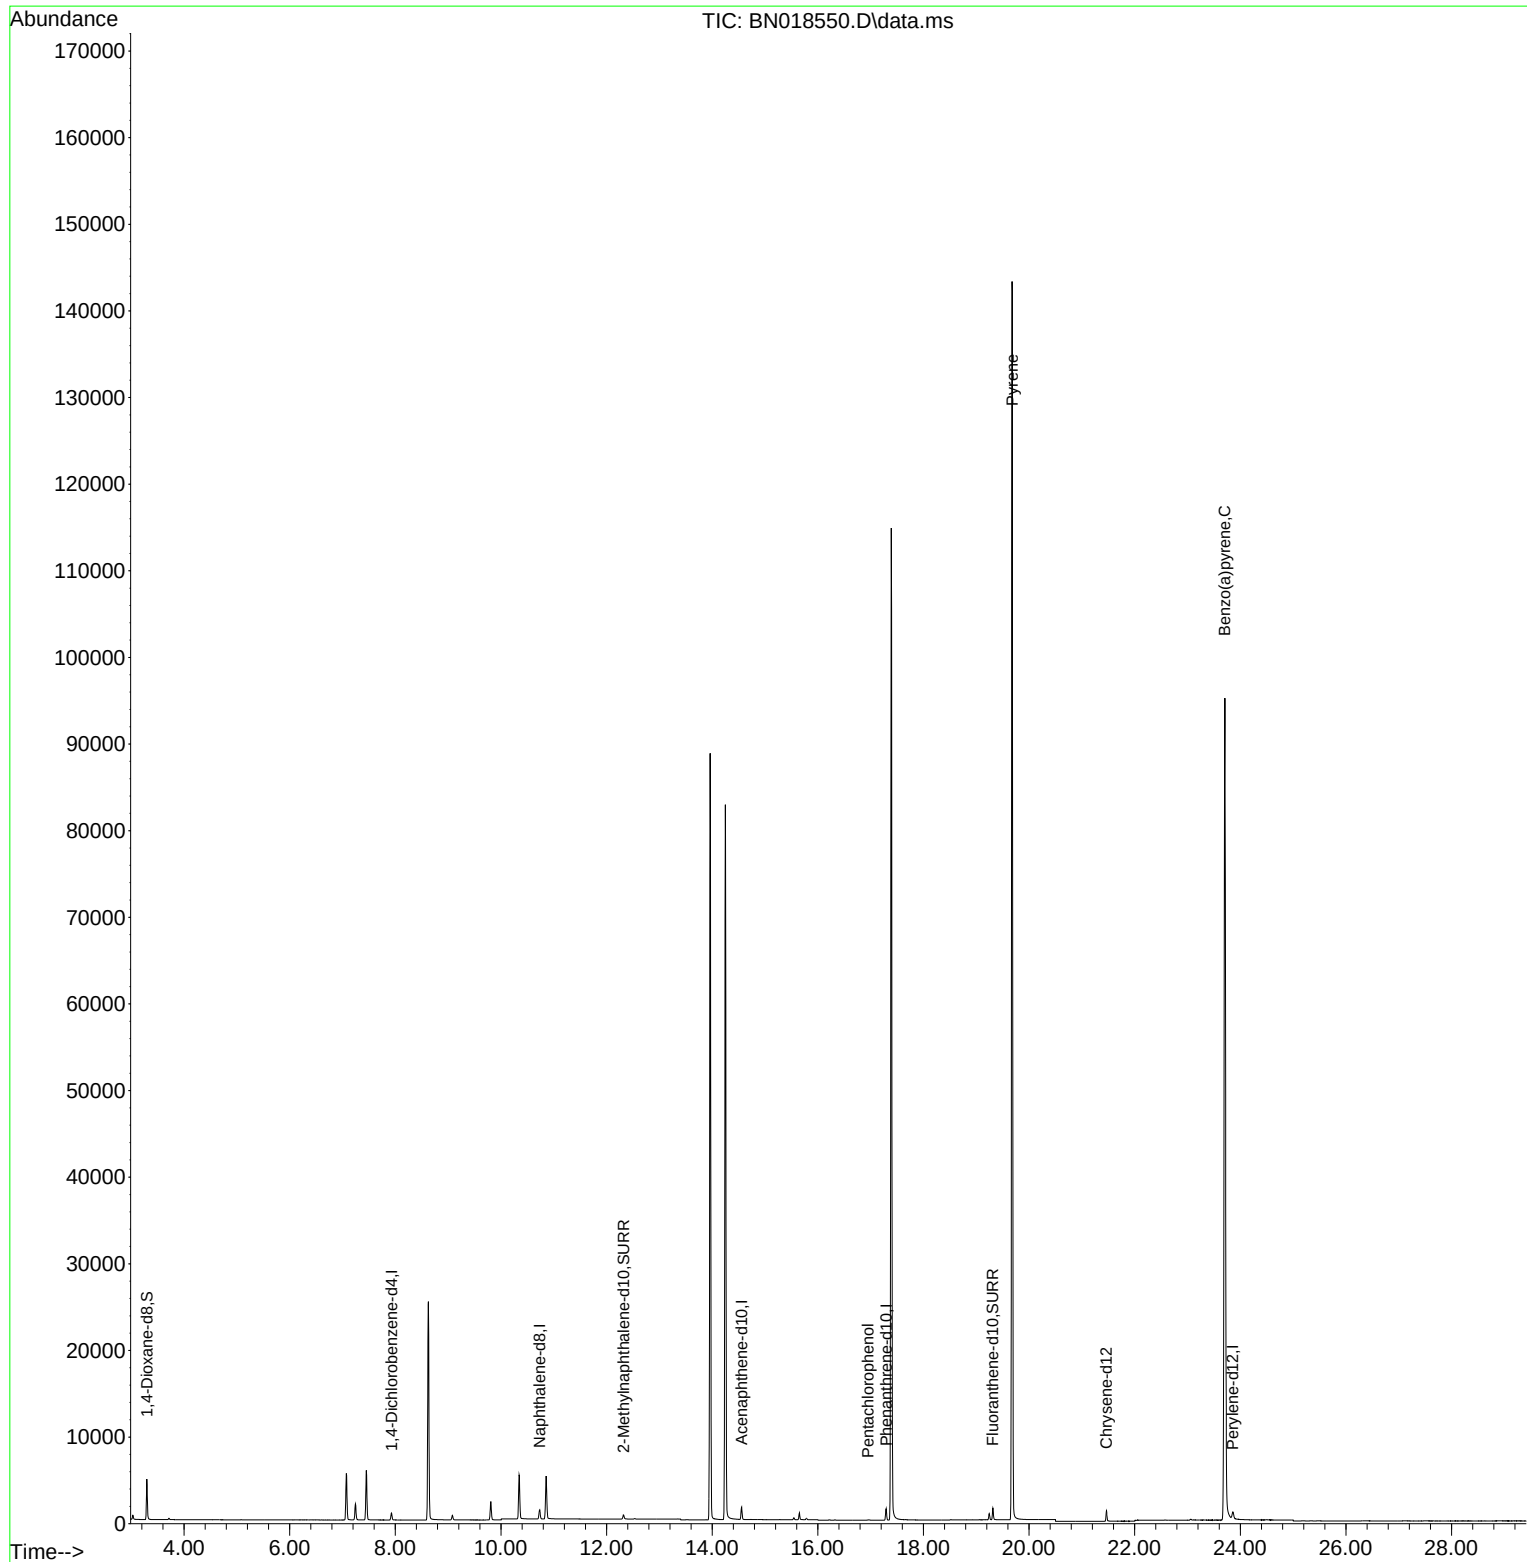



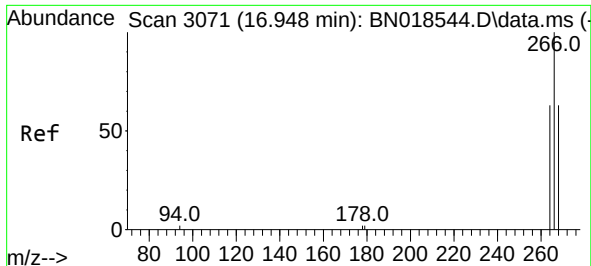


#14
 Pentachlorophenol
 Concen: 0.094 ng/ul
 RT: 16.948 min Scan# 3071
 Delta R.T. -0.000 min
 Lab File: BN018550.D
 Acq: 02 Feb 2022 15:28

Instrument :
 BNA_N
 ClientSampleId :
 SBLK349



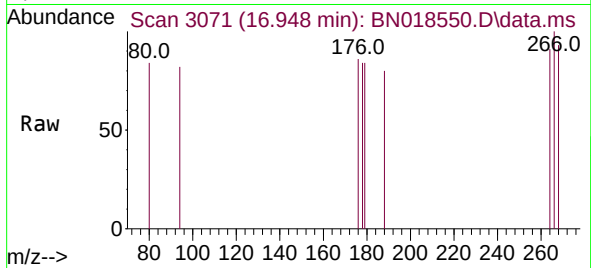



Tgt Ion:266 Resp: 27
 Ion Ratio Lower Upper
 266 100
 264 66.7 49.9 74.9
 268 66.7 51.7 77.5

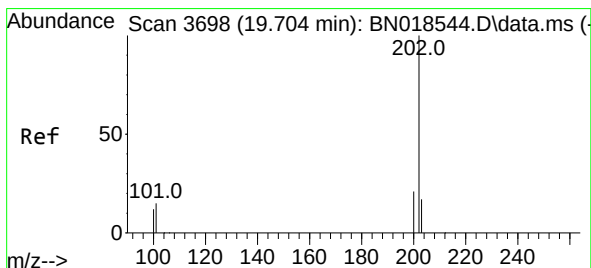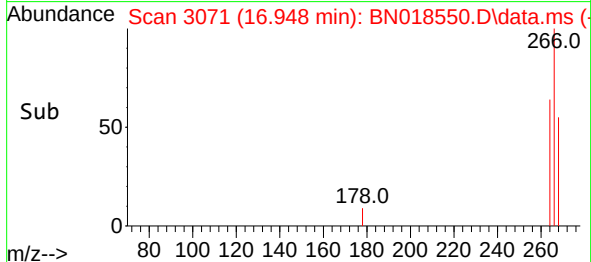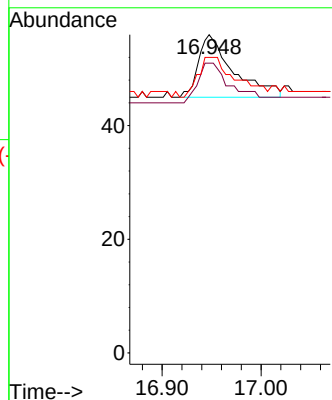

#20
 Pyrene
 Concen: 0.045 ng/ul
 RT: 19.681 min Scan# 3693
 Delta R.T. -0.023 min
 Lab File: BN018550.D
 Acq: 02 Feb 2022 15:28

Tgt Ion:202 Resp: 214
 Ion Ratio Lower Upper
 202 100
 101 136.1 9.0 13.4#
 100 835.6 7.0 10.4#

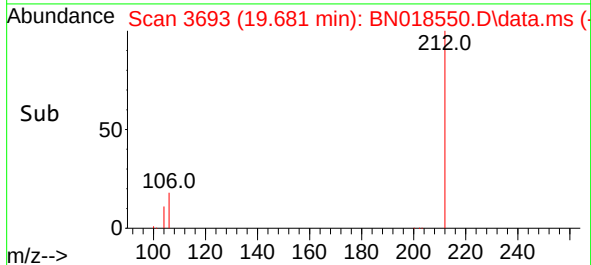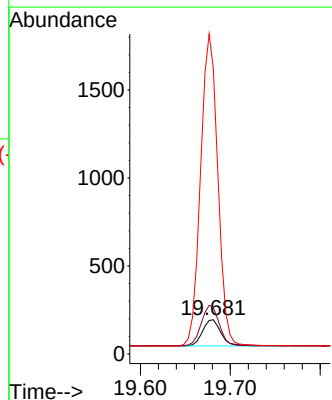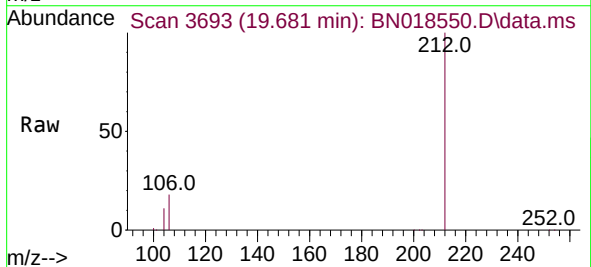

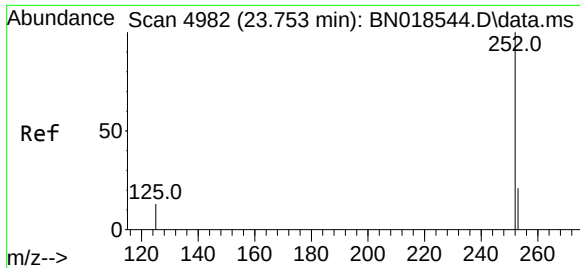

#26

Benzo(a)pyrene

Concen: 0.111 ng/ul

RT: 23.707 min Scan# 4966

Delta R.T. -0.047 min

Lab File: BN018550.D


Acq: 02 Feb 2022 15:28

Instrument :

BNA_N

ClientSampleId :

SBLK349

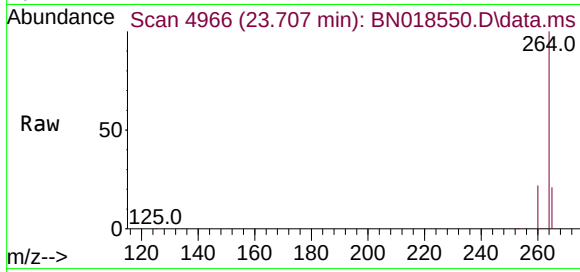

Tgt Ion:252 Resp: 499

Ion Ratio Lower Upper

252 100

253 48.8 18.9 28.3#

125 38.9 8.2 12.2#

