




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
Data File : BN018564.D
Acq On : 03 Feb 2022 00:21
Operator : CG/JU
Sample : N1307-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0Q11

Manual IntegrationsAPPROVED

Quant Time: Feb 03 03:35:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:08:46 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2022
Supervised By :mohammad ahmed 02/04/2022

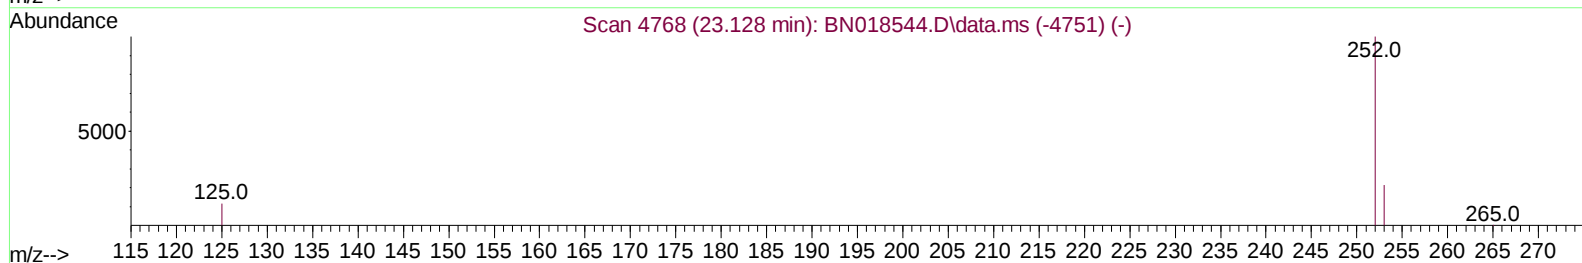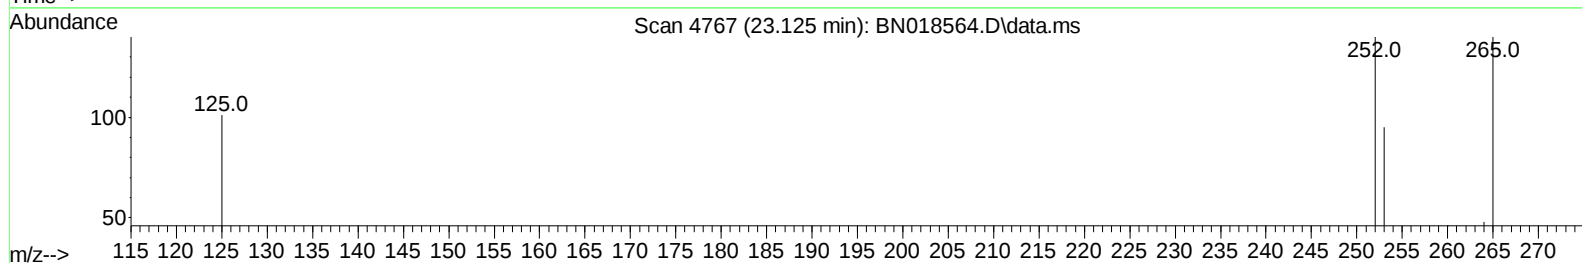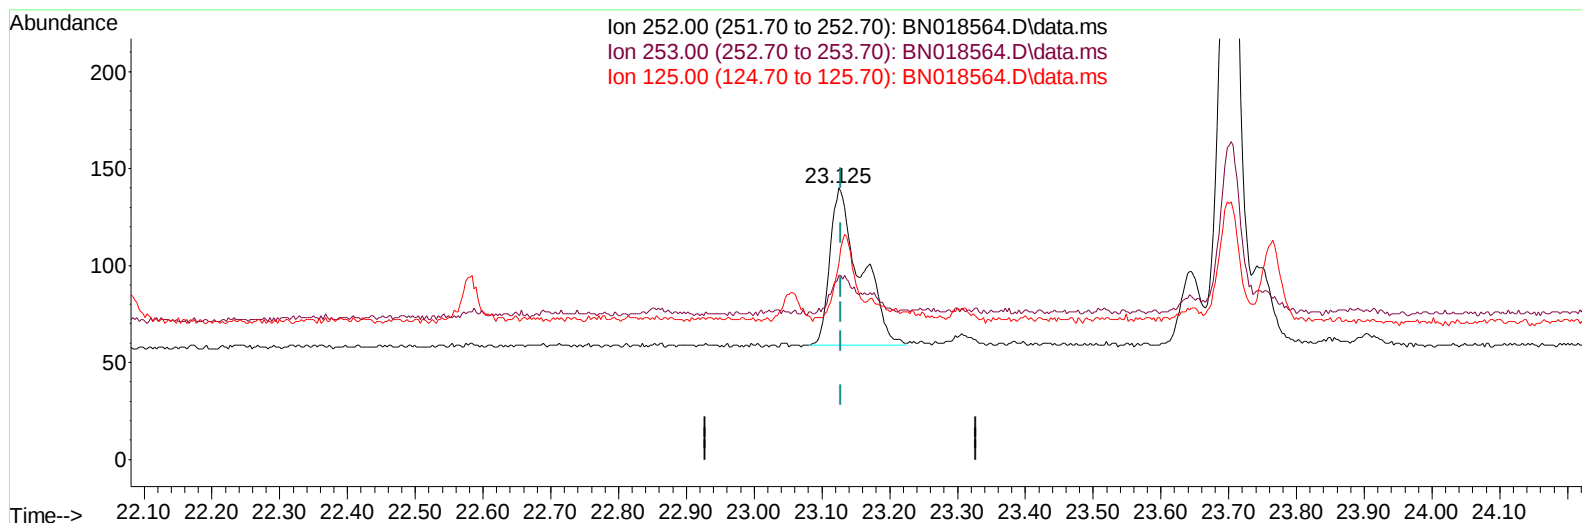

TIC: BN018564.D\data.ms

(24) Benzo(b)fluoranthene

23.125min (-0.003) 0.04 ng/u1

response 255

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.20	67.86#
125.00	8.90	72.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
Data File : BN018564.D
Acq On : 03 Feb 2022 00:21
Operator : CG/JU
Sample : N1307-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0Q11

Manual IntegrationsAPPROVED

Quant Time: Feb 03 03:35:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:08:46 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2022
Supervised By :mohammad ahmed 02/04/2022

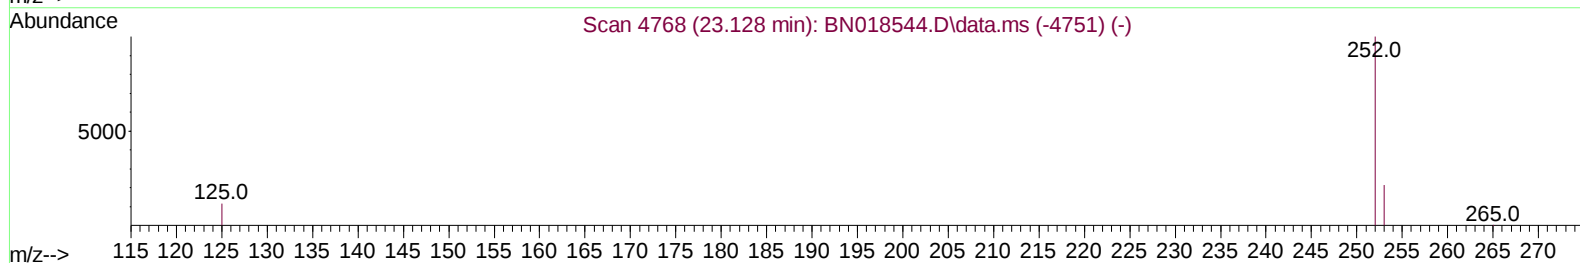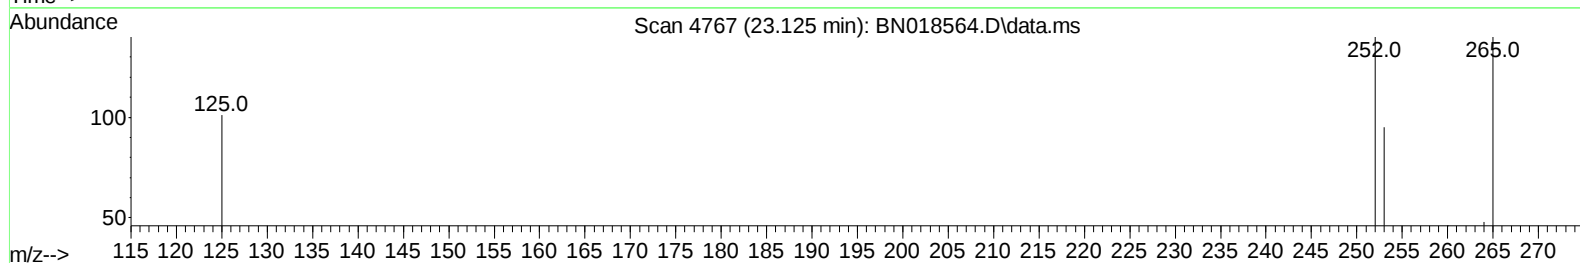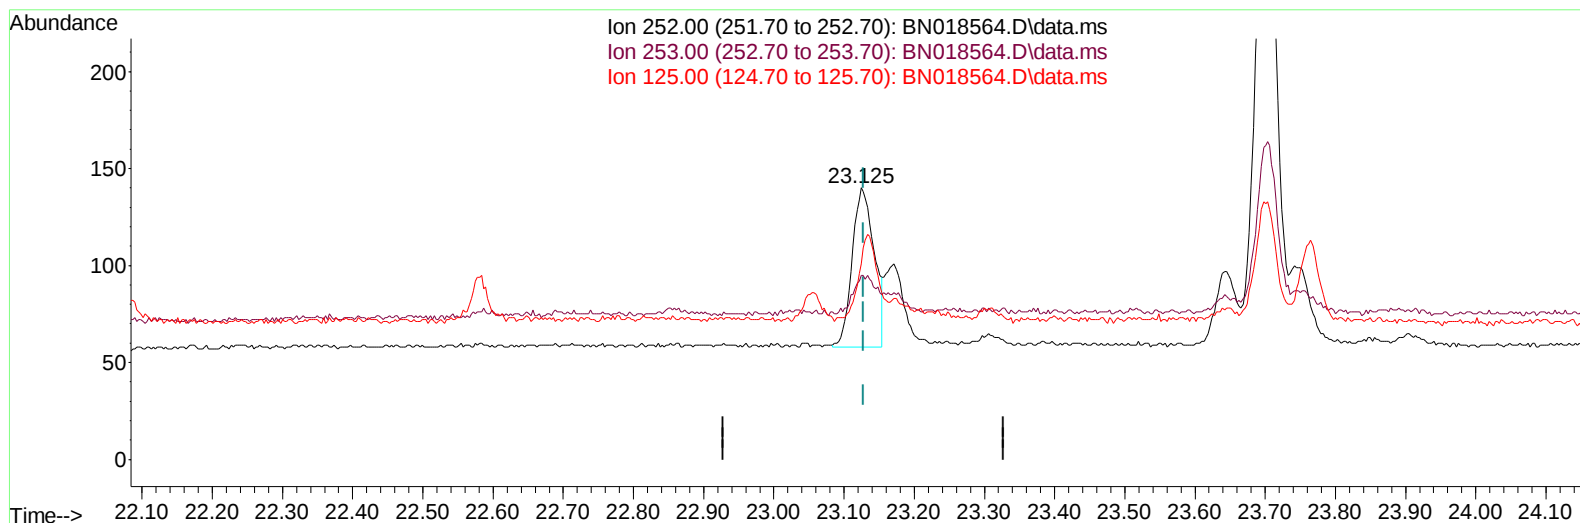

TIC: BN018564.D\data.ms

(24) Benzo(b)fluoranthene

23.125min (-0.003) 0.03 ng/u1 m

response 180

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	23.20	67.86#
125.00	8.90	72.14#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
 Data File : BN018564.D
 Acq On : 03 Feb 2022 00:21
 Operator : CG/JU
 Sample : N1307-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0Q11

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/03/2022
 Supervised By :mohammad ahmed 02/04/2022

Quant Time: Feb 03 03:35:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 02 14:08:46 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.927	152		431	0.400	ng/ul	0.00
4) Naphthalene-d8	10.728	136		1538	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.553	164		879	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.289	188		1702	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.461	240		1441	0.400	ng/ul	# 0.00
23) Perylene-d12	23.855	264		1506	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.294	96		2088	4.219	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.317	152		792	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.314	212		1923	0.467	ng/ul	0.00
Target Compounds							Qvalue
14) Pentachlorophenol	16.943	266		121	0.381	ng/ul	96
19) Fluoranthene	19.342	202		155	0.027	ng/ul#	18
24) Benzo(b)fluoranthene	23.125	252		180m	0.027	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
Data File : BN018564.D
Acq On : 03 Feb 2022 00:21
Operator : CG/JU
Sample : N1307-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0Q11

Manual IntegrationsAPPROVED

Quant Time: Feb 03 03:35:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:08:46 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2022
Supervised By :mohammad ahmed 02/04/2022

