

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
 Data File : BN018559.D
 Acq On : 02 Feb 2022 21:24
 Operator : CG/JU
 Sample : N1307-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0Q00

Quant Time: Feb 03 03:33:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 02 14:08:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	443	0.400	ng/ul	0.00
4) Naphthalene-d8	10.728	136	1601	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.553	164	944	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.289	188	1904	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.462	240	1578	0.400	ng/ul	# 0.00
23) Perylene-d12	23.859	264	1528	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.295	96	2094	4.117	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.317	152	712	0.326	ng/ul	0.00
18) Fluoranthene-d10	19.314	212	1804	0.400	ng/ul	0.00
Target Compounds				Qvalue		
12) Fluorene	15.599	166	799	0.224	ng/ul#	96
14) Pentachlorophenol	16.943	266	32091	90.410	ng/ul	99
19) Fluoranthene	19.342	202	269	0.043	ng/ul#	34
20) Pyrene	19.704	202	608	0.094	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
Data File : BN018559.D
Acq On : 02 Feb 2022 21:24
Operator : CG/JU
Sample : N1307-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0Q00

Quant Time: Feb 03 03:33:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:08:46 2022
Response via : Initial Calibration




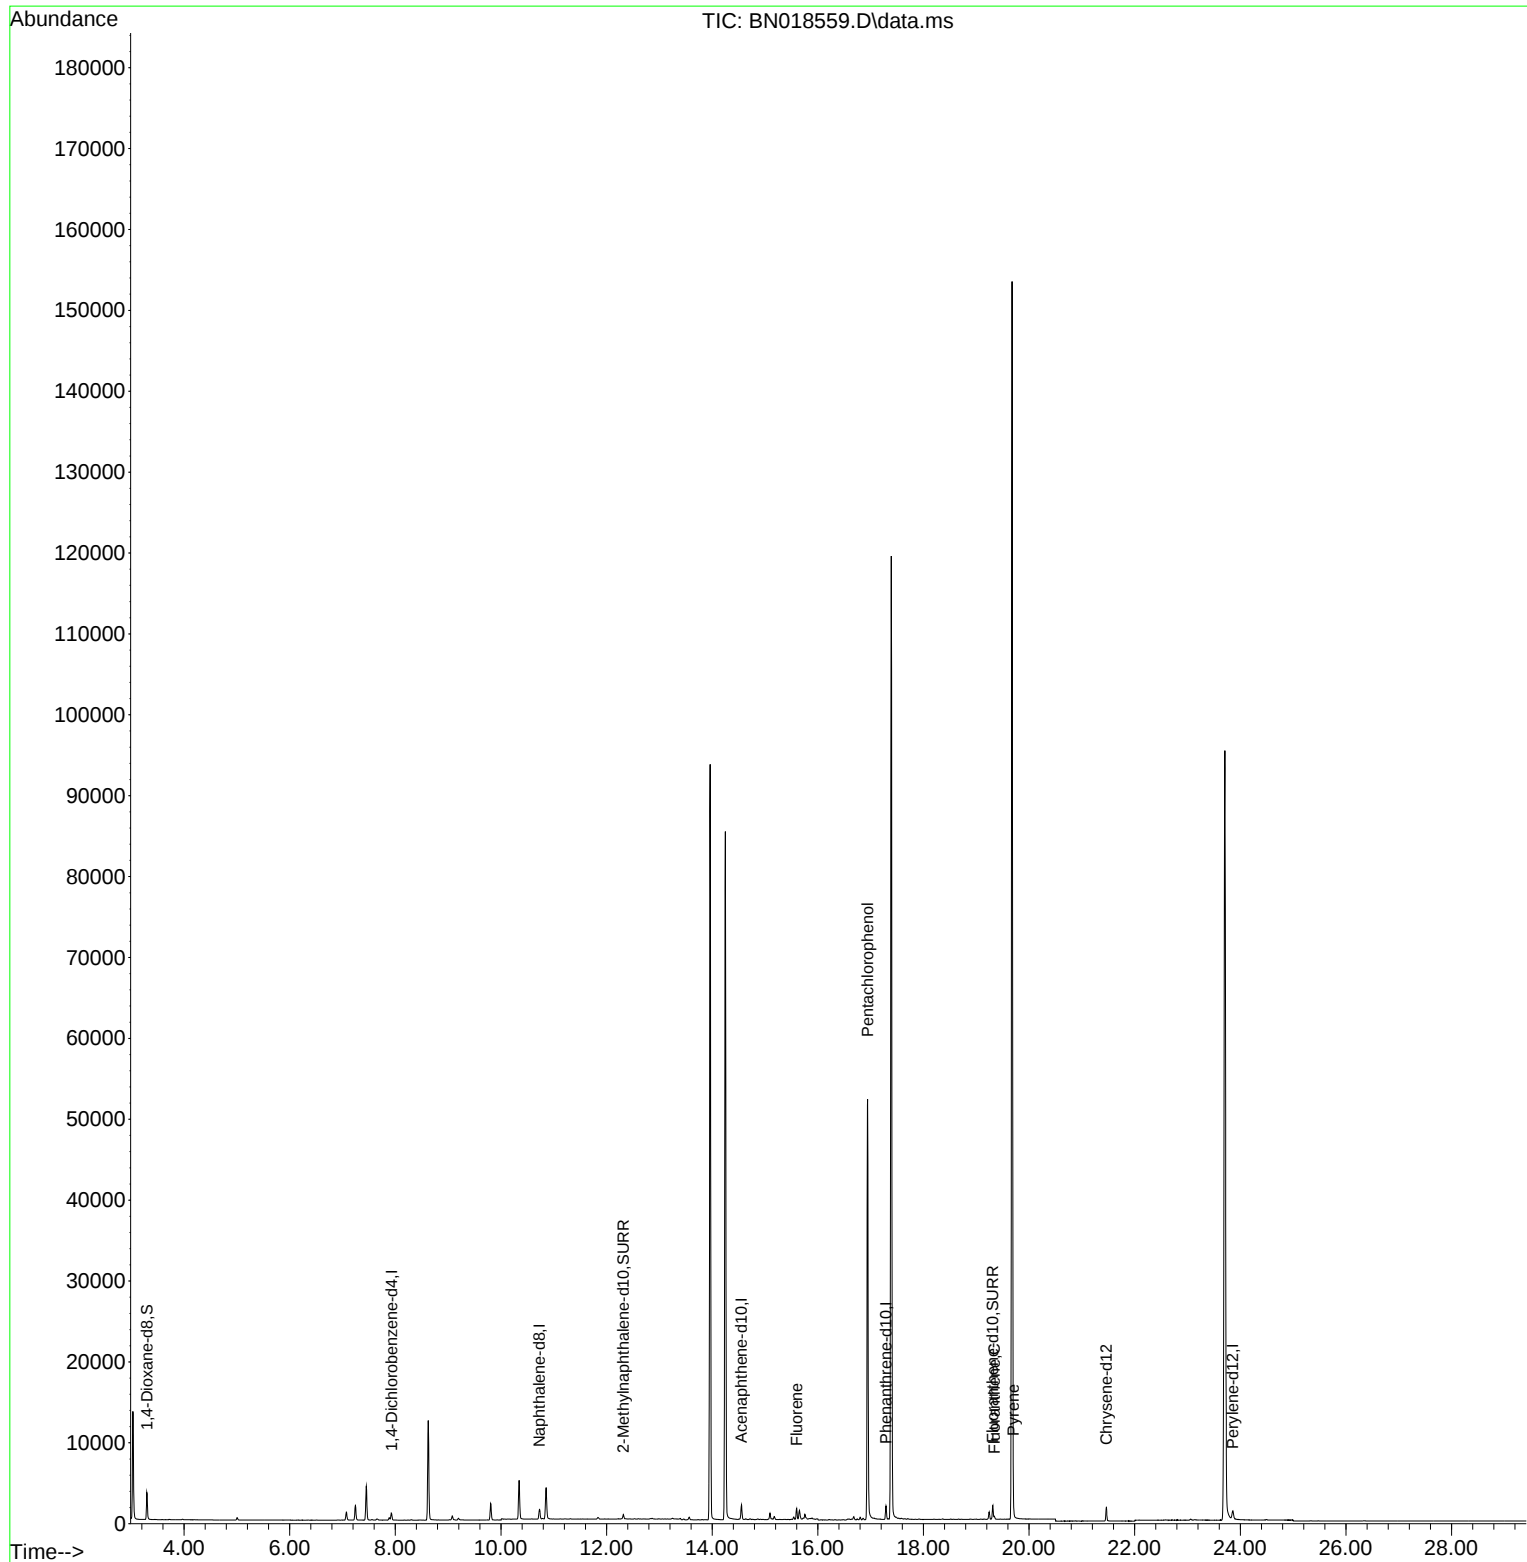


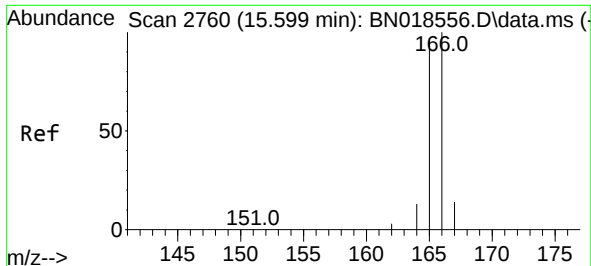

#12
Fluorene
Concen: 0.224 ng/ul
RT: 15.599 min Scan# 21
Delta R.T. -0.005 min
Lab File: BN018559.D
Acq: 02 Feb 2022 21:24




Instrument :
BNA_N
ClientSampleId :
C0Q00


Tgt Ion:166 Resp: 799
Ion Ratio Lower Upper
166 100
165 98.9 77.8 116.6
167 21.7 11.6 17.4#

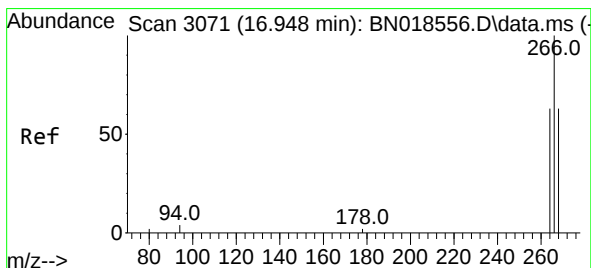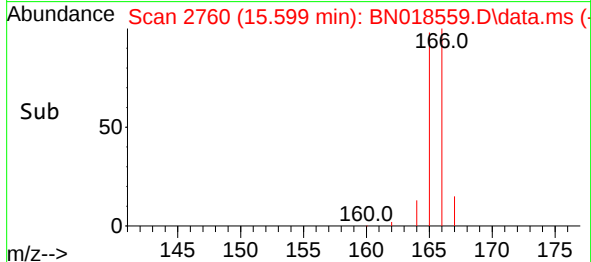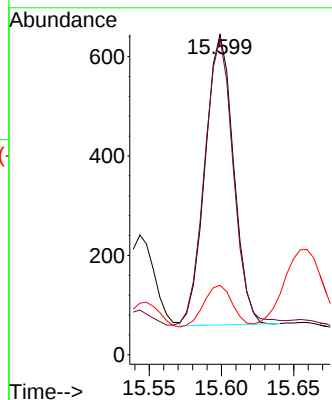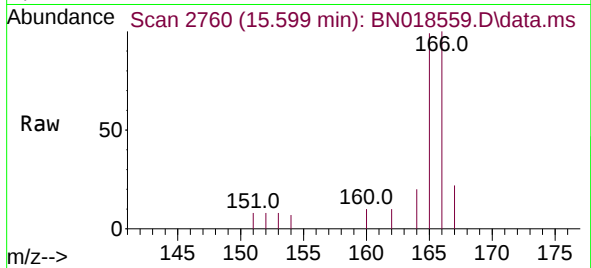

#14
Pentachlorophenol
Concen: 90.410 ng/ul
RT: 16.943 min Scan# 3070
Delta R.T. -0.004 min
Lab File: BN018559.D
Acq: 02 Feb 2022 21:24

Tgt Ion:266 Resp: 32091
Ion Ratio Lower Upper
266 100
264 62.8 49.9 74.9
268 63.7 51.7 77.5


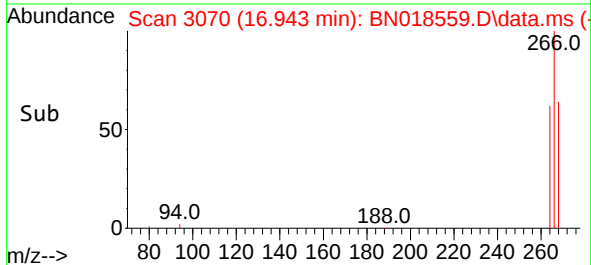
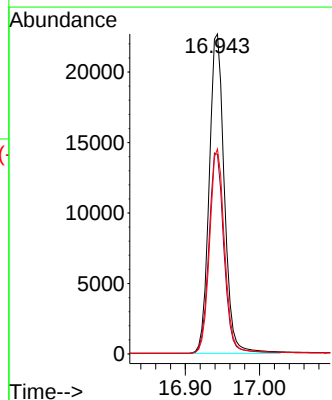
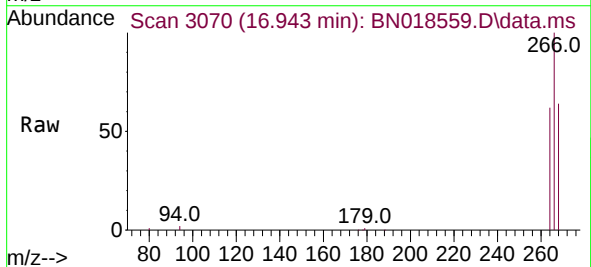


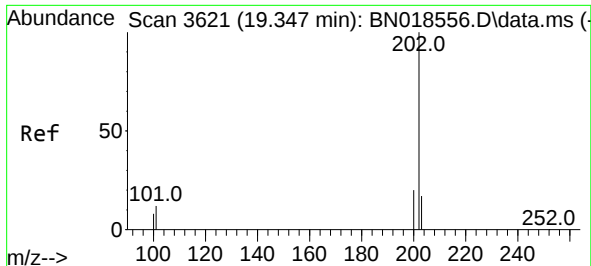

#19
Fluoranthene
Concen: 0.043 ng/ul
RT: 19.342 min Scan# 3620
Delta R.T. -0.005 min
Lab File: BN018559.D
Acq: 02 Feb 2022 21:24

Instrument :
BNA_N
ClientSampleId :
C0Q00

Tgt Ion:202 Resp: 269
Ion Ratio Lower Upper
202 100
101 34.0 7.5 11.3#
100 28.9 5.4 8.2#

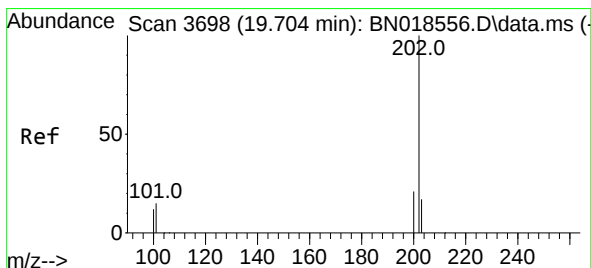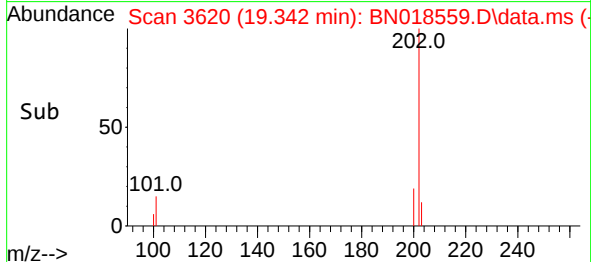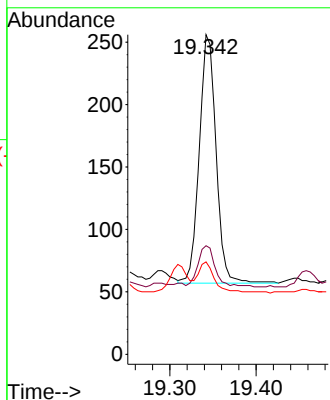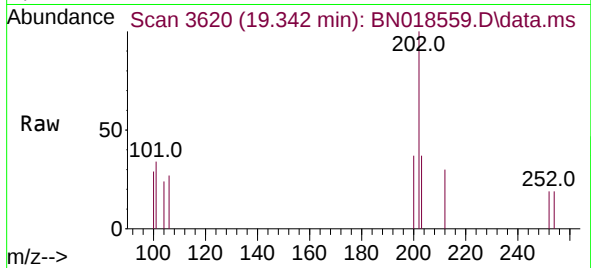

#20
Pyrene
Concen: 0.094 ng/ul
RT: 19.704 min Scan# 3698
Delta R.T. -0.000 min
Lab File: BN018559.D
Acq: 02 Feb 2022 21:24

Tgt Ion:202 Resp: 608
Ion Ratio Lower Upper
202 100
101 23.2 9.0 13.4#
100 22.2 7.0 10.4#

