

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
 Data File : BN018562.D
 Acq On : 02 Feb 2022 23:10
 Operator : CG/JU
 Sample : N1307-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0Q33

Quant Time: Feb 03 03:34:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 02 14:08:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.923	152	428	0.400	ng/ul	0.00
4) Naphthalene-d8	10.728	136	1554	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.553	164	904	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.289	188	1789	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.462	240	1451	0.400	ng/ul	# 0.00
23) Perylene-d12	23.856	264	1481	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	2194	4.465	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.317	152	783	0.370	ng/ul	0.00
18) Fluoranthene-d10	19.314	212	1822	0.439	ng/ul	0.00
Target Compounds					Qvalue	
14) Pentachlorophenol	16.939	266	714	2.141	ng/ul	99
15) Phenanthrene	17.332	178	118	0.020	ng/ul#	29


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
Data File : BN018562.D
Acq On : 02 Feb 2022 23:10
Operator : CG/JU
Sample : N1307-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0Q33

Quant Time: Feb 03 03:34:38 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:08:46 2022
Response via : Initial Calibration




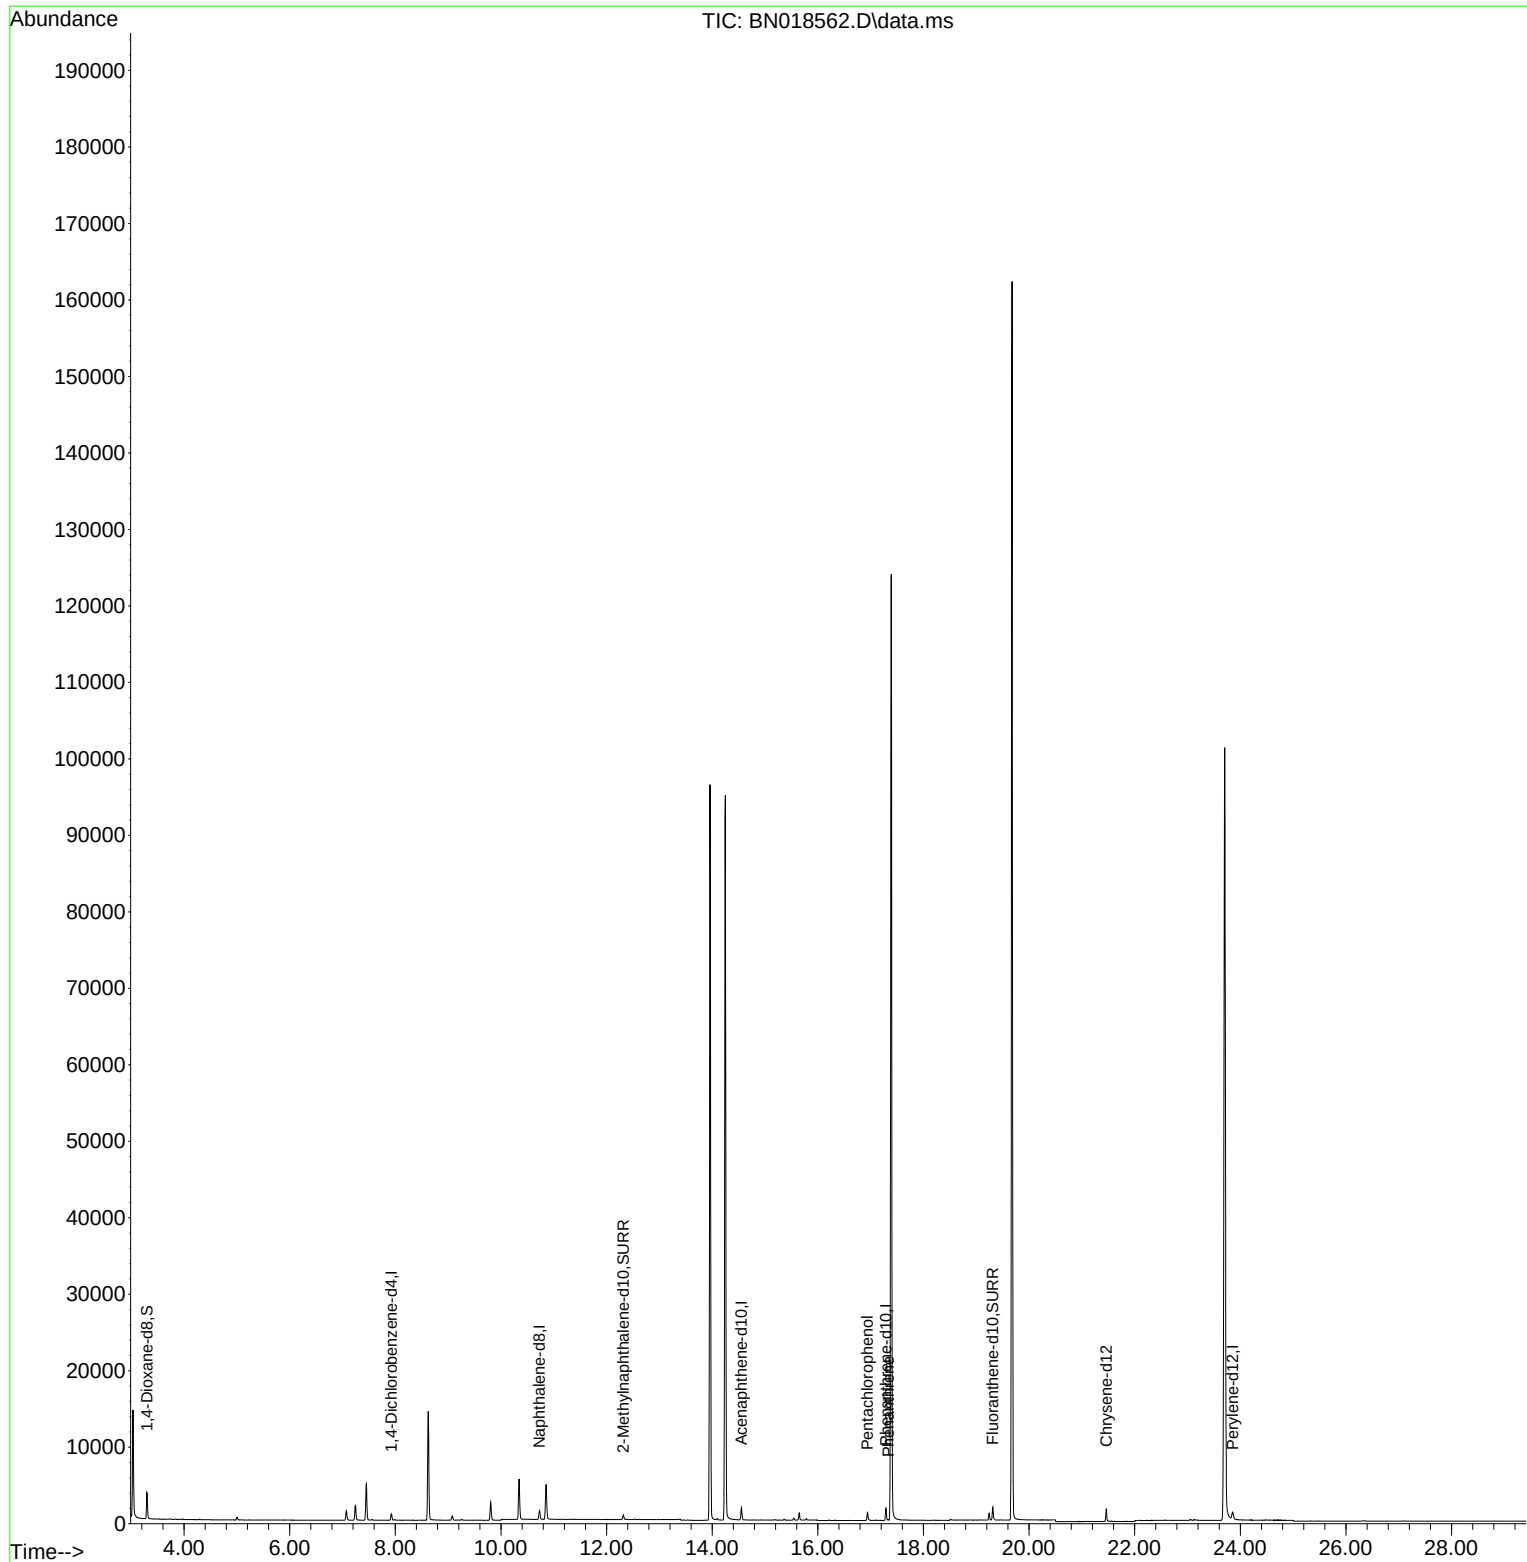


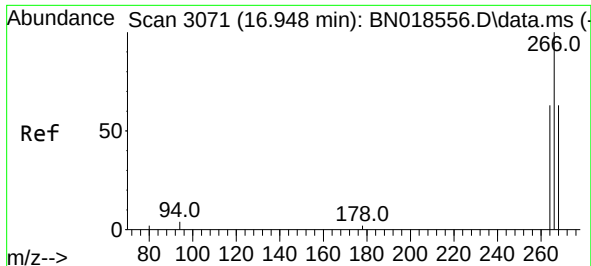

#14
 Pentachlorophenol
 Concen: 2.141 ng/uI
 RT: 16.939 min Scan# 3071
 Delta R.T. -0.009 min
 Lab File: BN018562.D
 Acq: 02 Feb 2022 23:10

Instrument :
 BNA_N
 ClientSampleId :
 C0Q33

Tgt Ion:266 Resp: 714
 Ion Ratio Lower Upper
 266 100
 264 62.9 49.9 74.9
 268 63.3 51.7 77.5

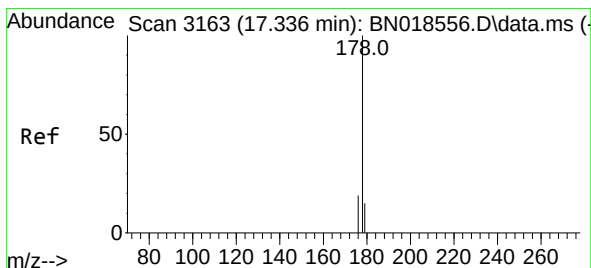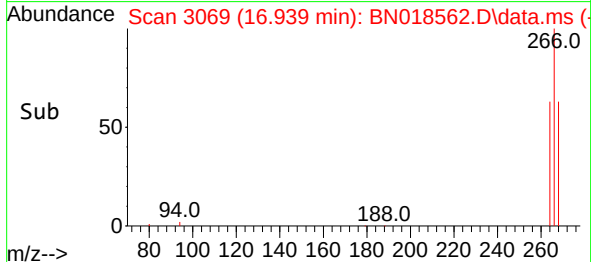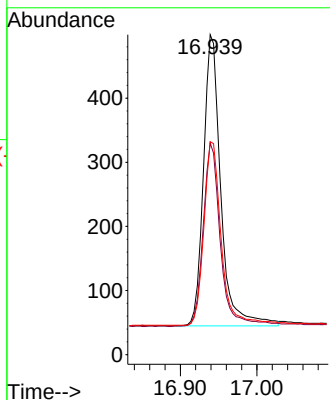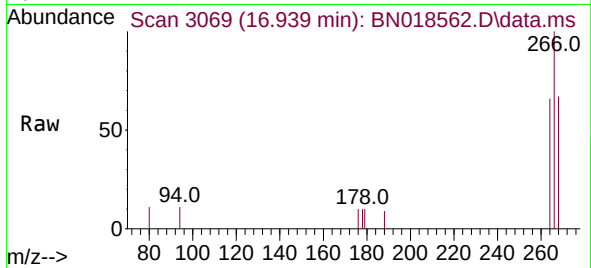

#15
 Phenanthrene
 Concen: 0.020 ng/uI
 RT: 17.332 min Scan# 3162
 Delta R.T. -0.004 min
 Lab File: BN018562.D
 Acq: 02 Feb 2022 23:10

Tgt Ion:178 Resp: 118
 Ion Ratio Lower Upper
 178 100
 179 47.7 12.2 18.4#
 176 49.2 15.4 23.2#

