

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
 Data File : BN018565.D
 Acq On : 03 Feb 2022 00:56
 Operator : CG/JU
 Sample : N1307-11
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0Q34

Quant Time: Feb 03 03:35:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 02 14:08:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	417	0.400	ng/ul	0.00
4) Naphthalene-d8	10.728	136	1547	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.553	164	895	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.289	188	1795	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.462	240	1450	0.400	ng/ul	# 0.00
23) Perylene-d12	23.853	264	1491	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.295	96	1915	4.000	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.317	152	766	0.363	ng/ul	0.00
18) Fluoranthene-d10	19.314	212	1840	0.444	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.943	266	600	1.793	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020222\
Data File : BN018565.D
Acq On : 03 Feb 2022 00:56
Operator : CG/JU
Sample : N1307-11
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0Q34

Quant Time: Feb 03 03:35:27 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:08:46 2022
Response via : Initial Calibration

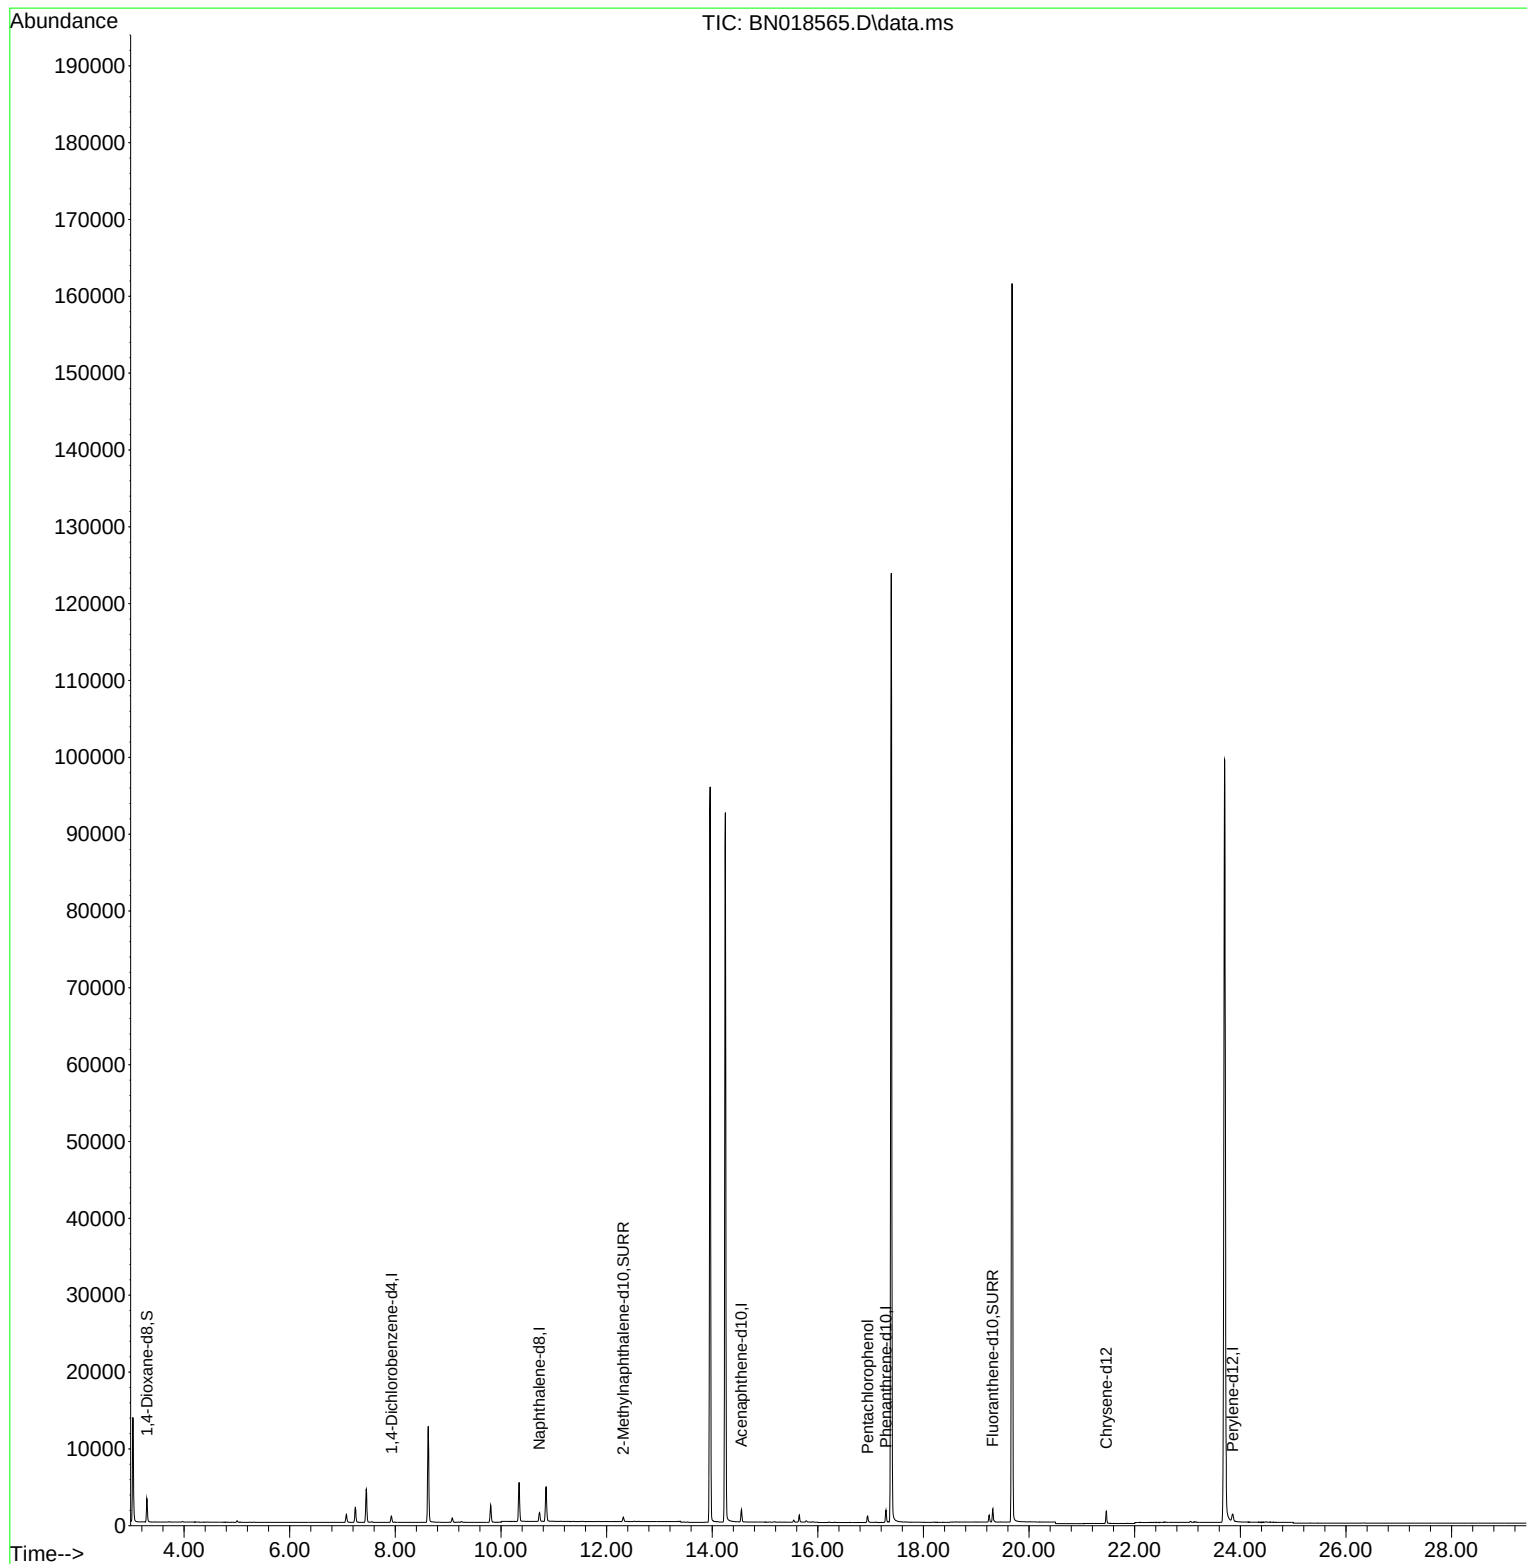

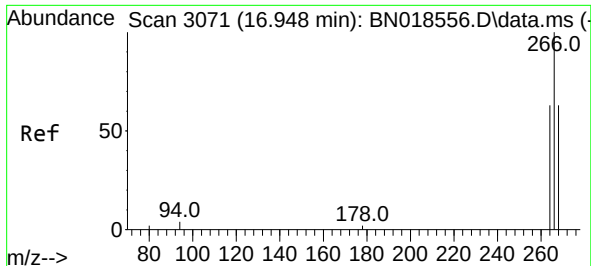

#14

Pentachlorophenol

Concen: 1.793 ng/ul

RT: 16.943 min Scan# 3070

Delta R.T. -0.004 min

Lab File: BN018565.D


Acq: 03 Feb 2022 00:56

Instrument :

BNA_N

ClientSampleId :

C0Q34

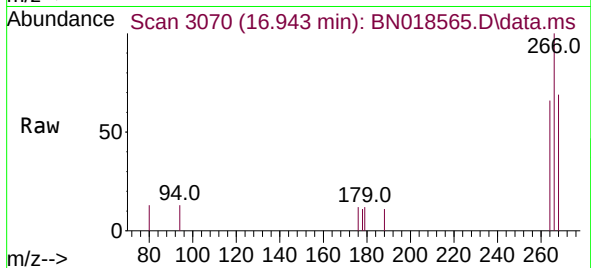

Tgt Ion:266 Resp: 600

Ion Ratio Lower Upper

266 100

264 63.5 49.9 74.9

268 63.2 51.7 77.5

