


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020224\
Data File : BN029492.D
Acq On : 02 Feb 2024 08:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 01:51:59 2024

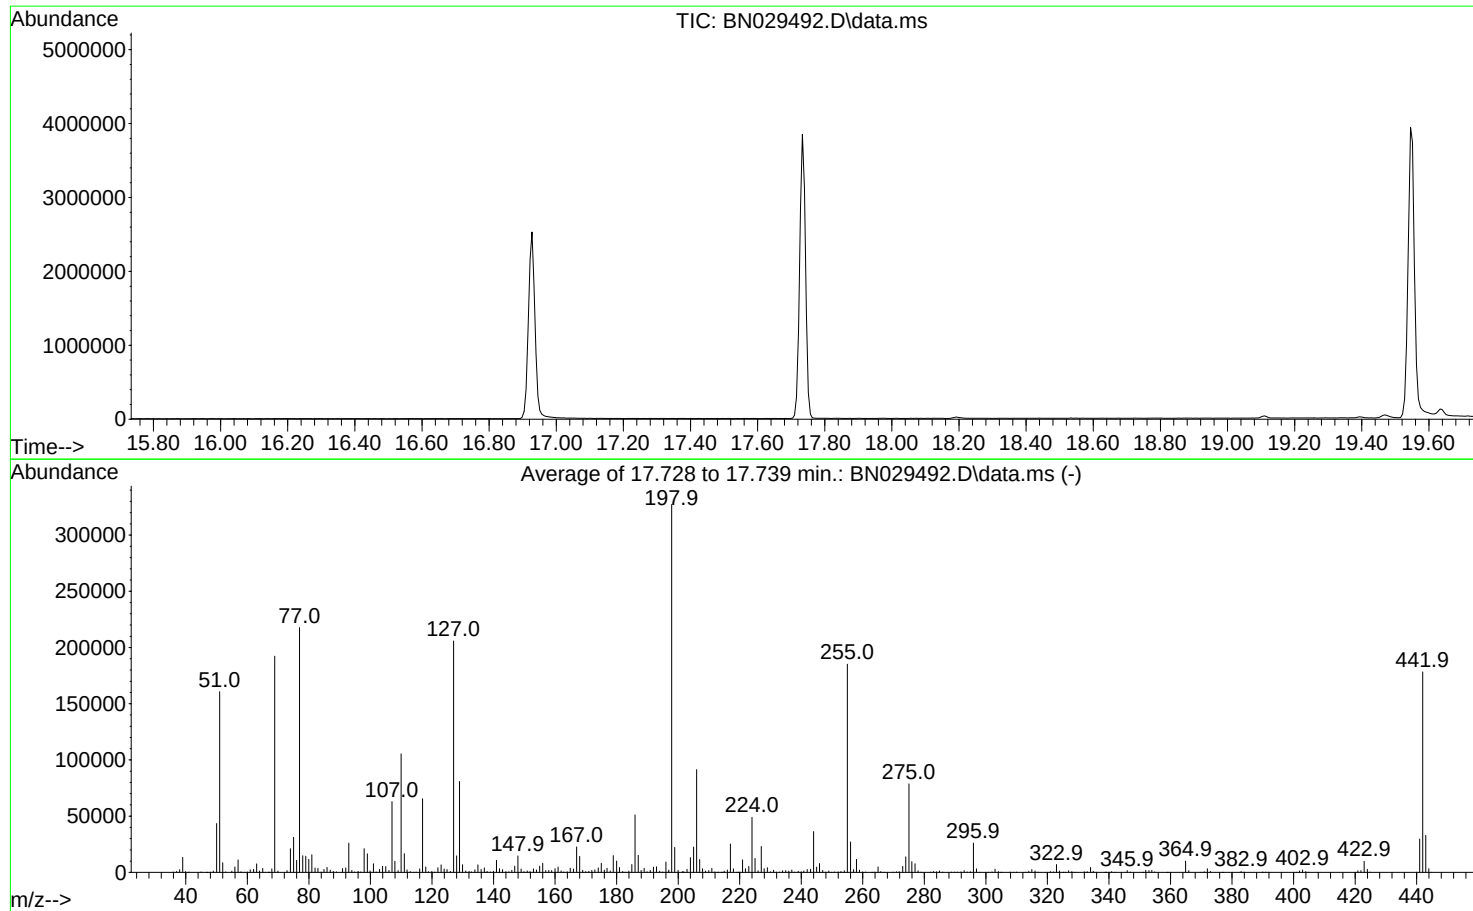




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	160667	PASS
68	69	0.00	2	1.6	3156	PASS
69	198	0.00	100	58.7	192235	PASS
70	69	0.00	2	0.6	1108	PASS
127	198	10	80	62.9	205760	PASS
197	198	0.00	2	0.6	1976	PASS
198	198	100	100	100.0	327211	PASS
199	198	5	9	6.8	22195	PASS
275	198	10	60	24.1	78704	PASS
365	198	1	100	3.1	9986	PASS
441	198	0.01	100	9.1	29656	PASS
442	442	50	100	100.0	178339	PASS
443	442	15	24	18.5	32941	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020224\
Data File : BN029492.D
Acq On : 02 Feb 2024 08:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 03 03:38:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 03:38:30 2024
Response via : Initial Calibration

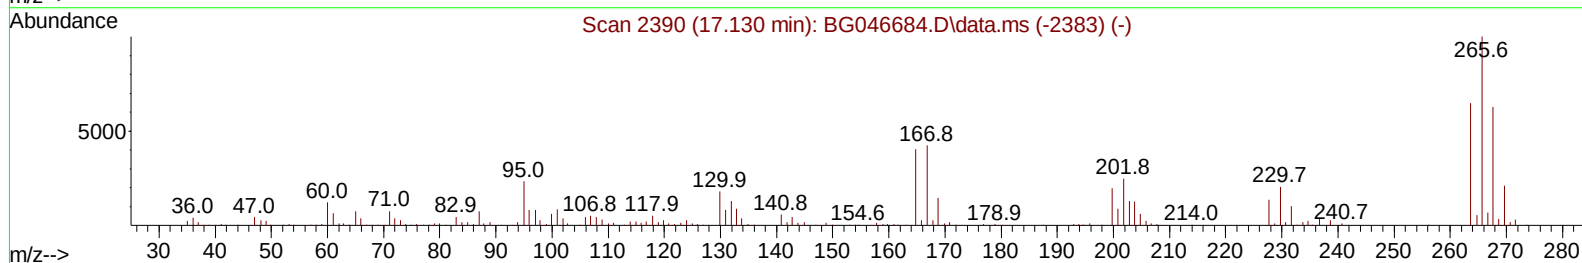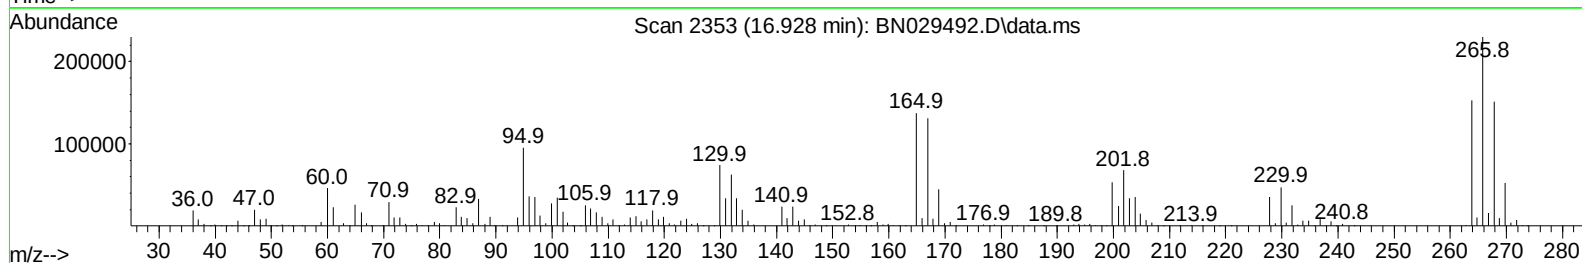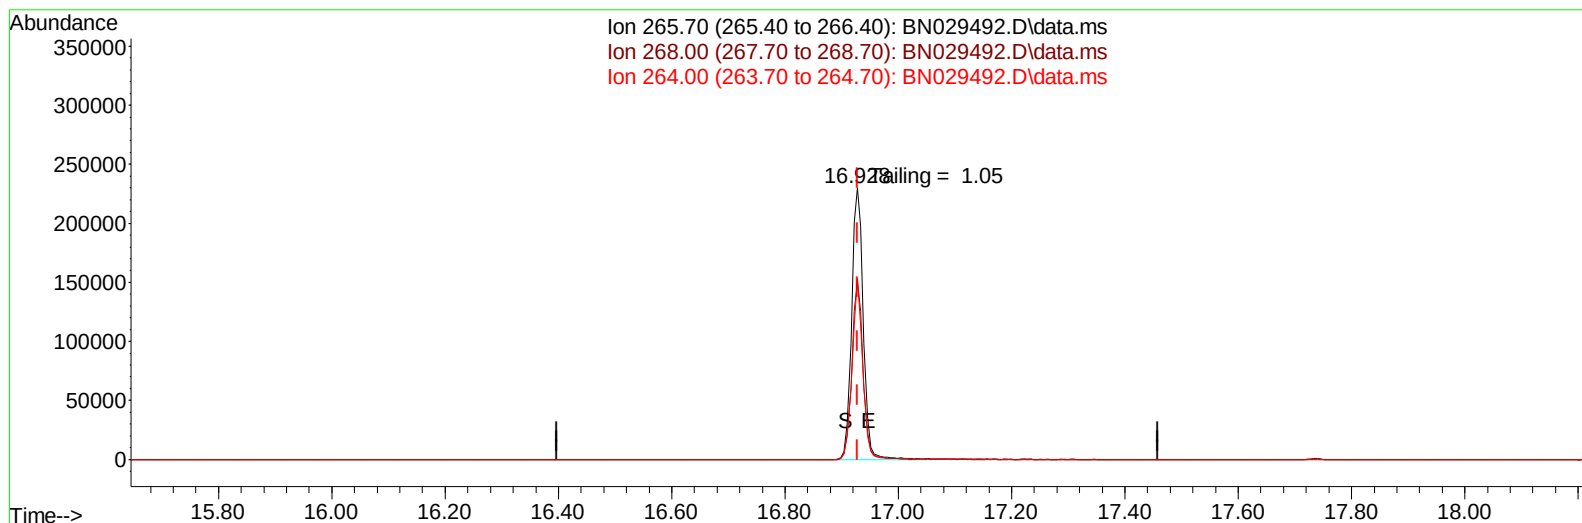

TIC: BN029492.D\data.ms

(70) Pentachlorophenol (C)

16.928min (0.000) 16738.55 ng




response 329582

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.79
264.00	61.60	66.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020224\
Data File : BN029492.D
Acq On : 02 Feb 2024 08:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 03 03:38:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 03:38:30 2024
Response via : Initial Calibration

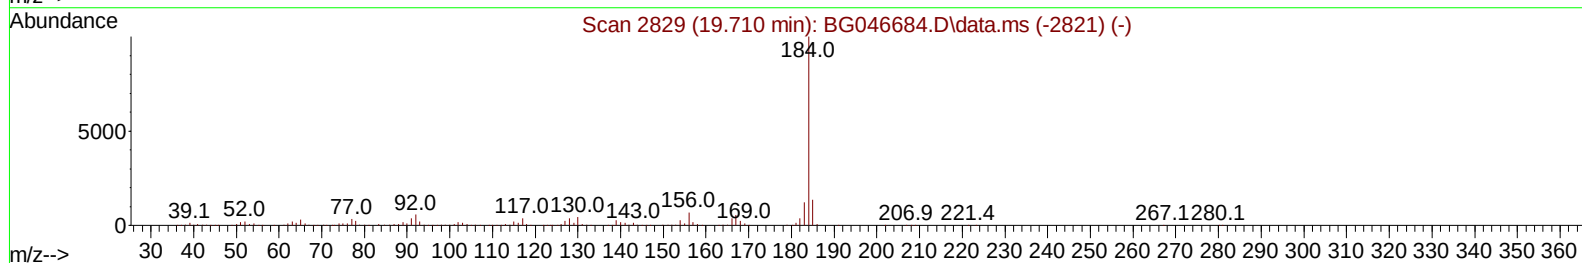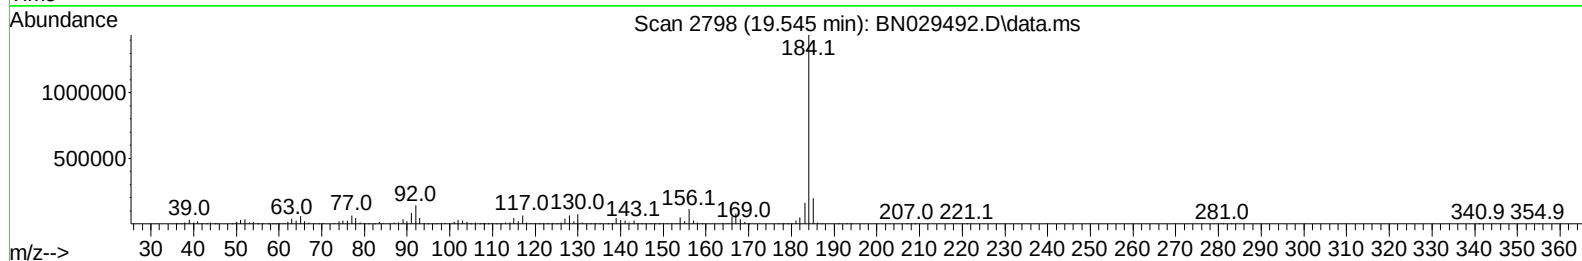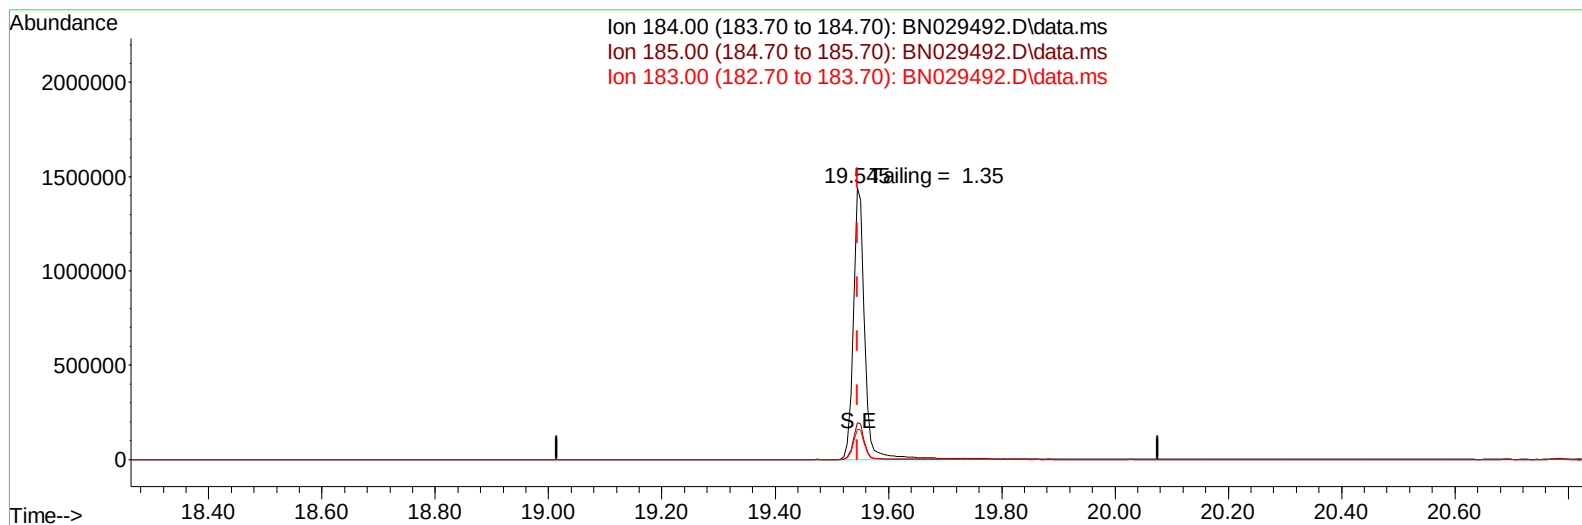

TIC: BN029492.D\data.ms

(77) Benzidine

19.545min (0.000) 0.00 ng

response 2008043

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.52
183.00	13.20	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/2/2024	BNA_N	<u>BN029492.D</u>
Compound Name	Response	Retention Time
DDT	977035	20.786
DDD	10062	20.392
DDE	117	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10179	987214	1.03

Instrument :
BNA_N
ClientSampleId :
DFTPP