

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
 Data File : BN009536.D
 Acq On : 03 Feb 2020 19:12
 Operator : CG/JU
 Sample : L1342-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Feb 04 00:21:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 16:39:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	130133	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	540211	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.08	164	349897	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.83	188	753232	20.00	ng/ul	0.00
77) Chrysene-d12	21.04	240	697558	20.00	ng/ul	0.00
85) Perylene-d12	23.16	264	762797	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	9003	2.84	ng/uL	0.00
5) Phenol-d5	6.64	99	155371	13.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	124215	16.29	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	123475	14.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	125317	13.86	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	64047	15.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	65596	14.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	118119	14.06	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	167183	18.51	ng/ul	0.00
43) Dimethylphthalate-d6	13.50	166	488213	19.11	ng/ul	0.00
46) Acenaphthylene-d8	13.77	160	479011	15.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	55438	11.49	ng/ul	0.00
57) Fluorene-d10	15.08	176	386432	17.20	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	53393	11.35	ng/ul	0.00
70) Anthracene-d10	16.93	188	592939	17.32	ng/ul	0.00
78) Pyrene-d10	19.24	212	647163	17.65	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.03	264	616810	16.42	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.55	163	75385	2.781	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
Data File : BN009536.D
Acq On : 03 Feb 2020 19:12
Operator : CG/JU
Sample : L1342-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Feb 04 00:21:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 16:39:56 2020
Response via : Initial Calibration

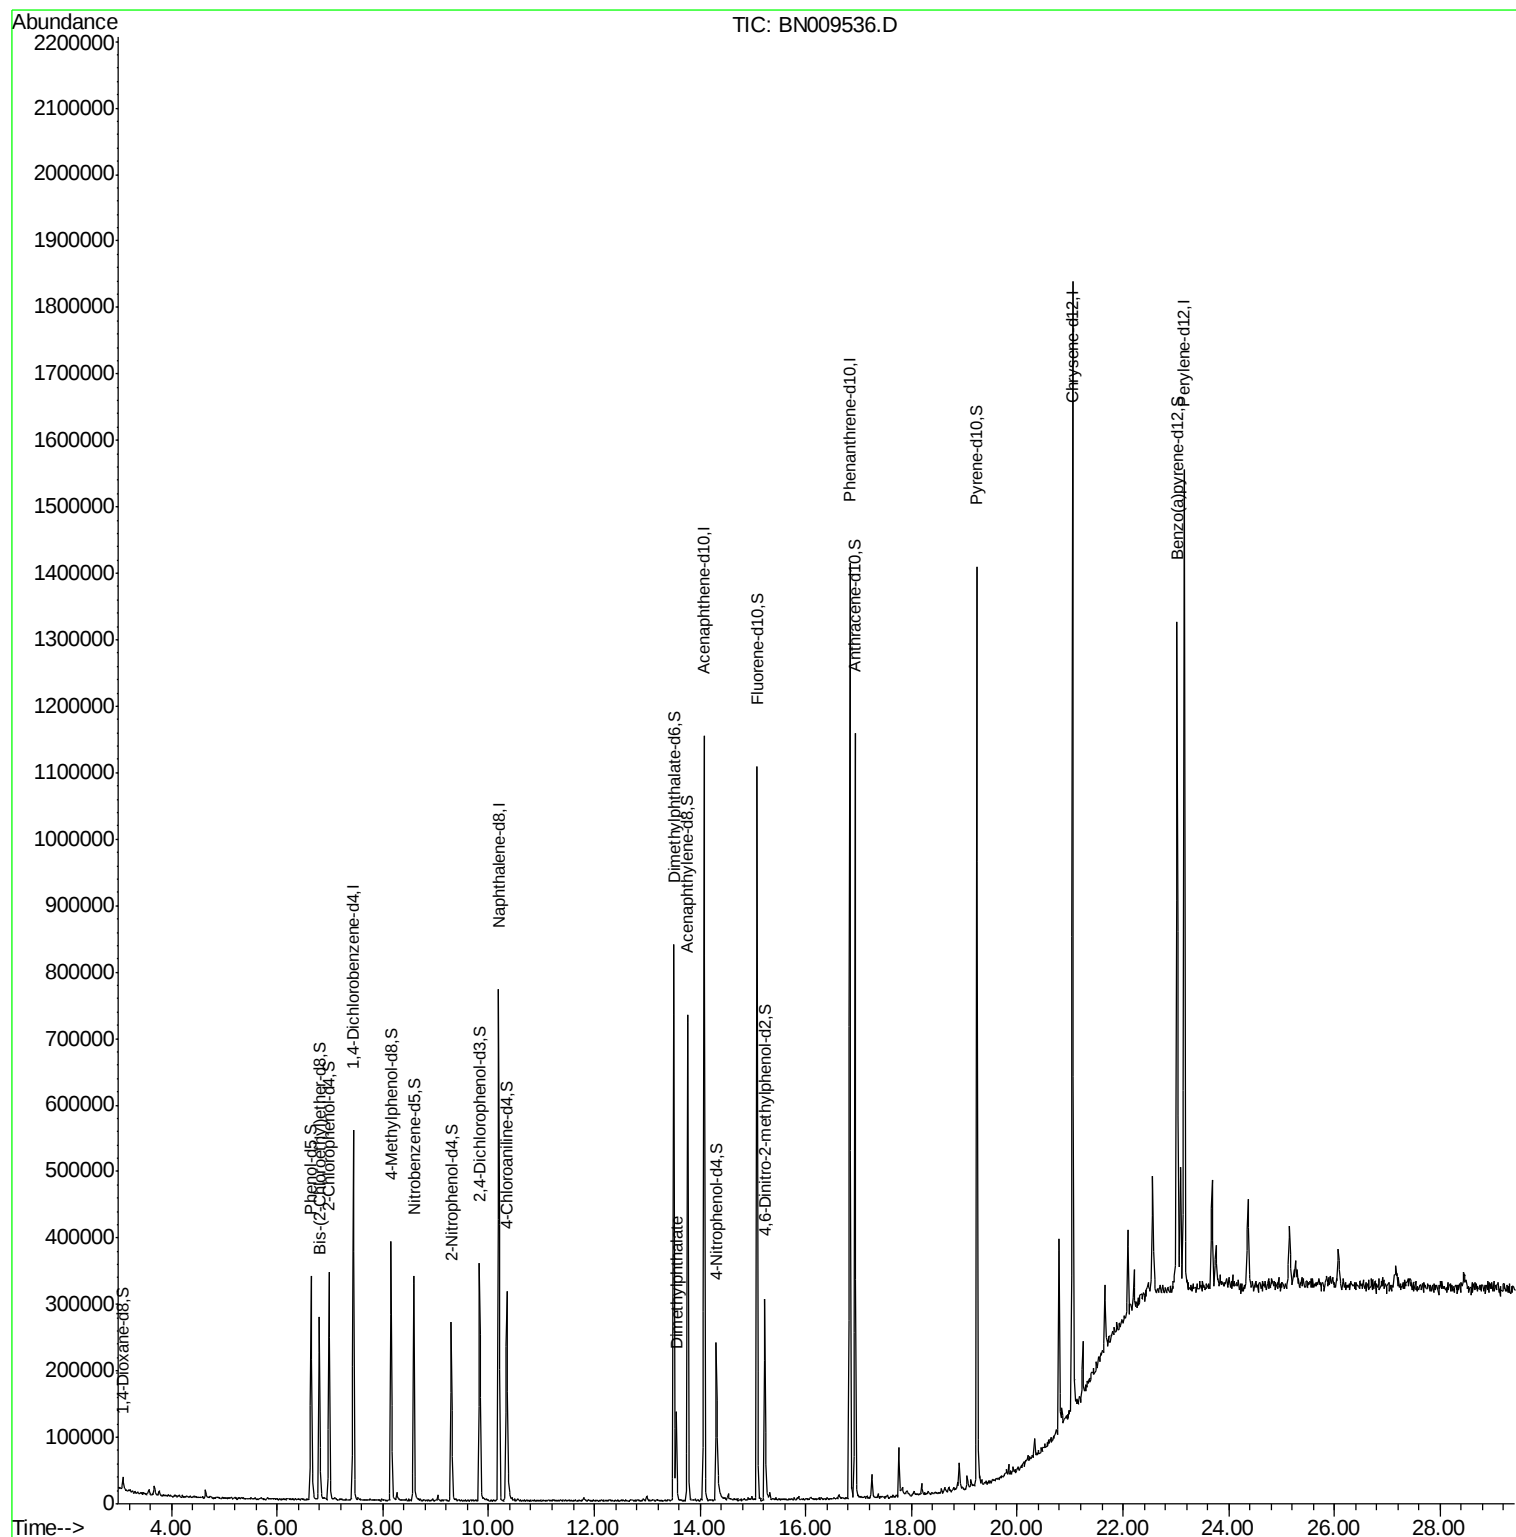

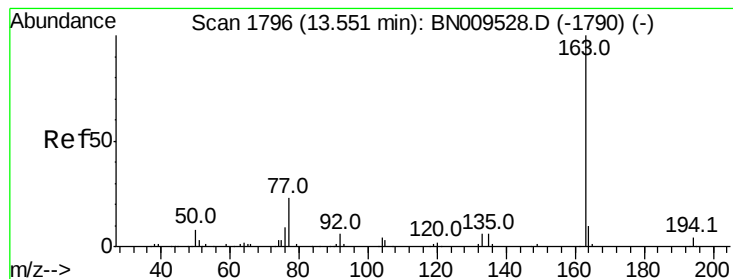

#44

Dimethylphthalate

Concen: 2.781 ng/ul

RT: 13.55 min Scan# 1796

Delta R.T. -0.00 min

Lab File: BN009536.D

Acq: 03 Feb 2020 19:12

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 75385

Ion Ratio Lower Upper

163 100

194 3.4 3.5 5.3#

164 10.4 8.0 12.0

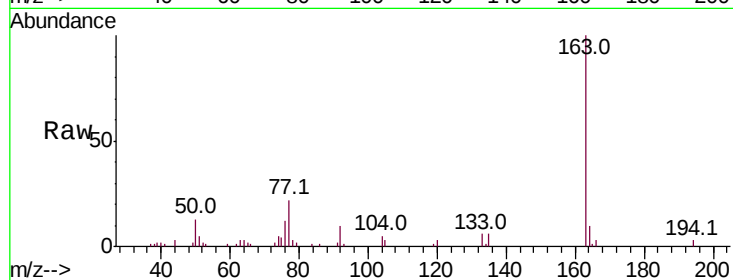

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

