

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
 Data File : BN009535.D
 Acq On : 03 Feb 2020 18:36
 Operator : CG/JU
 Sample : L1342-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AG7

Quant Time: Feb 04 00:20:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 16:39:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	137495	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	572299	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.08	164	367690	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.83	188	779536	20.00	ng/ul	0.00
77) Chrysene-d12	21.05	240	707709	20.00	ng/ul	0.00
85) Perylene-d12	23.16	264	807044	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	17921	5.35	ng/uL	0.00
5) Phenol-d5	6.64	99	316535	26.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	233546	29.00	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	257302	29.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	253272	26.52	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	121766	28.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	137251	28.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	240563	27.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.34	131	344871	36.05	ng/ul	0.00
43) Dimethylphthalate-d6	13.50	166	822444	30.64	ng/ul	0.00
46) Acenaphthylene-d8	13.76	160	947419	29.21	ng/ul	0.00
51) 4-Nitrophenol-d4	14.31	143	108946	21.49	ng/ul	0.00
57) Fluorene-d10	15.08	176	700111	29.66	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.22	200	100802	20.70	ng/ul	0.00
70) Anthracene-d10	16.93	188	1077280	30.41	ng/ul	0.00
78) Pyrene-d10	19.24	212	1176362	31.62	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.03	264	1211843	30.50	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	13.55	163	117058	4.109	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
Data File : BN009535.D
Acq On : 03 Feb 2020 18:36
Operator : CG/JU
Sample : L1342-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
B0AG7

Quant Time: Feb 04 00:20:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 16:39:56 2020
Response via : Initial Calibration

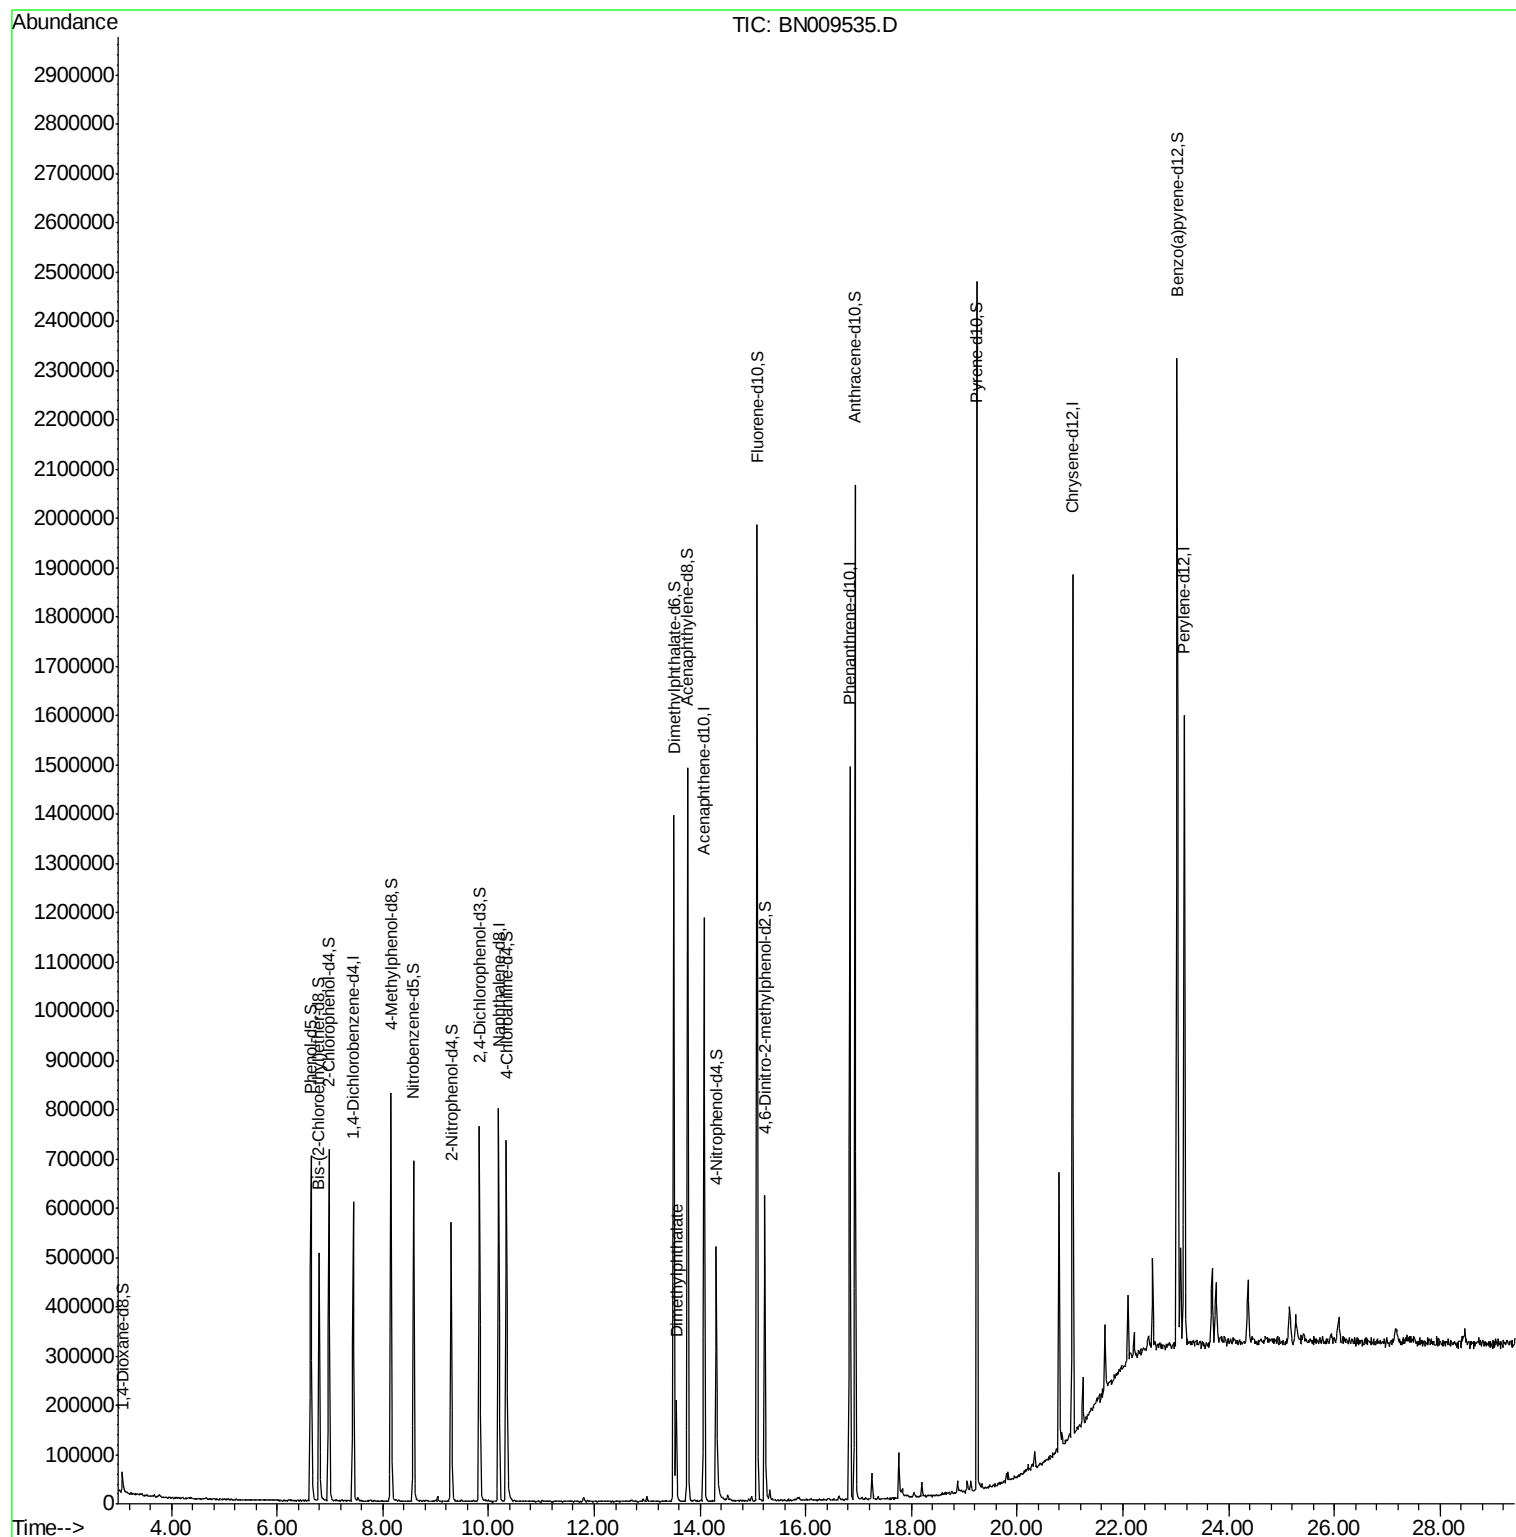

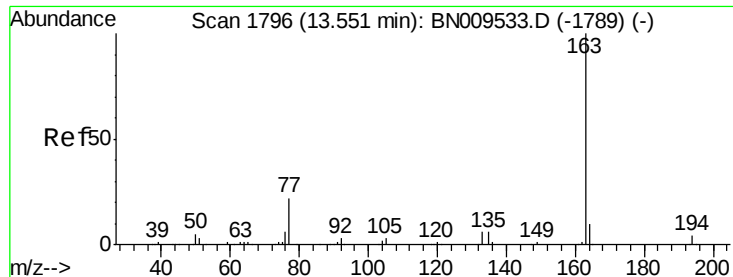

#44

Dimethylphthalate

Concen: 4.109 ng/ul

RT: 13.55 min Scan# 1796

Delta R.T. 0.00 min

Lab File: BN009535.D

Acq: 03 Feb 2020 18:36

Instrument :

BNA_N

ClientSampleId :

B0AG7


Tot Ion:163 Resp: 117058

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 9.0 8.0 12.0

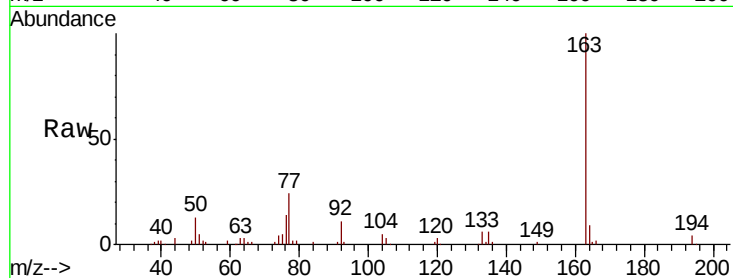

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

