

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
 Data File : BN009539.D
 Acq On : 03 Feb 2020 21:00
 Operator : CG/JU
 Sample : L1342-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AH2

Quant Time: Feb 04 00:21:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 16:39:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	145942	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	615501	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.08	164	398469	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.83	188	841938	20.00	ng/ul	0.00
77) Chrysene-d12	21.05	240	783517	20.00	ng/ul	0.00
85) Perylene-d12	23.16	264	831664	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	7550	2.12	ng/uL	0.00
5) Phenol-d5	6.64	99	125694	9.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	102659	12.01	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	100612	10.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	102523	10.11	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	51993	11.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	54124	10.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	92950	9.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	128942	12.53	ng/ul	0.00
43) Dimethylphthalate-d6	13.50	166	384791	13.23	ng/ul	0.00
46) Acenaphthylene-d8	13.76	160	369239	10.51	ng/ul	0.00
51) 4-Nitrophenol-d4	14.31	143	42241	7.69	ng/ul	0.00
57) Fluorene-d10	15.08	176	306553	11.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	39823	7.57	ng/ul	0.00
70) Anthracene-d10	16.93	188	439725	11.49	ng/ul	0.00
78) Pyrene-d10	19.23	212	484656	11.77	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.02	264	467664	11.42	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.55	163	55641	1.802	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
Data File : BN009539.D
Acq On : 03 Feb 2020 21:00
Operator : CG/JU
Sample : L1342-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
B0AH2

Quant Time: Feb 04 00:21:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 16:39:56 2020
Response via : Initial Calibration

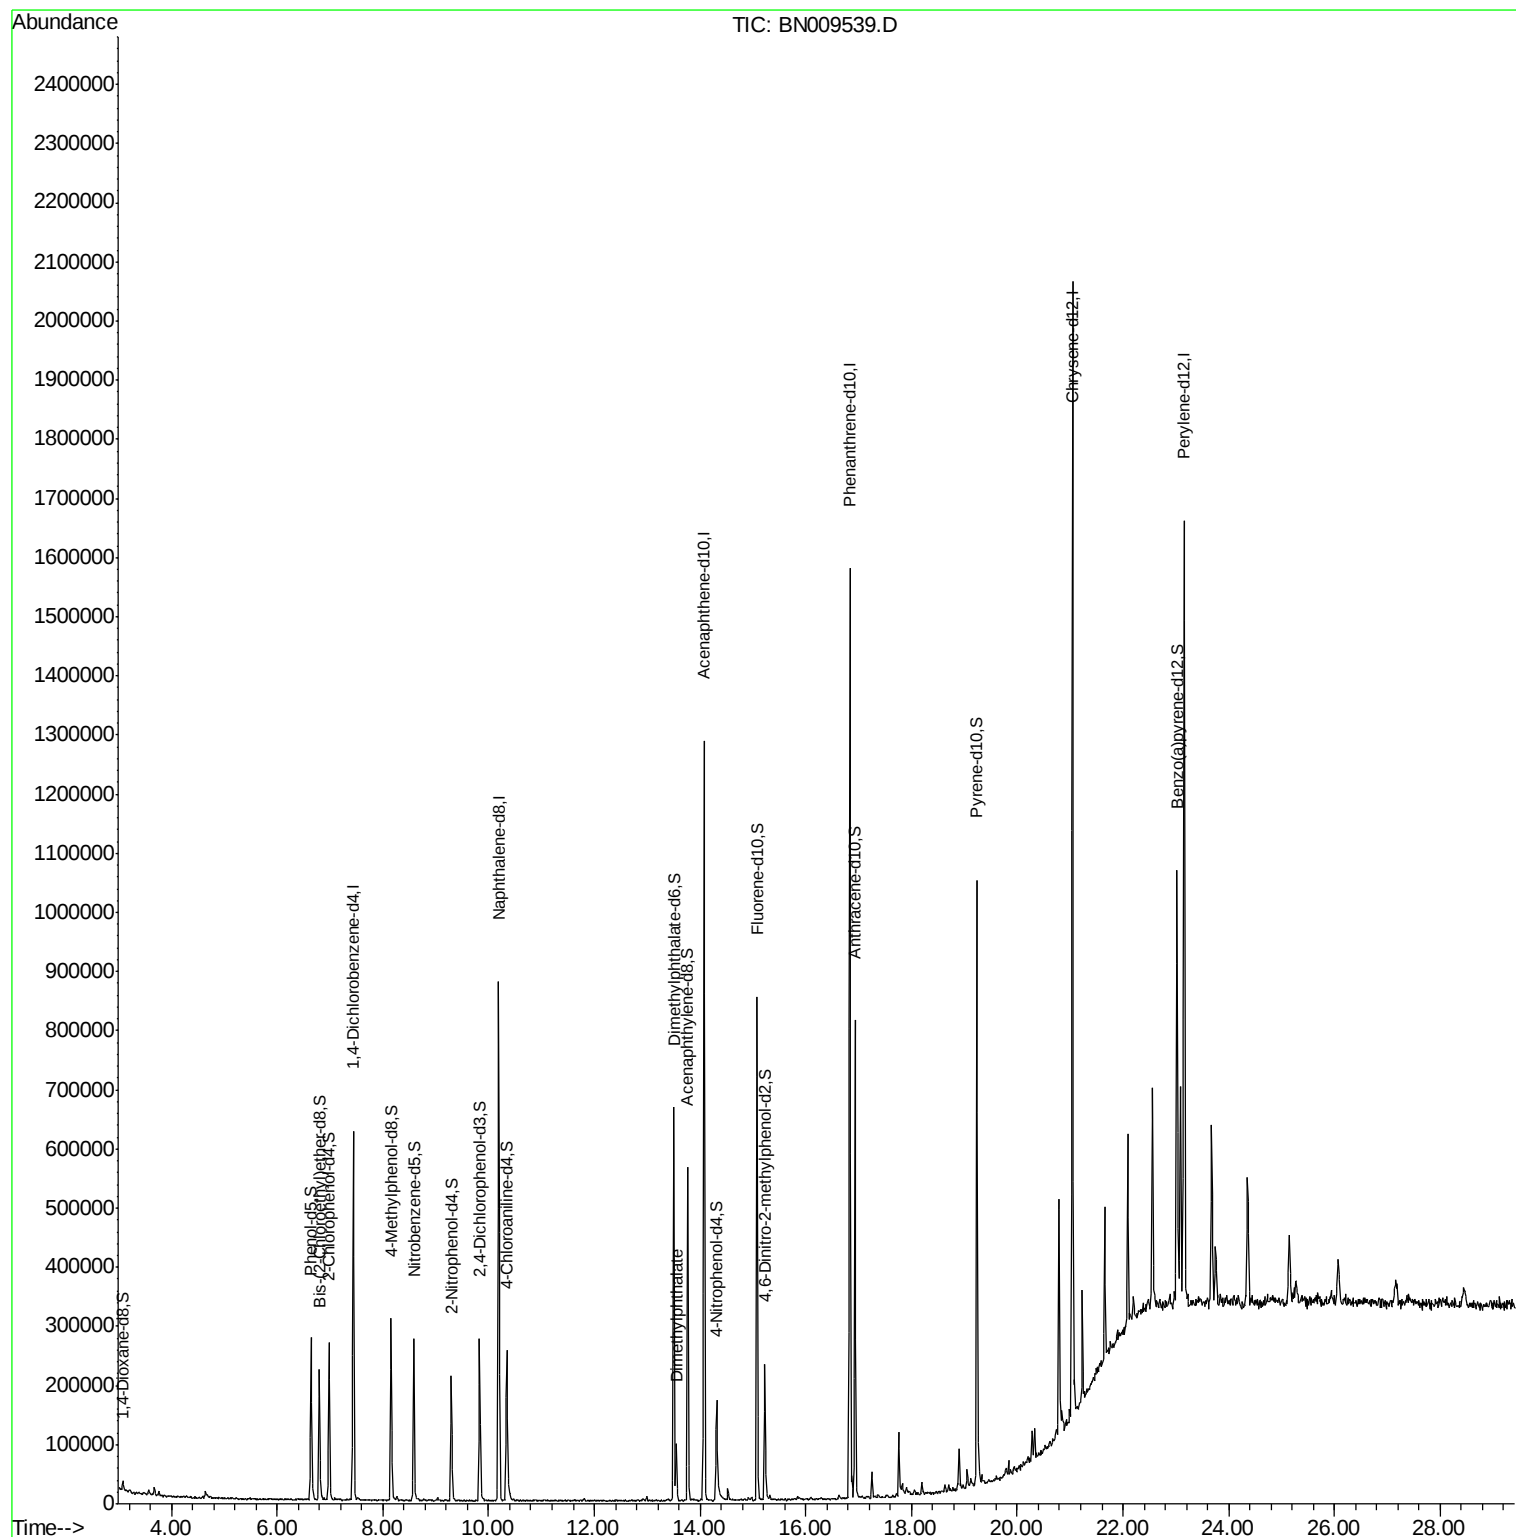

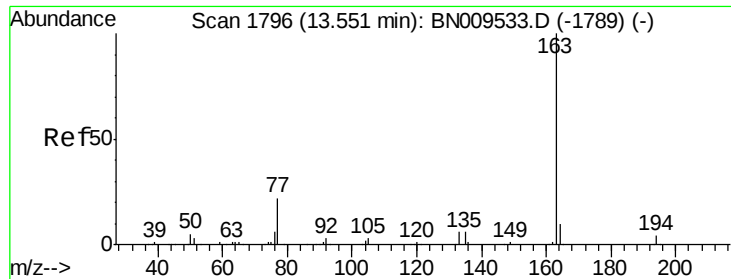

#44

Dimethylphthalate

Concen: 1.802 ng/ul

RT: 13.55 min Scan# 1796

Delta R.T. 0.00 min

Lab File: BN009539.D

Acq: 03 Feb 2020 21:00

Instrument :

BNA_N

ClientSampleId :

B0AH2


Tot Ion:163 Resp: 55641

Ion Ratio Lower Upper

163 100

194 3.8 3.5 5.3

164 11.6 8.0 12.0

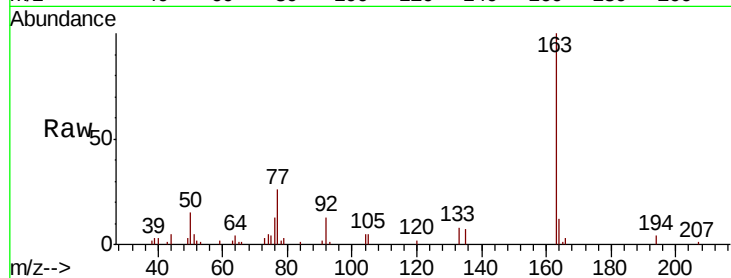

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

