

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
 Data File : BN009563.D
 Acq On : 04 Feb 2020 14:26
 Operator : CG/JU
 Sample : L1302-02
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C5AK8

Quant Time: Feb 04 15:11:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 16:39:56 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	126412	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	534086	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.07	164	328475	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.83	188	702404	20.00	ng/ul	0.00
77) Chrysene-d12	21.05	240	685913	20.00	ng/ul	0.00
85) Perylene-d12	23.16	264	711689	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	5267	1.71	ng/uL	0.00
5) Phenol-d5	6.64	99	107706	9.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	78931	10.66	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	86456	10.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	59044	6.72	ng/ul	0.00
19) Nitrobenzene-d5	8.59	128	41828	10.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	47015	10.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	84344	10.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	92729	10.39	ng/ul	0.00
43) Dimethylphthalate-d6	13.50	166	283959	11.84	ng/ul	0.00
46) Acenaphthylene-d8	13.76	160	328524	11.34	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	31832	7.03	ng/ul	0.00
57) Fluorene-d10	15.08	176	252689	11.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	22960	5.23	ng/ul	0.00
70) Anthracene-d10	16.93	188	374963	11.75	ng/ul	0.00
78) Pyrene-d10	19.23	212	459481	12.74	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.03	264	448775	12.81	ng/ul	0.00
Target Compounds						
6) Phenol	6.66	94	15382	1.306	ng/ul	98
14) Acetophenone	8.26	105	15533	1.106	ng/ul	96
44) Dimethylphthalate	13.55	163	96752	3.802	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020320\
Data File : BN009563.D
Acq On : 04 Feb 2020 14:26
Operator : CG/JU
Sample : L1302-02
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C5AK8

Quant Time: Feb 04 15:11:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 16:39:56 2020
Response via : Initial Calibration

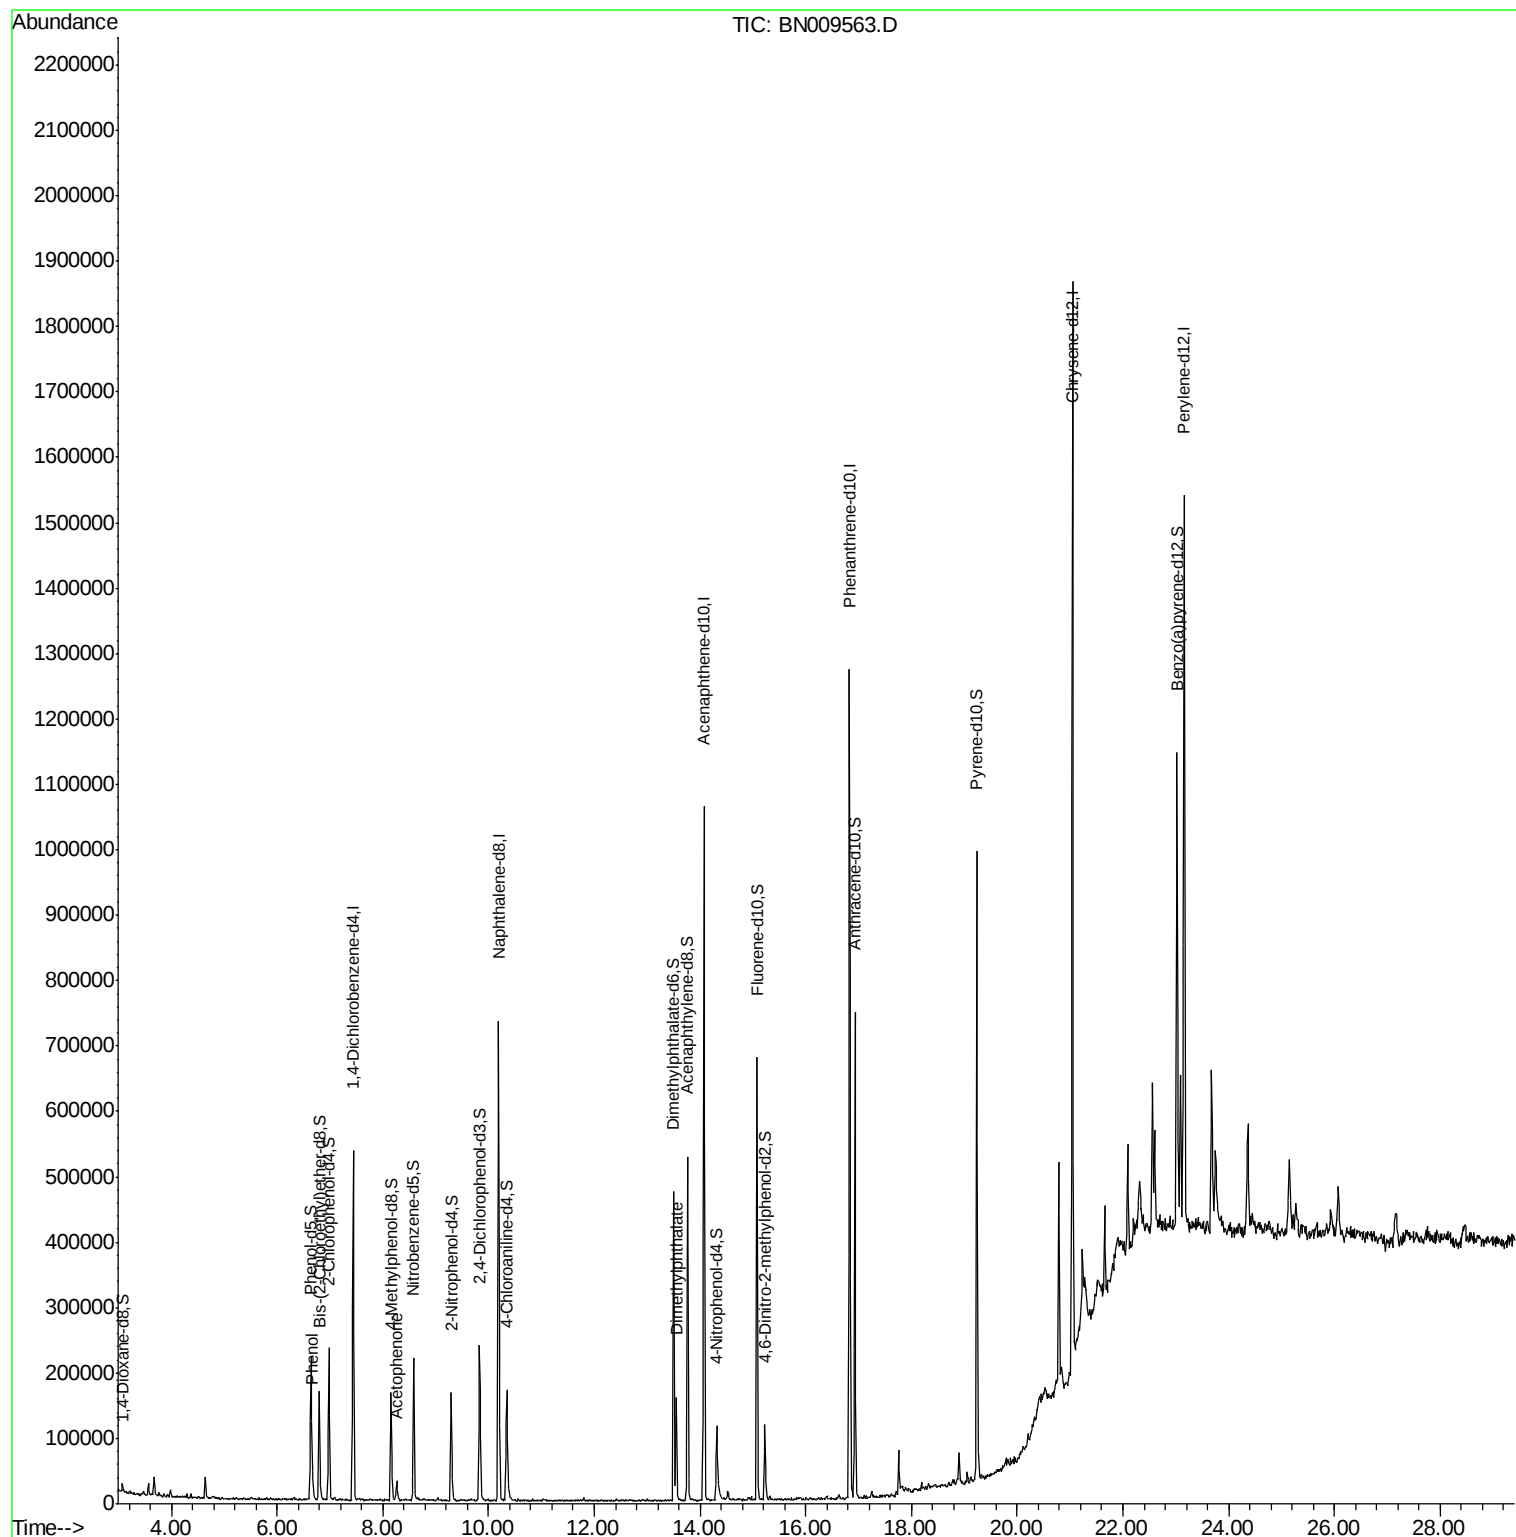

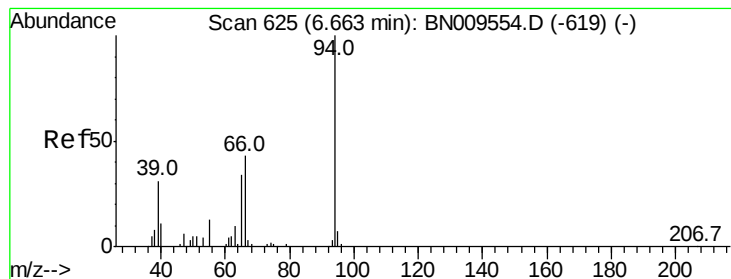





#6

Phenol

Concen: 1.306 ng/ul
 RT: 6.66 min Scan# 625
 Delta R.T. -0.01 min
 Lab File: BN009563.D
 Acq: 04 Feb 2020 14:26

Instrument :
 BNA_N
 ClientSampleId :
 C5AK8

Tot Ion: 94 Resp: 15382
 Ion Ratio Lower Upper
 94 100
 65 37.3 29.8 44.6
 66 52.2 39.5 59.3

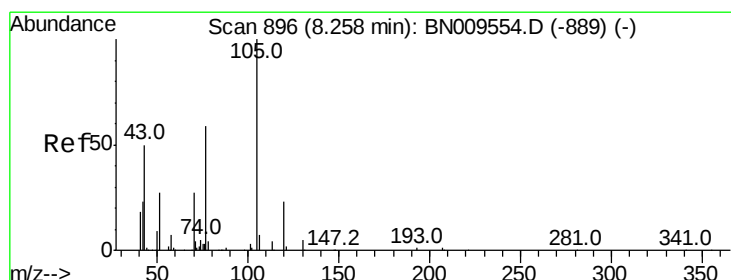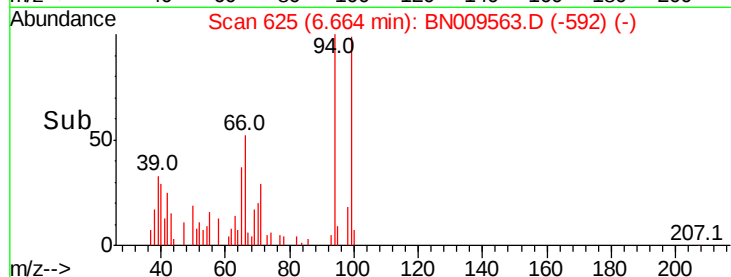
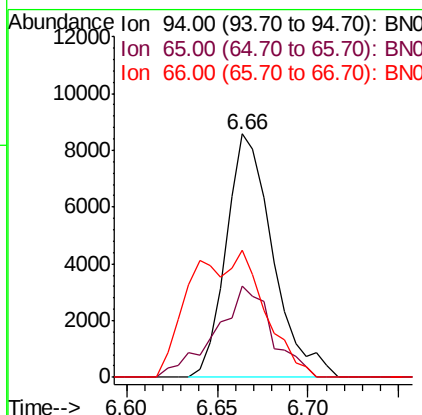
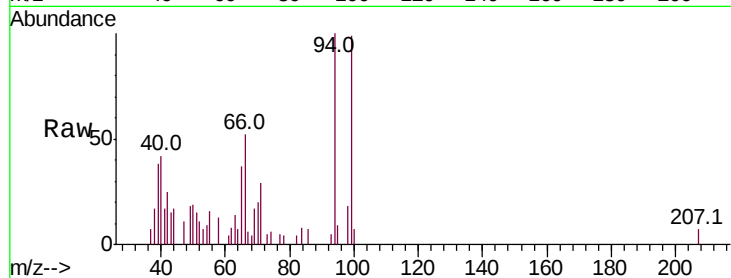



#14

Acetophenone

Concen: 1.106 ng/ul
 RT: 8.26 min Scan# 897
 Delta R.T. 0.01 min
 Lab File: BN009563.D
 Acq: 04 Feb 2020 14:26

Tgt Ion: 105 Resp: 15533
 Ion Ratio Lower Upper
 105 100
 77 90.2 67.7 101.5
 51 43.0 34.3 51.5

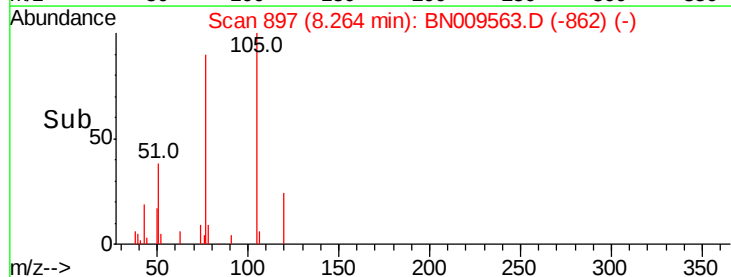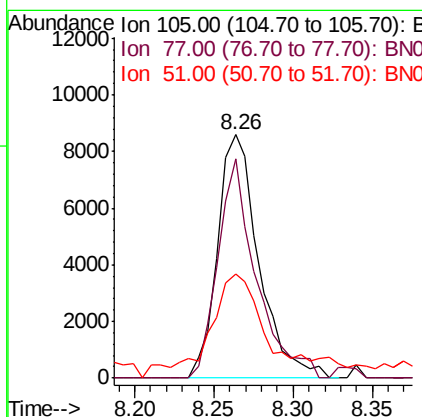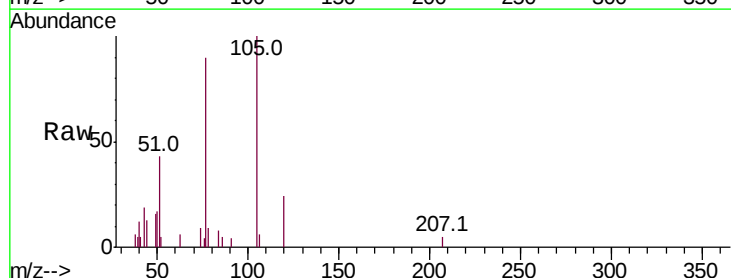

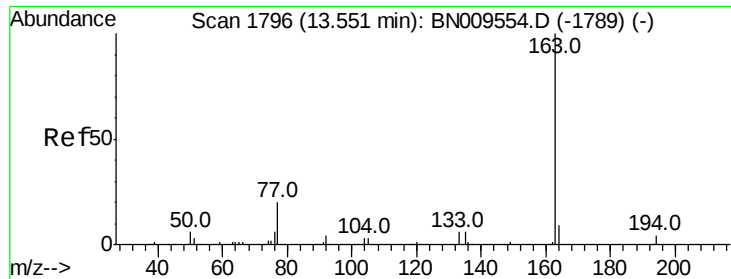

#44

Dimethylphthalate

Concen: 3.802 ng/ul

RT: 13.55 min Scan# 1796

Delta R.T. 0.00 min

Lab File: BN009563.D

Acq: 04 Feb 2020 14:26

Instrument :

BNA_N

ClientSampleId :

C5AK8


Tot Ion:163 Resp: 96752

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 9.8 8.0 12.0

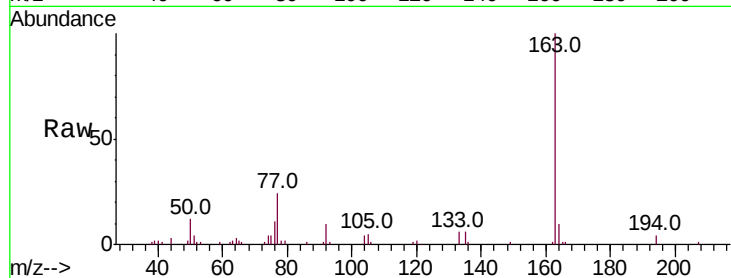

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

