

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020320\
 Data File : BN009575.D
 Acq On : 04 Feb 2020 21:39
 Operator : CG/JU
 Sample : L1302-13
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C5AN0

Manual Integrations
 APPROVED

mohammad
 2/6/2020 8:12:19 AM

Quant Time: Feb 05 01:08:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 16:39:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	141902	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	597377	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.07	164	379497	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.83	188	792695	20.00	ng/ul	0.00
77) Chrysene-d12	21.04	240	793702	20.00	ng/ul	0.00
85) Perylene-d12	23.15	264	850854	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	4729	1.37	ng/uL	0.00
5) Phenol-d5	6.64	99	87790	7.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	66961	8.06	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	70524	7.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	56209	5.70	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	34674	7.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	35544	7.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	65806	7.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	73946	7.41	ng/ul	0.00
43) Dimethylphthalate-d6	13.50	166	230370	8.32	ng/ul	0.00
46) Acenaphthylene-d8	13.76	160	264910	7.91	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	19955	3.81	ng/ul	0.01
57) Fluorene-d10	15.08	176	202948	8.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	17286	3.49	ng/ul	0.00
70) Anthracene-d10	16.93	188	305460	8.48	ng/ul	0.00
78) Pyrene-d10	19.23	212	381755	9.15	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.02	264	390108	9.31	ng/ul	0.00
Target Compounds				Ovalue		
44) Dimethylphthalate	13.55	163	111355	3.788	ng/ul	99
69) Phenanthrene	16.87	178	253157	5.600	ng/ul	98
76) Fluoranthene	18.90	202	521048	10.099	ng/ul	100
79) Pyrene	19.26	202	432939	7.472	ng/ul	98
82) Benzo(a)anthracene	21.03	228	206498	3.768	ng/ul	98
84) Chrysene	21.07	228	235952	4.325	ng/ul	98
87) Benzo(b)fluoranthene	22.53	252	278328	5.228	ng/ul	100
88) Benzo(k)fluoranthene	22.57	252	101566m	1.937	ng/ul	
90) Benzo(a)pyrene	23.06	252	177323	3.595	ng/ul	96
91) Indeno(1,2,3-cd)pyrene	25.21	276	119975	2.046	ng/ul#	93
93) Benzo(g,h,i)perylene	25.83	276	108226	2.202	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
Data File : BN009575.D
Acq On : 04 Feb 2020 21:39
Operator : CG/JU
Sample : L1302-13
Misc :
ALS Vial : 51 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C5AN0

Manual Integrations
APPROVED

mohammad
2/6/2020 8:12:19 AM

Quant Time: Feb 05 01:08:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 16:39:56 2020
Response via : Initial Calibration

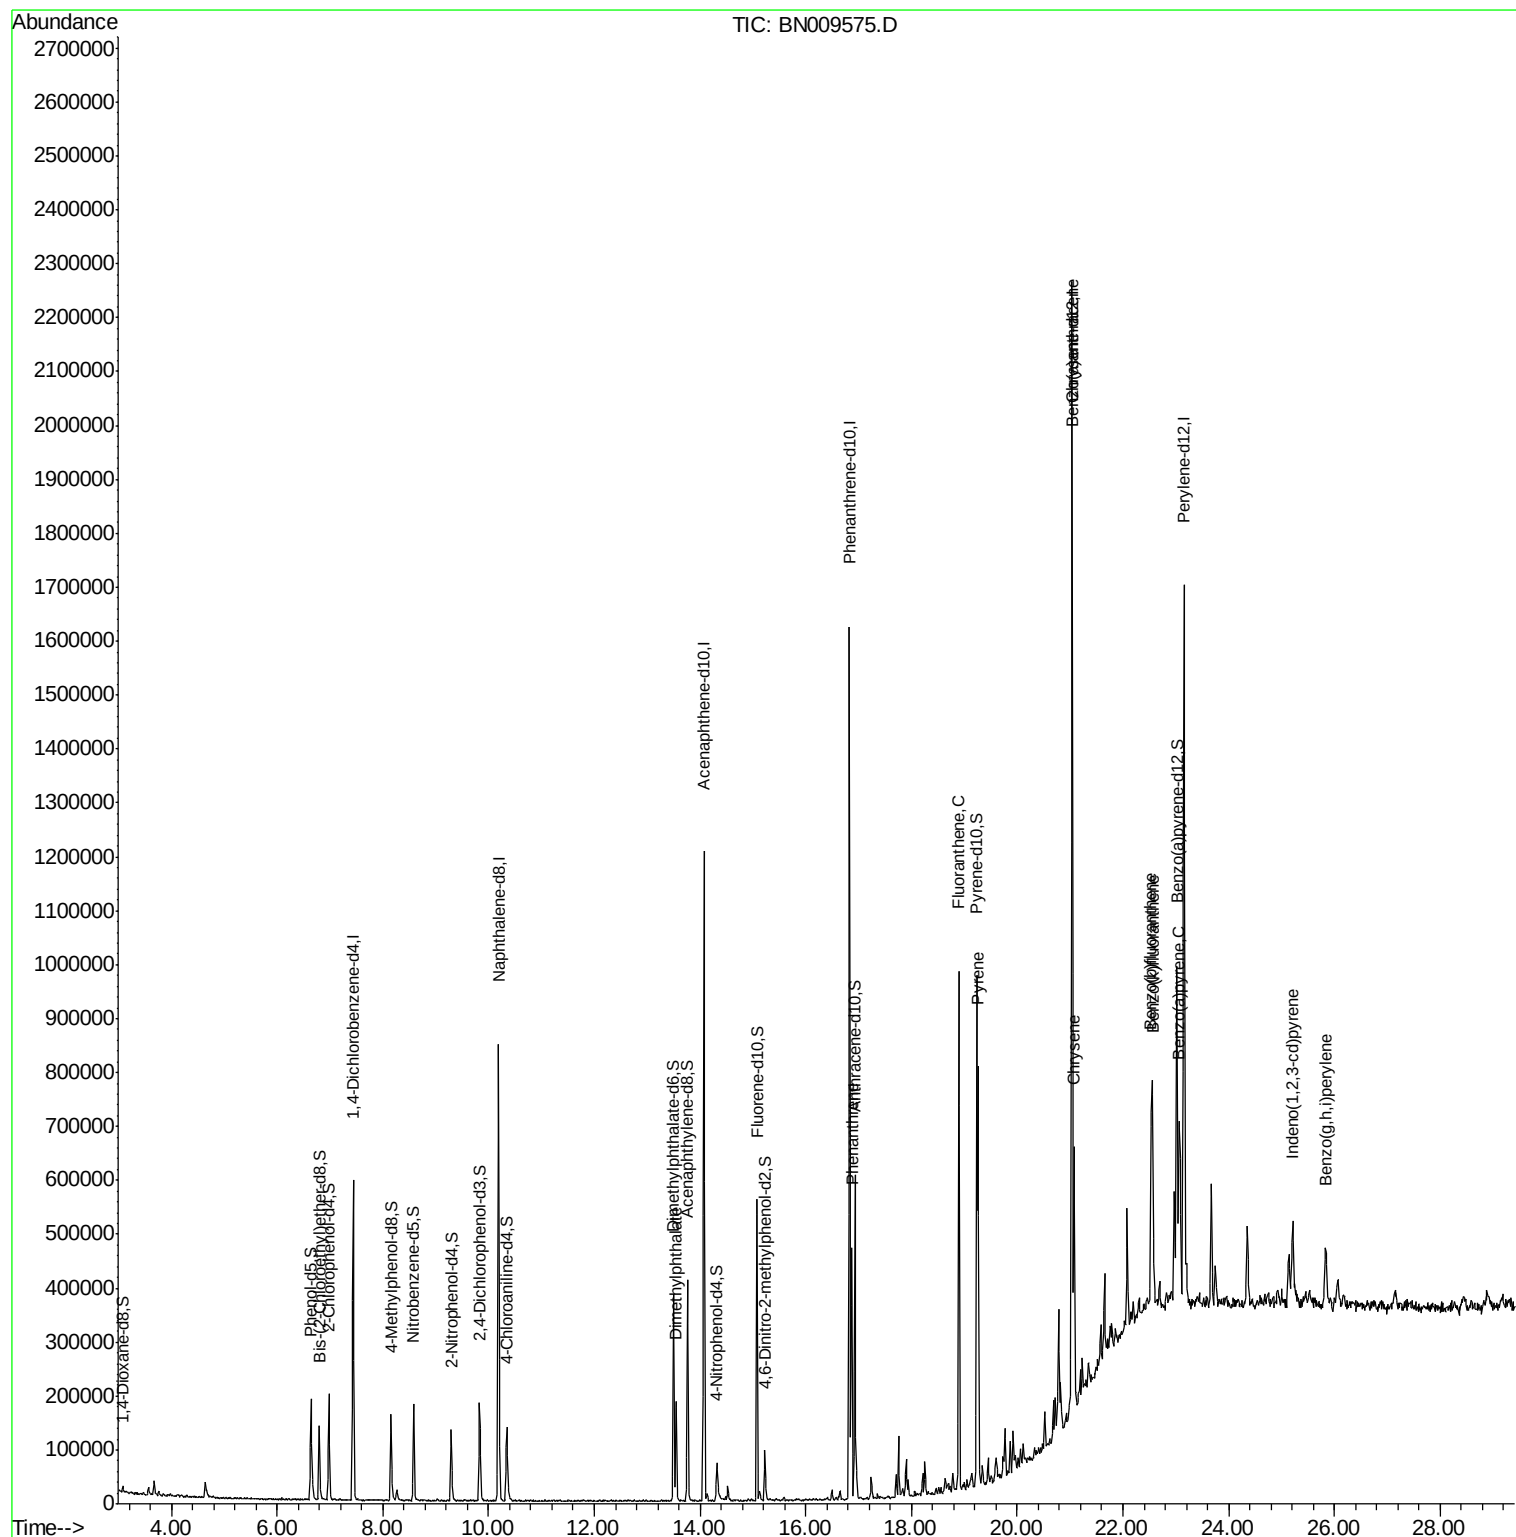

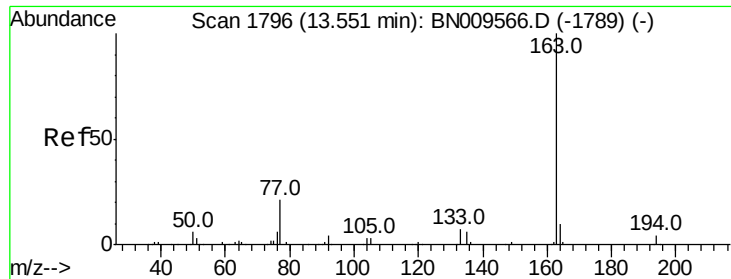


#44
Dimethylphthalate
Concen: 3.788 ng/ul
RT: 13.55 min Scan# 1796
Delta R.T. 0.00 min
Lab File: BN009575.D
Acq: 04 Feb 2020 21:39

Instrument :
BNA_N
ClientSampled :
C5AN0




Tot Ion	Ratio	Resp	Lower	Upper
163	100	111355		
194	4.9	3.5	5.3	
164	9.9	8.0	12.0	

Manual Integrations
APPROVED

mohammad
2/6/2020 8:12:19 AM

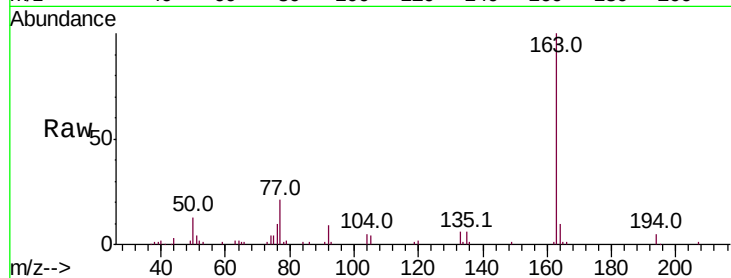


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

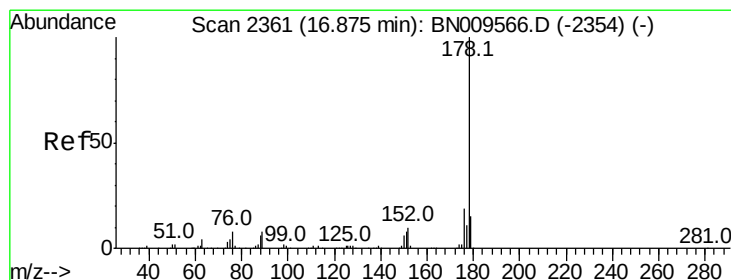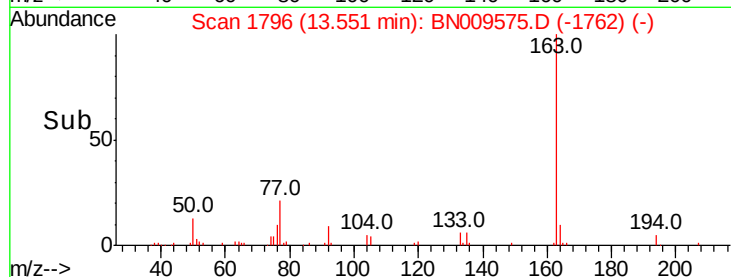
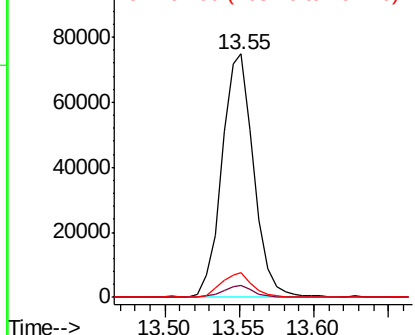



#69
Phenanthrene
Concen: 5.600 ng/ul
RT: 16.87 min Scan# 2360
Delta R.T. -0.01 min
Lab File: BN009575.D
Acq: 04 Feb 2020 21:39

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	253157		
179	16.0	12.2	18.2	
176	19.4	14.8	22.2	

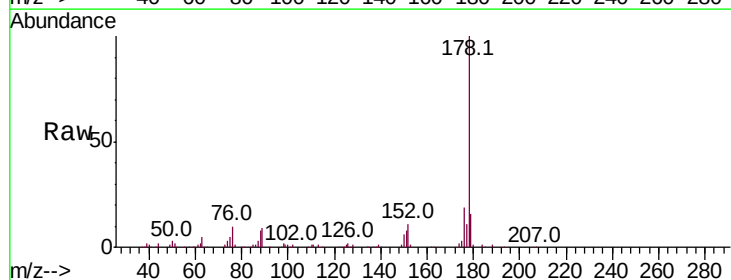

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

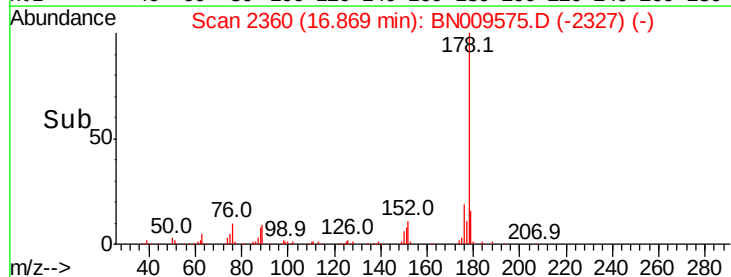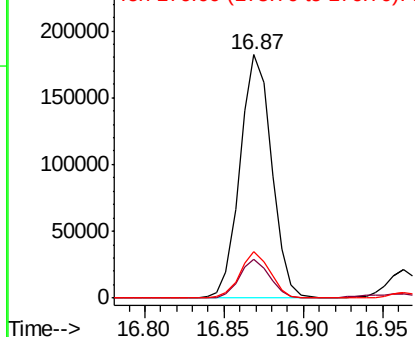

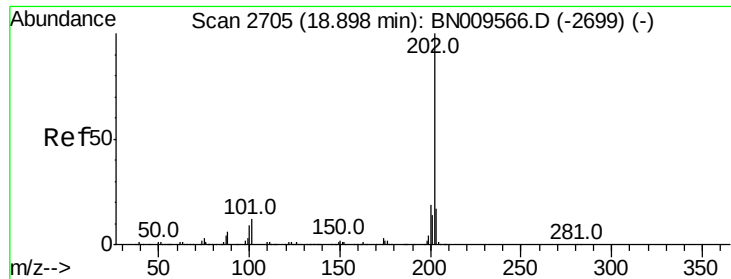


#76
Fluoranthene
Concen: 10.099 ng/ul
RT: 18.90 min Scan# 2705
Delta R.T. -0.01 min
Lab File: BN009575.D
Acq: 04 Feb 2020 21:39

Instrument :
BNA_N
ClientSampleId :
C5AN0




Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	11.5	9.2	13.8
100	8.9	6.9	10.3

Manual Integrations
APPROVED

mohammad
2/6/2020 8:12:19 AM

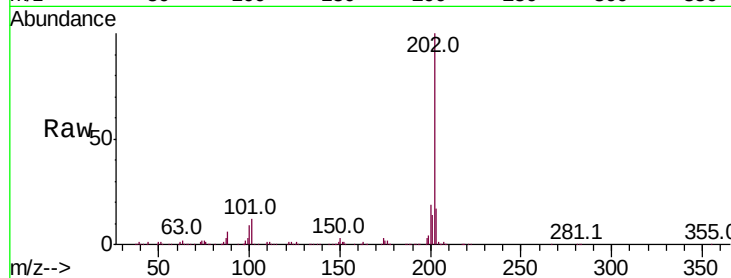




Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

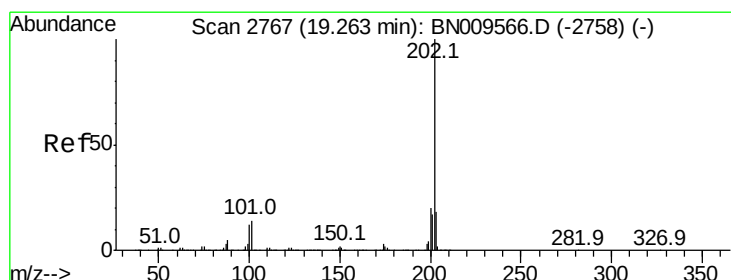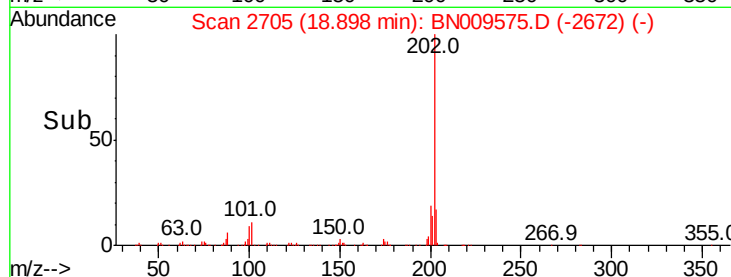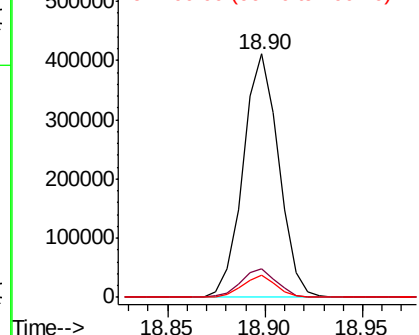


#79
Pyrene
Concen: 7.472 ng/ul
RT: 19.26 min Scan# 2767
Delta R.T. -0.01 min
Lab File: BN009575.D
Acq: 04 Feb 2020 21:39

Tgt Ion	Ratio	Resp Lower	Upper
202	100		
101	13.6	10.3	15.5
100	10.9	8.4	12.6

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

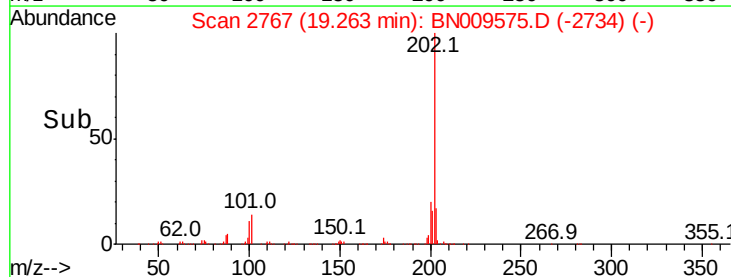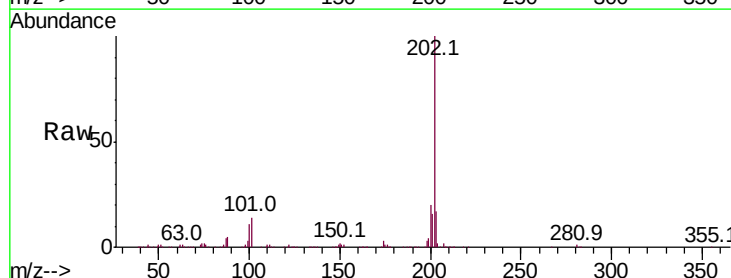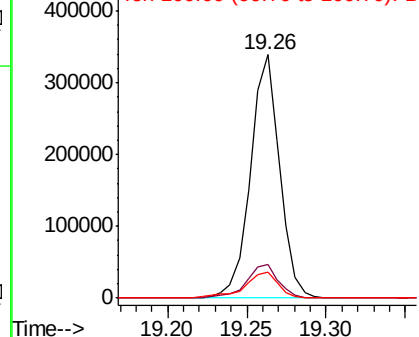

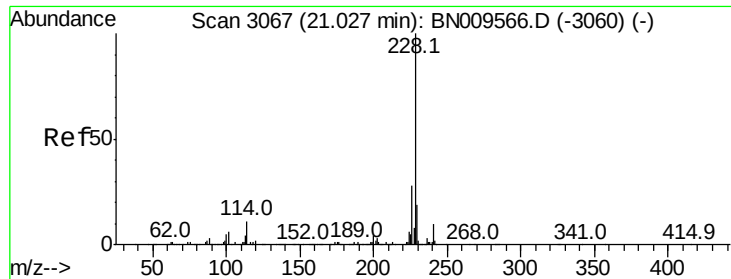





#82
Benzo(a)anthracene
Concen: 3.768 ng/ul
RT: 21.03 min Scan# 3067
Delta R.T. 0.00 min
Lab File: BN009575.D
Acq: 04 Feb 2020 21:39

Instrument :
BNA_N
ClientSampleId :
C5AN0

Tot Ion:	228	Resp:	206498
Ion Ratio	Lower	Upper	
228	100		
229	20.2	15.0	22.4
226	26.4	20.9	31.3




Manual Integrations
APPROVED


mohammad
2/6/2020 8:12:19 AM

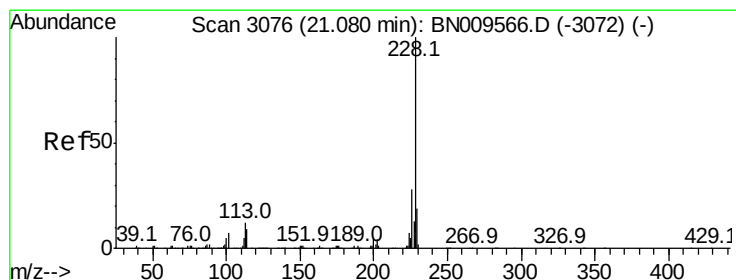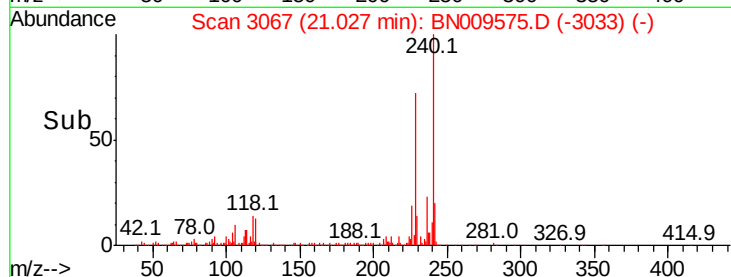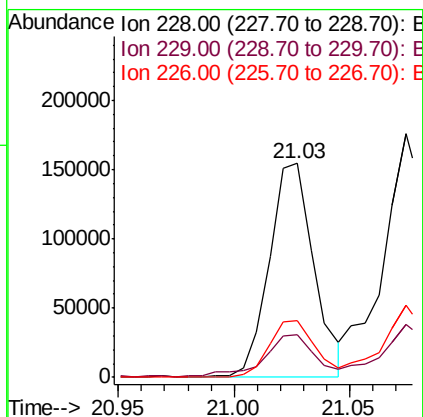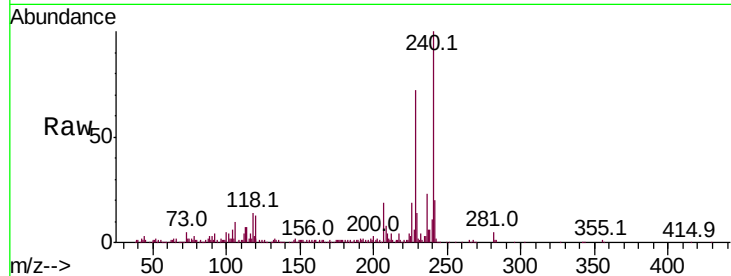

#84
Chrysene
Concen: 4.325 ng/ul
RT: 21.07 min Scan# 3075
Delta R.T. -0.01 min
Lab File: BN009575.D
Acq: 04 Feb 2020 21:39

Tgt Ion:	228	Resp:	235952
Ion Ratio	Lower	Upper	
228	100		
226	29.7	23.5	35.3
229	21.6	15.8	23.8

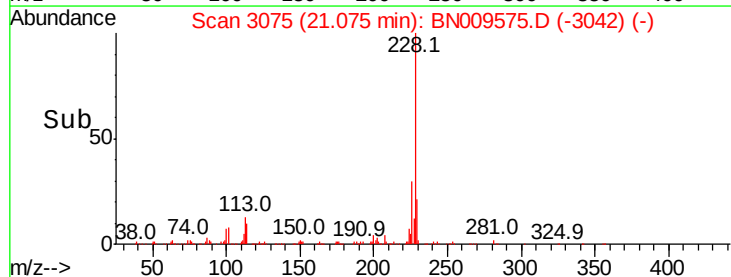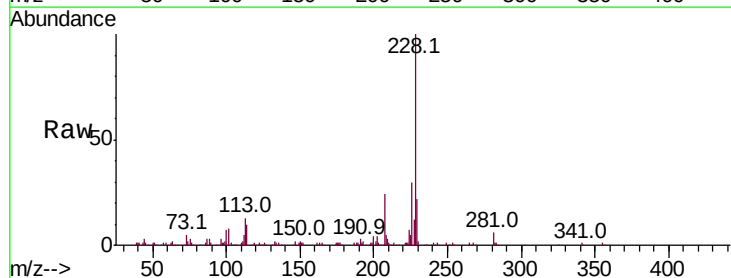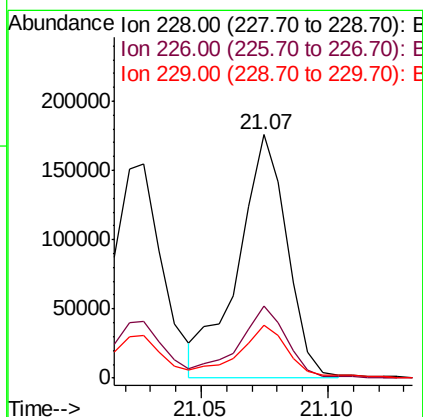

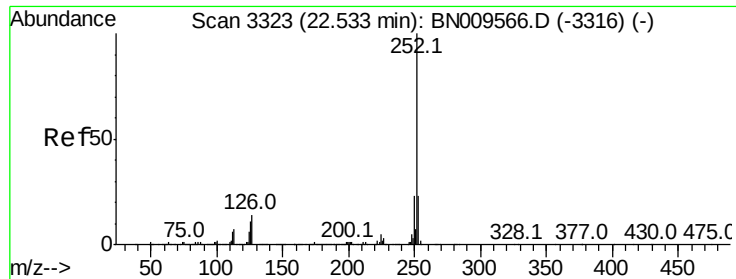





#87
Benzo(b)fluoranthene
Concen: 5.228 ng/ul
RT: 22.53 min Scan# 3323
Delta R.T. 0.00 min
Lab File: BN009575.D
Acq: 04 Feb 2020 21:39

Instrument :
BNA_N
ClientSampleId :
C5AN0

Tot Ion	Ratio	Resp	Lower	Upper
252	100			
253	21.5	17.0	25.6	
125	10.2	8.2	12.2	




Manual Integrations
APPROVED


mohammad
2/6/2020 8:12:19 AM

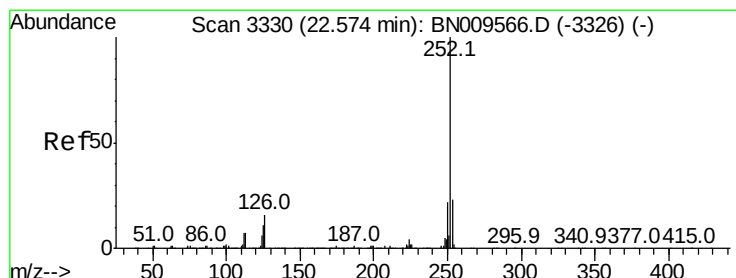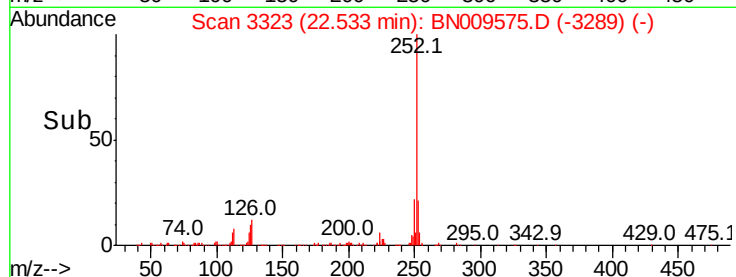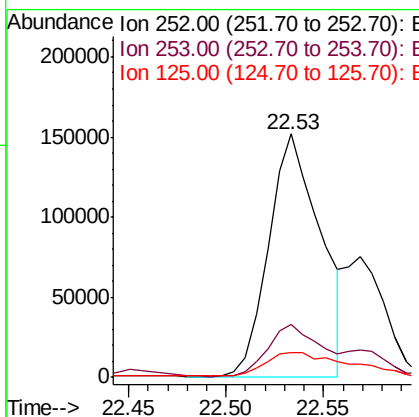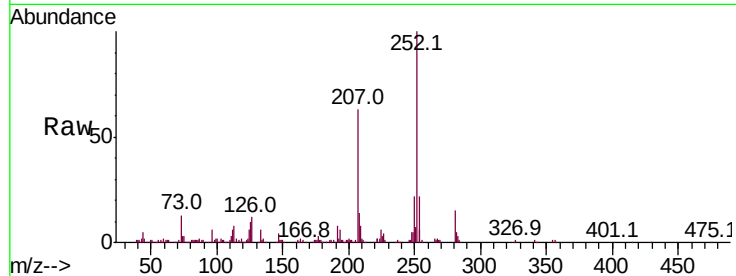

#88
Benzo(k)fluoranthene
Concen: 1.937 ng/ul m
RT: 22.57 min Scan# 3329
Delta R.T. -0.01 min
Lab File: BN009575.D
Acq: 04 Feb 2020 21:39

Tgt Ion	Ratio	Resp	Lower	Upper
252	100			
253	23.2	17.0	25.4	
125	10.6	8.0	12.0	

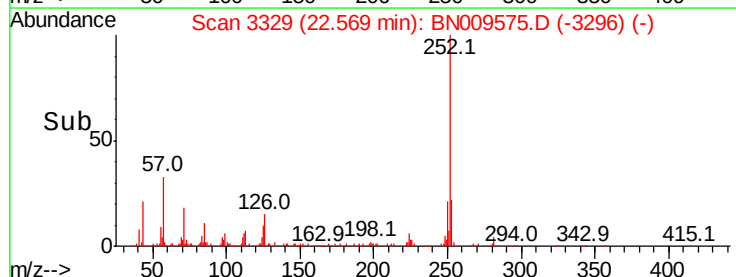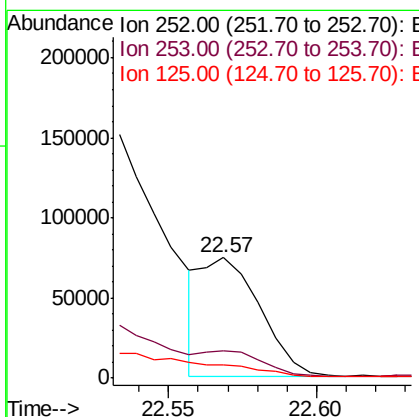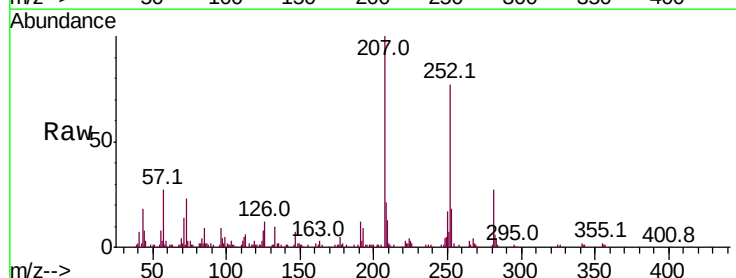

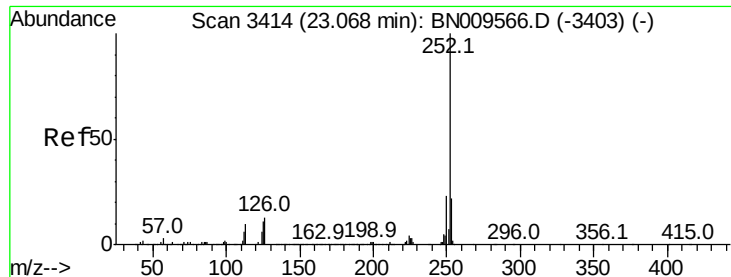


#90
Benzo(a)pyrene
Concen: 3.595 ng/ul
RT: 23.06 min Scan# 3413
Delta R.T. -0.01 min
Lab File: BN009575.D
Acq: 04 Feb 2020 21:39

Instrument :
BNA_N
ClientSampled :
C5AN0

Tot Ion:	252	Resp:	177323
Ion Ratio	Lower	Upper	
252	100		
253	21.6	15.8	23.8
125	12.0	8.7	13.1

Manual Integrations
APPROVED

mohammad
2/6/2020 8:12:19 AM



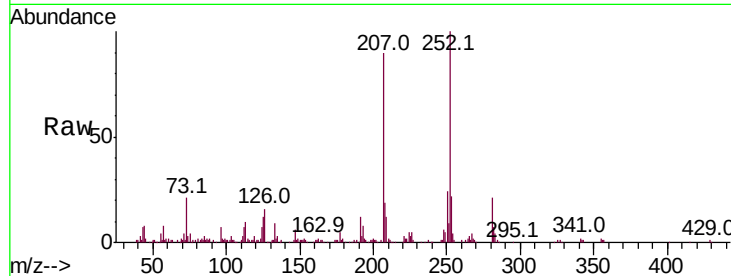


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

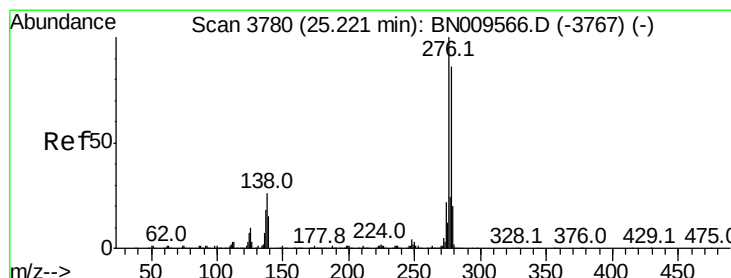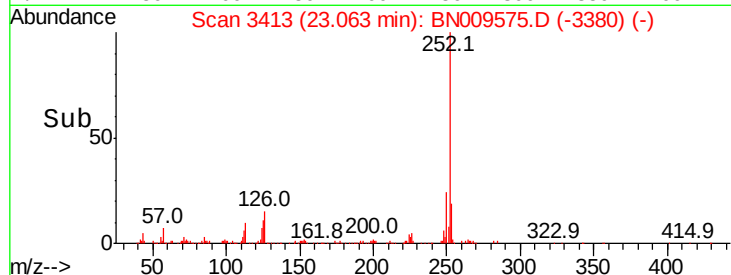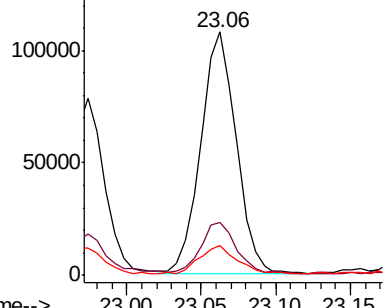

#91
Indeno(1,2,3-cd)pyrene
Concen: 2.046 ng/ul
RT: 25.21 min Scan# 3778
Delta R.T. -0.01 min
Lab File: BN009575.D
Acq: 04 Feb 2020 21:39




Tgt Ion:	276	Resp:	119975
Ion Ratio	Lower	Upper	
276	100		
138	20.1	20.3	30.5#
277	24.7	21.2	31.8


Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

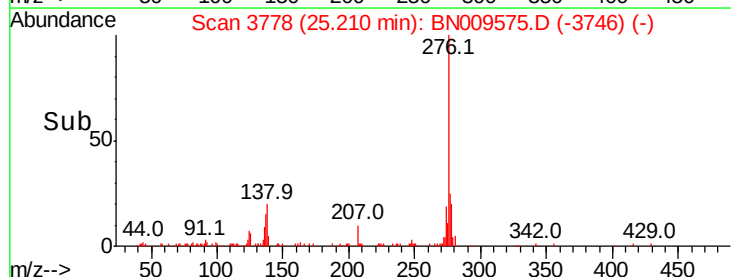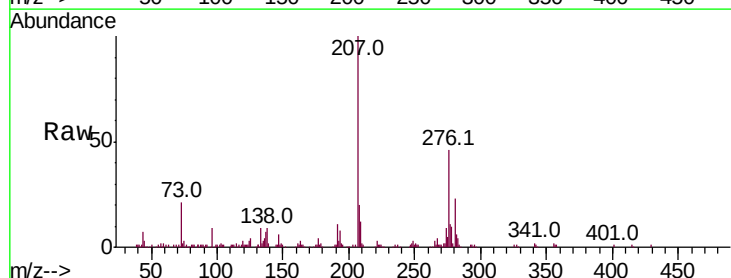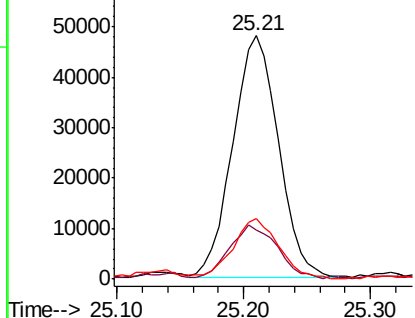

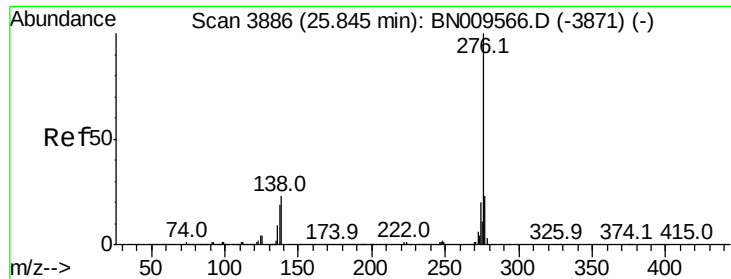

#93

Benzo(a,h,i)perylene

Concen: 2.202 ng/ul

RT: 25.83 min Scan# 3884

Delta R.T. -0.02 min

Lab File: BN009575.D

Acq: 04 Feb 2020 21:39

Instrument :

BNA_N

ClientSampleId :

C5AN0

Tot Ion:	276	Resp:	108226
Ion Ratio	Lower	Upper	
276	100		
138	25.3	16.0	24.0#
277	24.4	17.0	25.6

Manual Integrations
APPROVED

mohammad
2/6/2020 8:12:19 AM

