

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
 Data File : BN009583.D
 Acq On : 05 Feb 2020 03:04
 Operator : CG/JU
 Sample : L1323-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAT41

Quant Time: Feb 05 03:54:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 05 02:53:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	147963	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	601257	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.07	164	381961	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.83	188	789697	20.00	ng/ul	0.00
77) Chrysene-d12	21.04	240	713325	20.00	ng/ul	0.00
85) Perylene-d12	23.15	264	800054	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	16394	4.55	ng/uL	0.00
5) Phenol-d5	6.64	99	282683	21.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	198465	22.90	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	218234	22.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	221547	21.56	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	107321	24.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	115589	23.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	210169	22.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	299936	29.84	ng/ul	0.00
43) Dimethylphthalate-d6	13.50	166	658914	23.63	ng/ul	0.00
46) Acenaphthylene-d8	13.76	160	796267	23.63	ng/ul	0.00
51) 4-Nitrophenol-d4	14.30	143	91825	17.44	ng/ul	0.00
57) Fluorene-d10	15.07	176	582153	23.74	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.22	200	73955	14.99	ng/ul	0.00
70) Anthracene-d10	16.93	188	872439	24.31	ng/ul	0.00
78) Pyrene-d10	19.23	212	960734	25.62	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.02	264	976739	24.79	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.55	163	111653	3.773	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
Data File : BN009583.D
Acq On : 05 Feb 2020 03:04
Operator : CG/JU
Sample : L1323-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAT41

Quant Time: Feb 05 03:54:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 05 02:53:53 2020
Response via : Initial Calibration

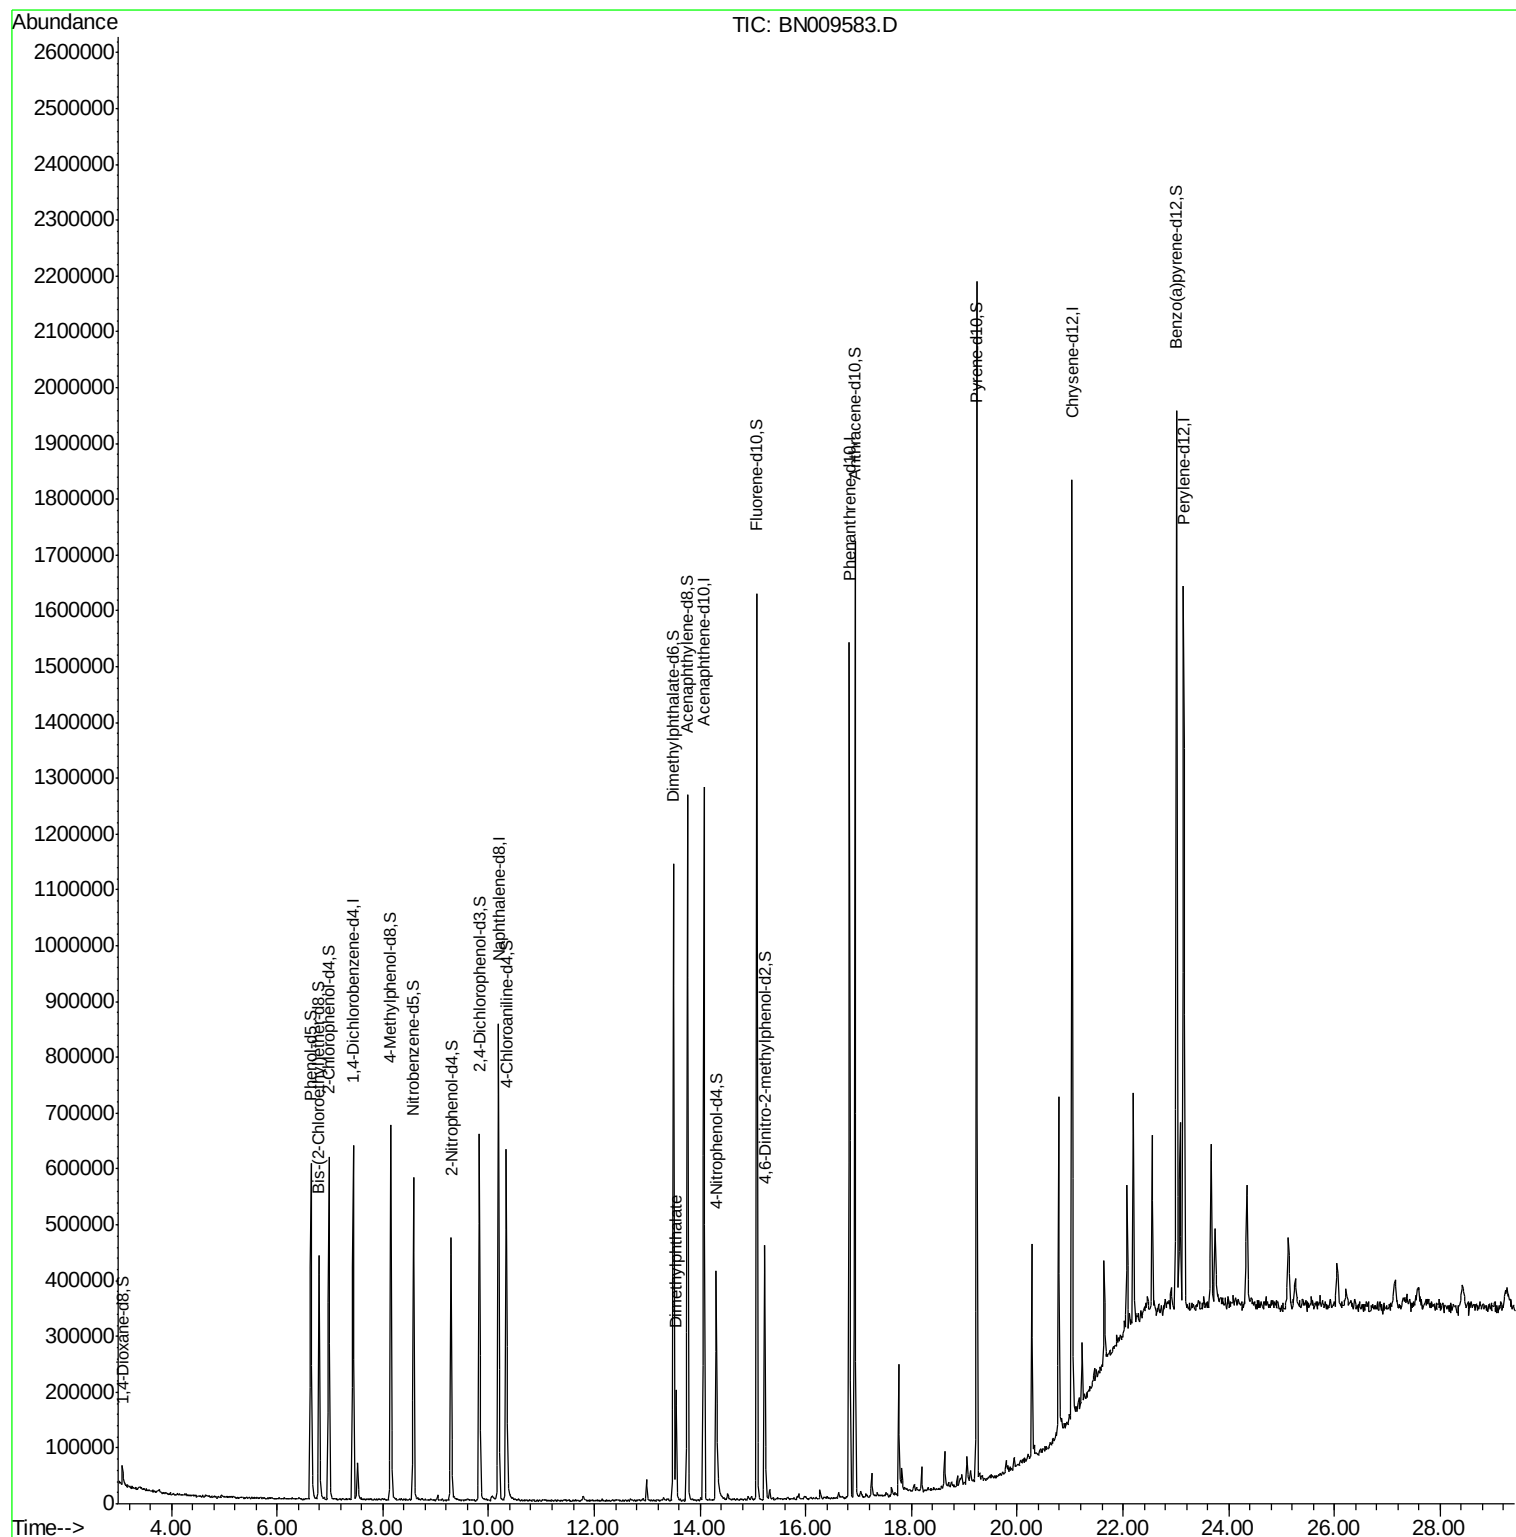

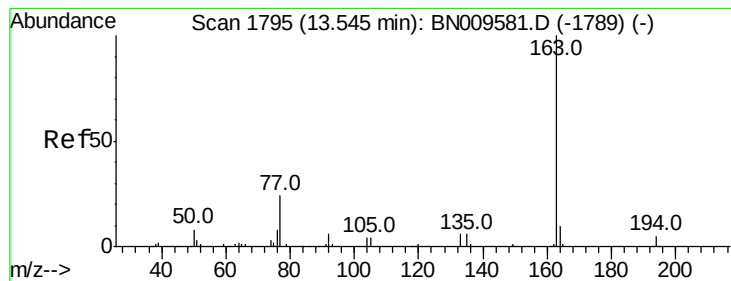

#44

Dimethylphthalate

Concen: 3.773 ng/ul

RT: 13.55 min Scan# 1795

Delta R.T. -0.01 min

Lab File: BN009583.D

Acq: 05 Feb 2020 03:04

Instrument :

BNA_N

ClientSampleId :

GAT41


Tot Ion:163 Resp: 111653

Ion Ratio Lower Upper

163 100

194 3.6 3.5 5.3

164 10.2 8.0 12.0

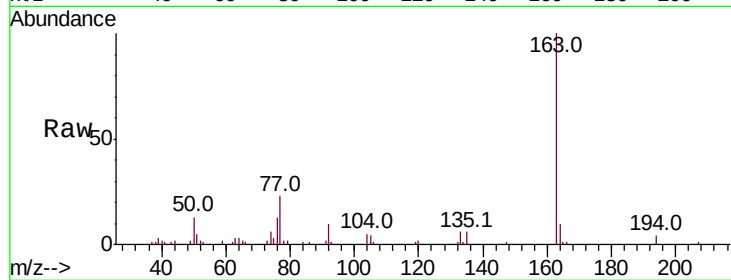

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

