

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
 Data File : BN009584.D
 Acq On : 05 Feb 2020 03:40
 Operator : CG/JU
 Sample : L1323-05
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAT45

Quant Time: Feb 05 04:12:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 05 02:53:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	146456	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	623915	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.07	164	394166	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.83	188	821723	20.00	ng/ul	0.00
77) Chrysene-d12	21.04	240	739610	20.00	ng/ul	0.00
85) Perylene-d12	23.15	264	807516	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	16296	4.57	ng/uL	0.00
5) Phenol-d5	6.63	99	322519	25.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	230184	26.83	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	258555	27.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	256466	25.21	ng/ul	-0.01
19) Nitrobenzene-d5	8.58	128	122951	26.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	135615	26.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	251932	25.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	298713	28.64	ng/ul	0.00
43) Dimethylphthalate-d6	13.50	166	765571	26.61	ng/ul	0.00
46) Acenaphthylene-d8	13.76	160	943708	27.14	ng/ul	0.00
51) 4-Nitrophenol-d4	14.30	143	115559	21.26	ng/ul	0.00
57) Fluorene-d10	15.07	176	693051	27.39	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.22	200	89755	17.49	ng/ul	0.00
70) Anthracene-d10	16.93	188	1058228	28.34	ng/ul	0.00
78) Pyrene-d10	19.23	212	1123148	28.89	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.02	264	1108931	27.89	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.55	163	133626	4.376	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
Data File : BN009584.D
Acq On : 05 Feb 2020 03:40
Operator : CG/JU
Sample : L1323-05
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAT45

Quant Time: Feb 05 04:12:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 05 02:53:53 2020
Response via : Initial Calibration

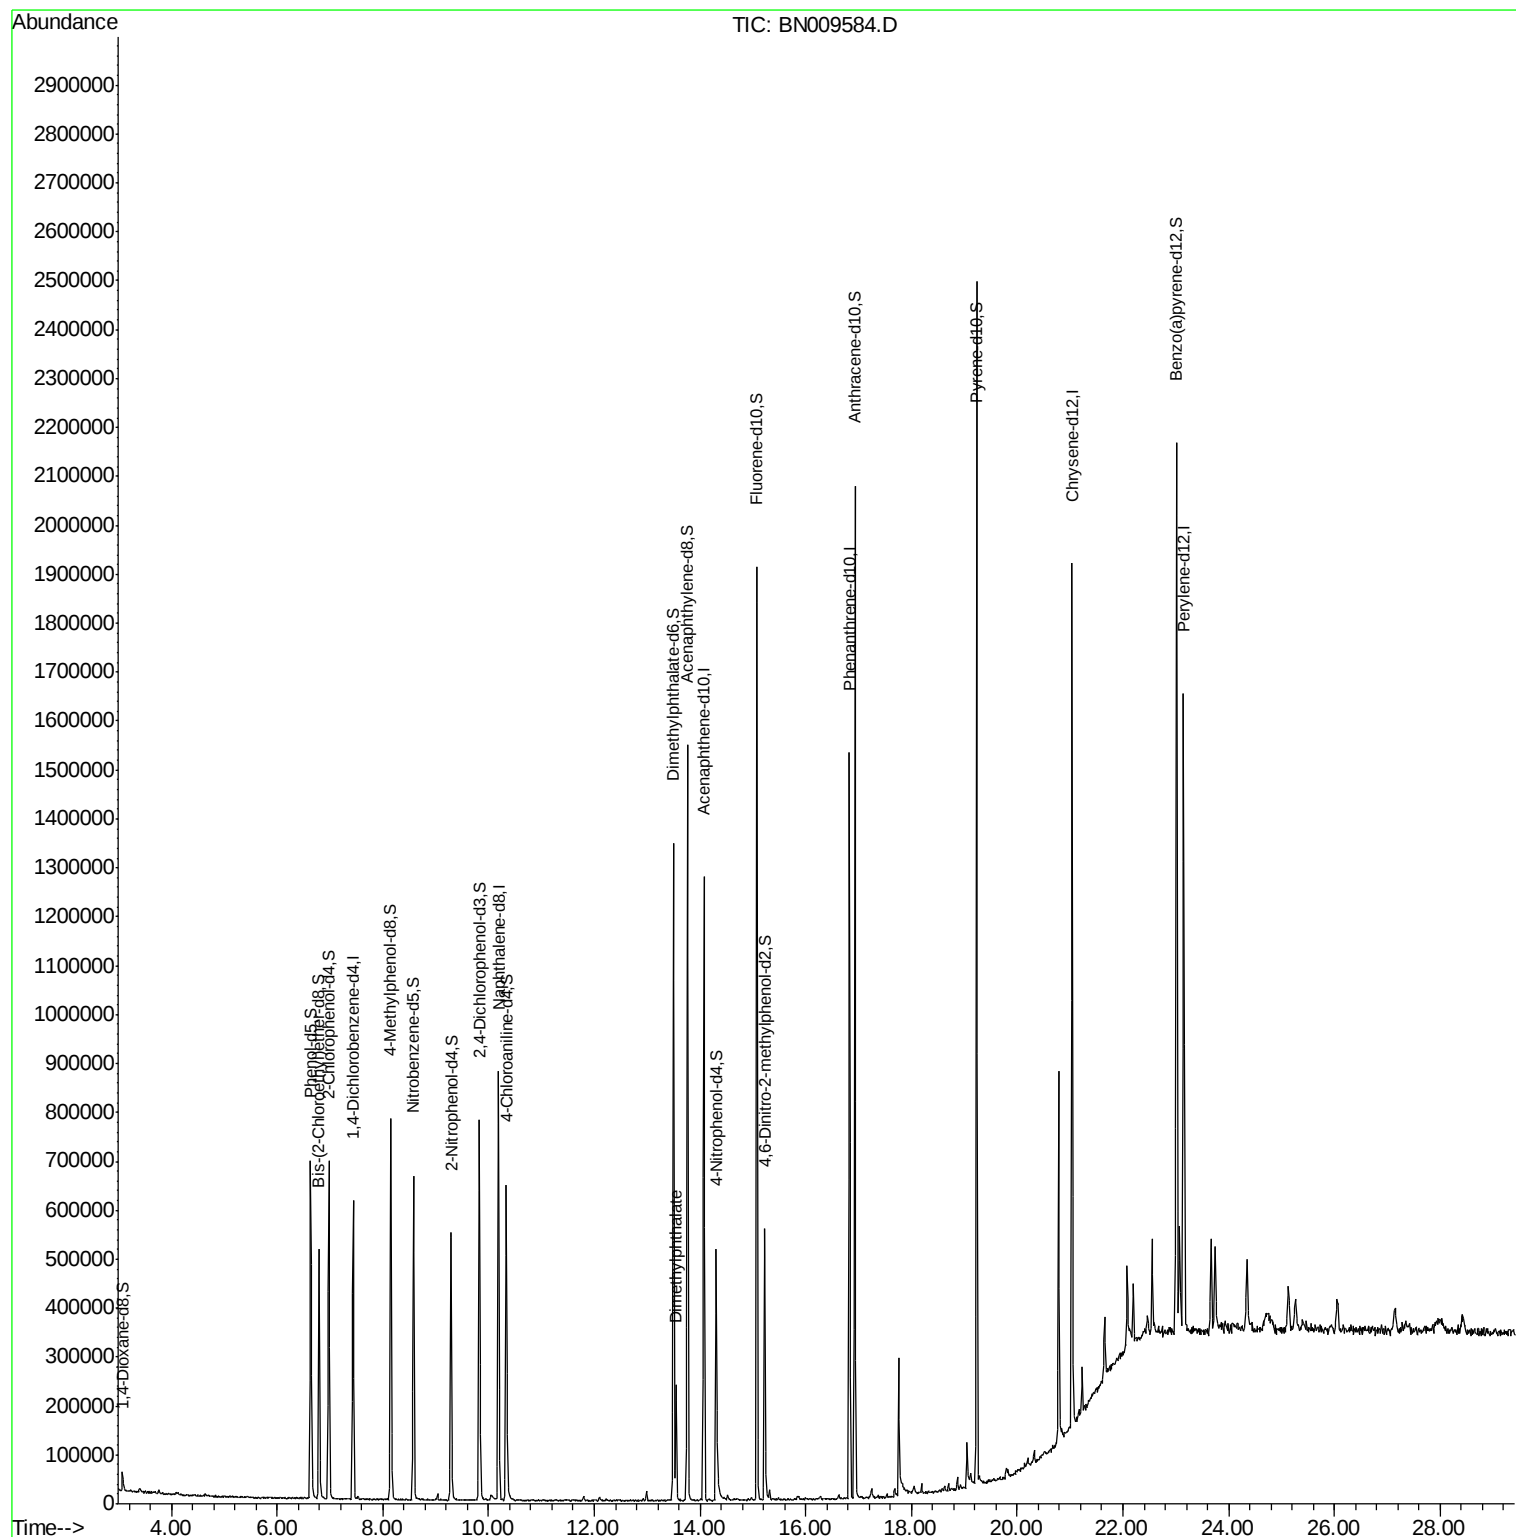

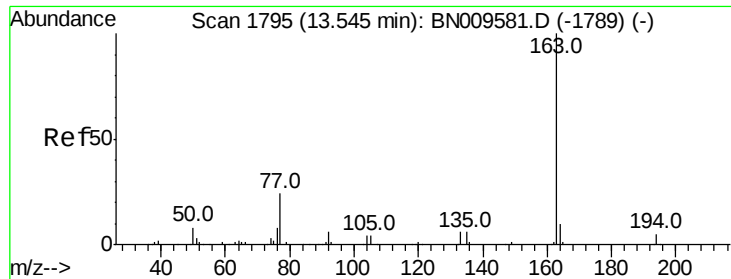

#44

Dimethylphthalate

Concen: 4.376 ng/ul

RT: 13.55 min Scan# 1795

Delta R.T. -0.01 min

Lab File: BN009584.D

Acq: 05 Feb 2020 03:40

Instrument :

BNA_N

ClientSampleId :

GAT45


Tot Ion:163 Resp: 133626

Ion Ratio Lower Upper

163 100

194 4.7 3.5 5.3

164 10.3 8.0 12.0

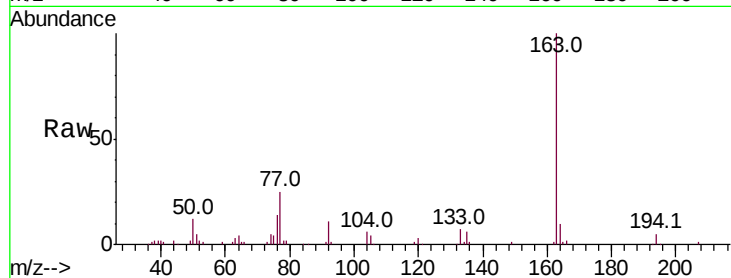

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

