

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
 Data File : BN009593.D
 Acq On : 05 Feb 2020 09:02
 Operator : CG/JU
 Sample : L1323-15
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAT53

Quant Time: Feb 05 11:22:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 16:39:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	171275	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	730785	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.07	164	468521	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.83	188	973976	20.00	ng/ul	0.00
77) Chrysene-d12	21.04	240	888340	20.00	ng/ul	0.00
85) Perylene-d12	23.16	264	941812	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	26148	6.26	ng/uL	0.00
5) Phenol-d5	6.63	99	534350	35.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	374008	37.28	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	414108	37.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	433428	36.43	ng/ul	-0.01
19) Nitrobenzene-d5	8.58	128	208723	38.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	236125	38.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.82	165	410753	36.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	579502	47.44	ng/ul	0.00
43) Dimethylphthalate-d6	13.50	166	1275604	37.29	ng/ul	0.00
46) Acenaphthylene-d8	13.76	160	1564659	37.86	ng/ul	0.00
51) 4-Nitrophenol-d4	14.30	143	206031	31.89	ng/ul	0.00
57) Fluorene-d10	15.07	176	1139133	37.88	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.22	200	181246	29.80	ng/ul	0.00
70) Anthracene-d10	16.93	188	1694103	38.28	ng/ul	0.00
78) Pyrene-d10	19.23	212	1866614	39.97	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.02	264	1883084	40.61	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.66	94	78317	4.906	ng/ul	99
44) Dimethylphthalate	13.55	163	354343	9.762	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
Data File : BN009593.D
Acq On : 05 Feb 2020 09:02
Operator : CG/JU
Sample : L1323-15
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAT53

Quant Time: Feb 05 11:22:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 16:39:56 2020
Response via : Initial Calibration

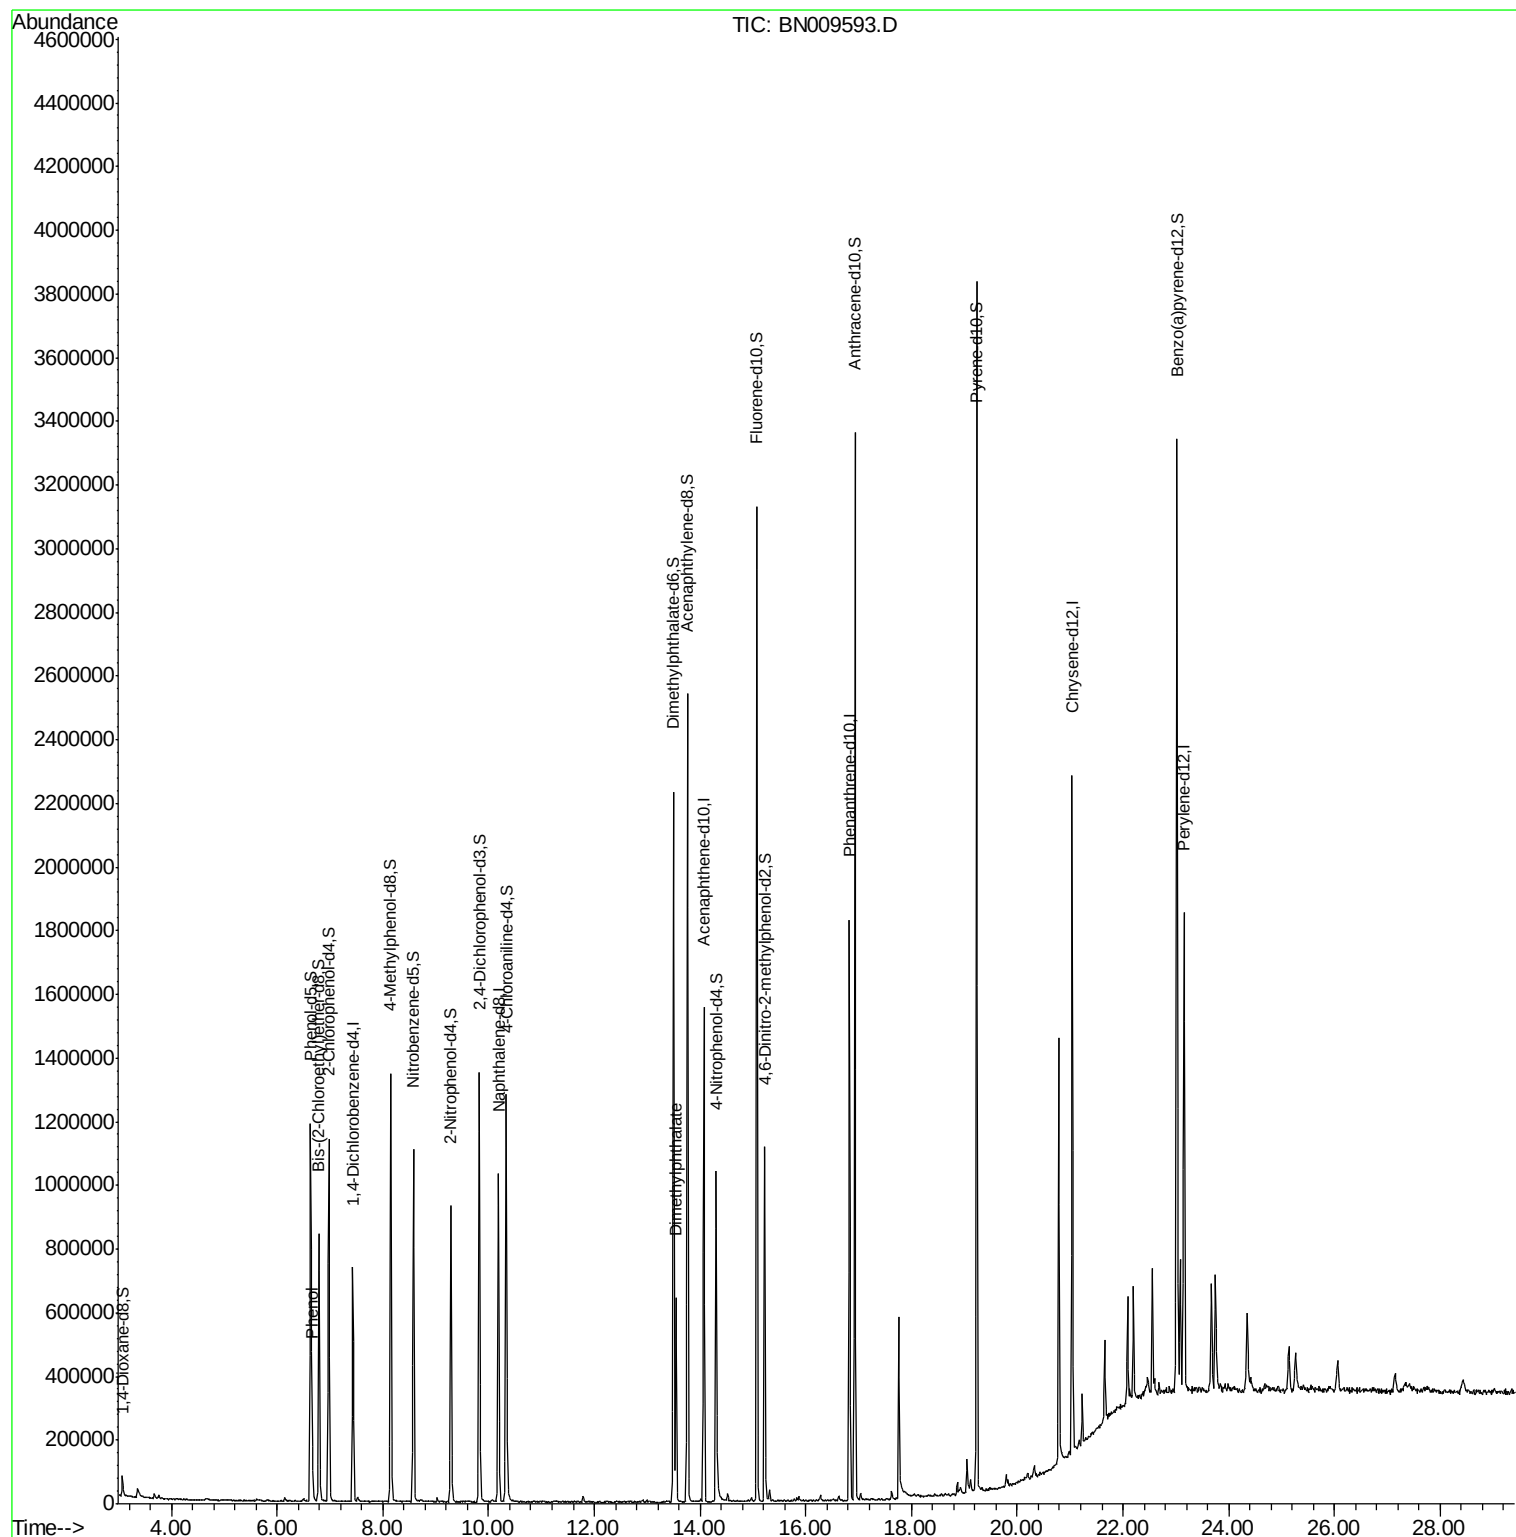

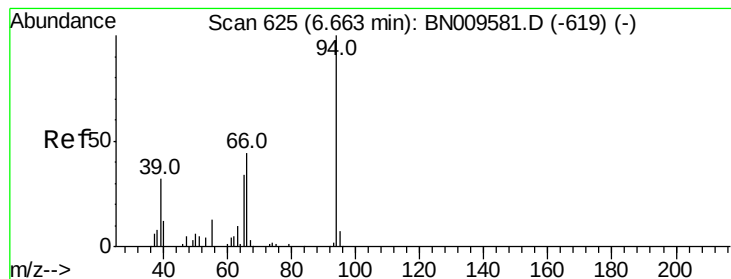





#6

Phenol

Concen: 4.906 ng/ul
 RT: 6.66 min Scan# 625
 Delta R.T. -0.01 min
 Lab File: BN009593.D
 Acq: 05 Feb 2020 09:02

Instrument :
 BNA_N
 ClientSampleId :
 GAT53

Tot Ion: 94 Resp: 78317
 Ion Ratio Lower Upper
 94 100
 65 38.3 29.8 44.6
 66 49.2 39.5 59.3

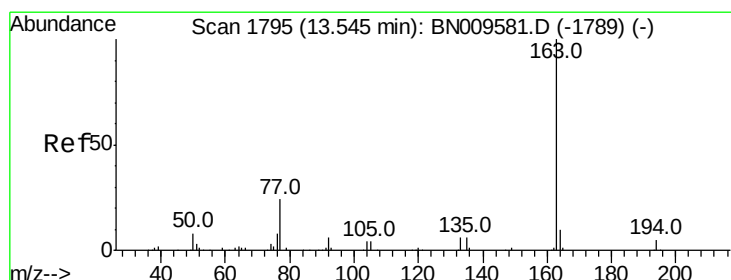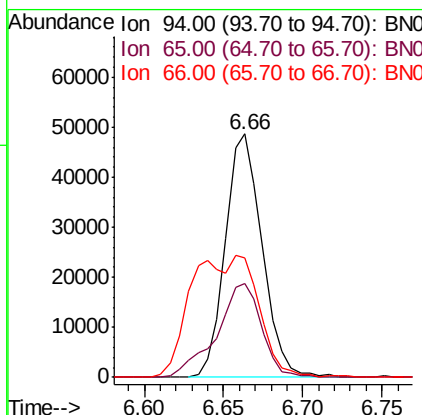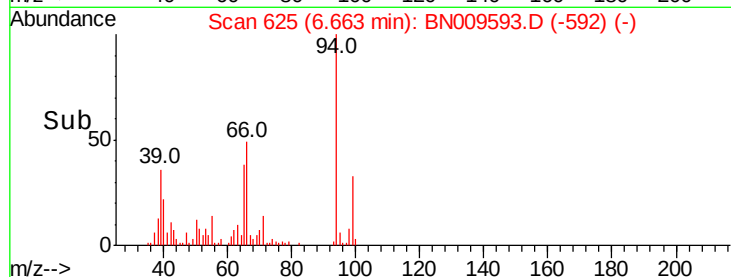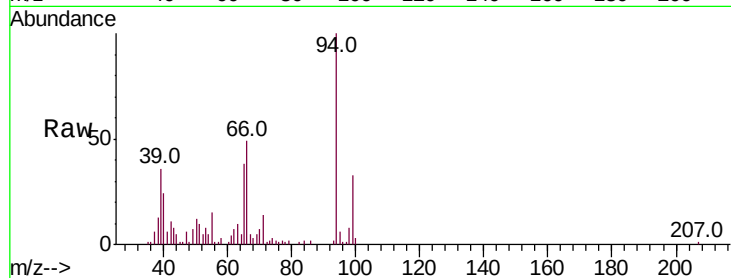

#44

Dimethylphthalate

Concen: 9.762 ng/ul
 RT: 13.55 min Scan# 1795
 Delta R.T. -0.01 min
 Lab File: BN009593.D
 Acq: 05 Feb 2020 09:02

Tgt Ion: 163 Resp: 354343
 Ion Ratio Lower Upper
 163 100
 194 4.1 3.5 5.3
 164 10.4 8.0 12.0

