

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
 Data File : BN009594.D
 Acq On : 05 Feb 2020 09:38
 Operator : CG/JU
 Sample : L1323-17
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAT55

Quant Time: Feb 05 11:50:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 03 16:39:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.44	152	153071	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	660354	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.07	164	422173	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.83	188	880321	20.00	ng/ul	0.00
77) Chrysene-d12	21.04	240	788351	20.00	ng/ul	0.00
85) Perylene-d12	23.15	264	865042	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	16752	4.49	ng/uL	0.00
5) Phenol-d5	6.63	99	350997	26.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.79	67	244945	27.32	ng/ul	0.00
9) 2-Chlorophenol-d4	6.98	132	274950	27.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	274140	25.79	ng/ul	-0.01
19) Nitrobenzene-d5	8.58	128	133957	27.28	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.29	143	150251	27.42	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.82	165	271459	26.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	289474	26.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.50	166	809485	26.27	ng/ul	0.00
46) Acenaphthylene-d8	13.76	160	1009534	27.11	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.30	143	122414	21.03	ng/ul	0.00
57) Fluorene-d10	15.07	176	752126	27.75	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.22	200	97943	17.81	ng/ul	0.00
70) Anthracene-d10	16.93	188	1102643	27.57	ng/ul	0.00
78) Pyrene-d10	19.23	212	1211536	29.23	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.02	264	1163598	27.32	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.55	163	126313	3.862	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN020320\
Data File : BN009594.D
Acq On : 05 Feb 2020 09:38
Operator : CG/JU
Sample : L1323-17
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAT55

Quant Time: Feb 05 11:50:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 03 16:39:56 2020
Response via : Initial Calibration

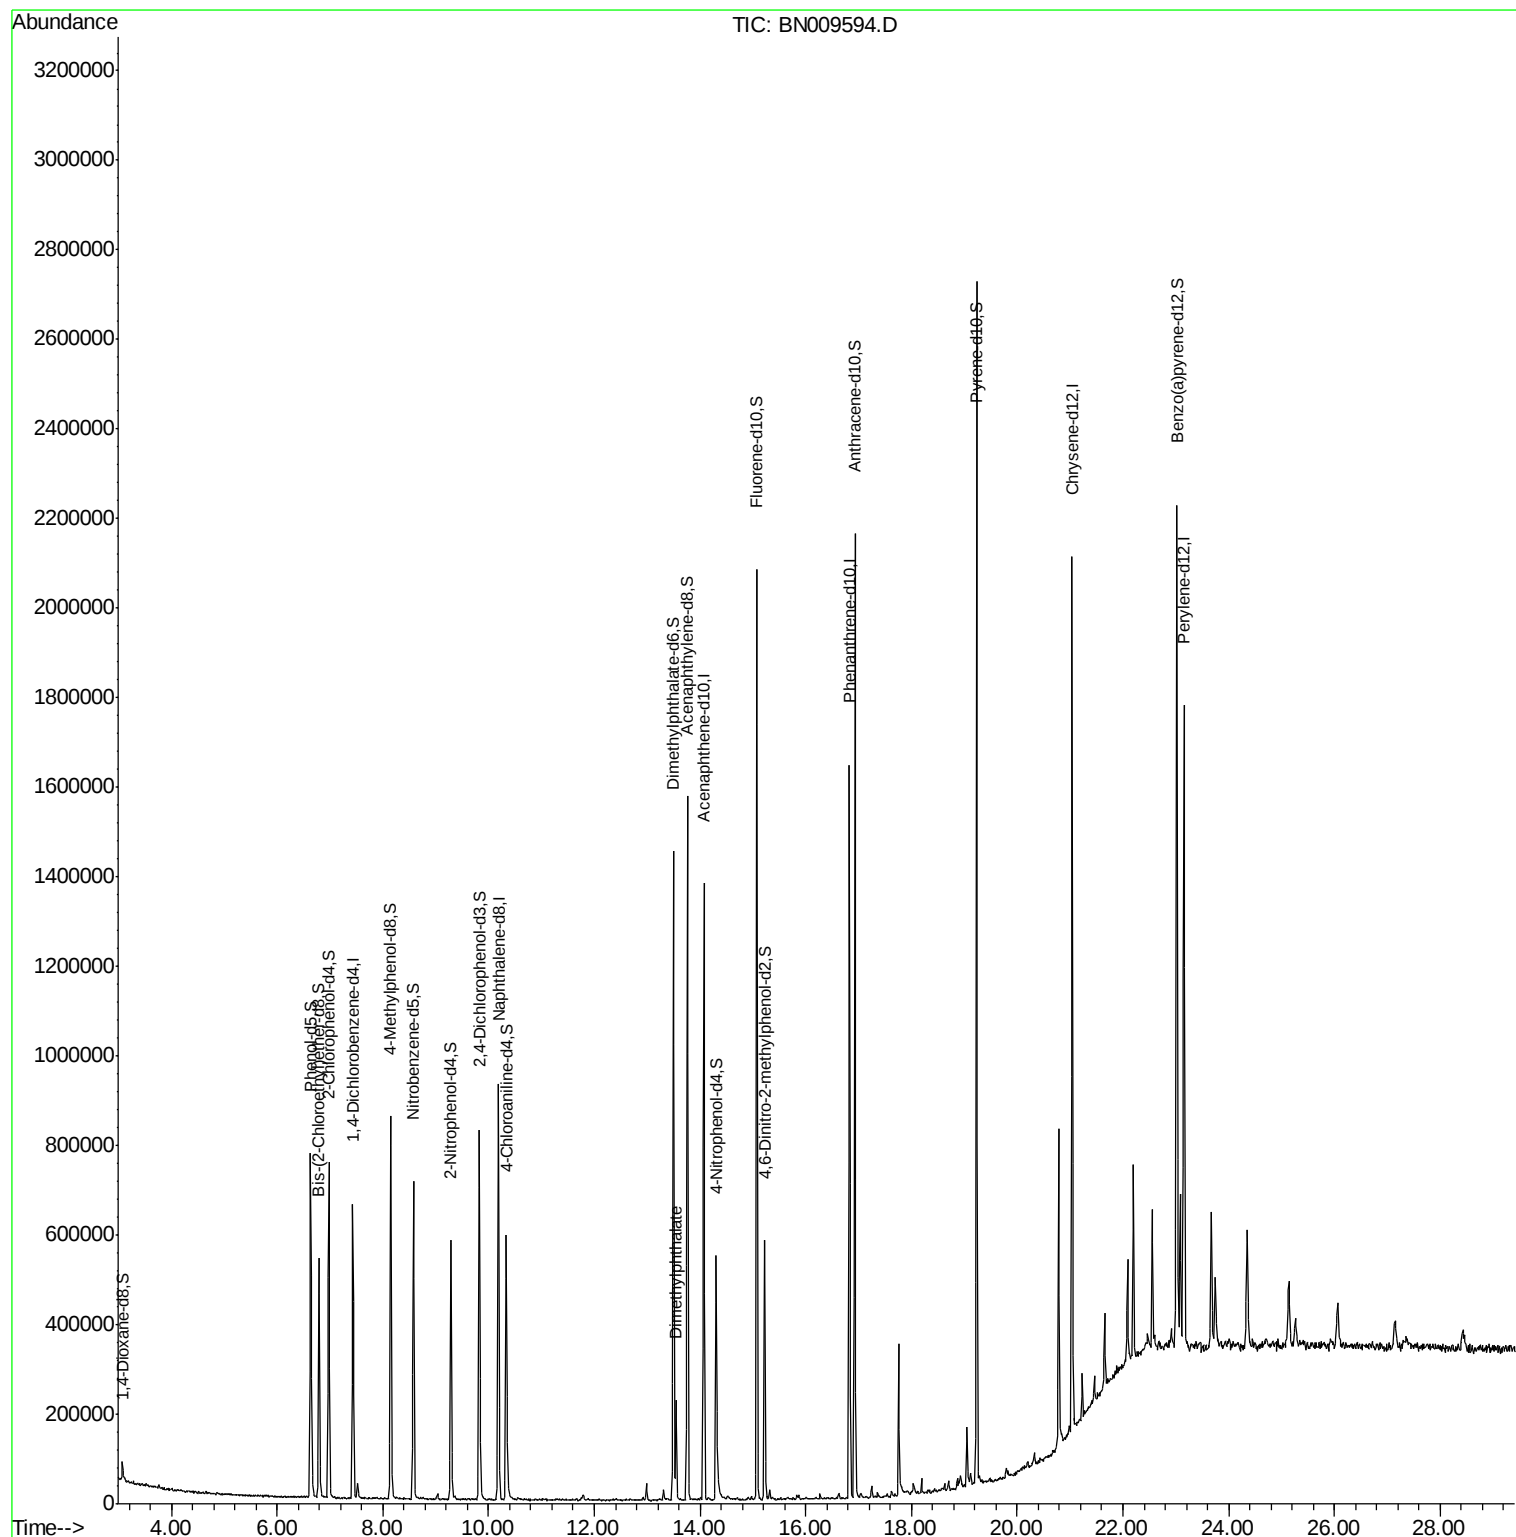

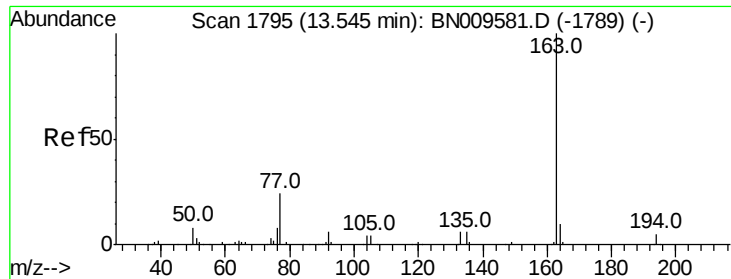

#44

Dimethylphthalate

Concen: 3.862 ng/ul

RT: 13.55 min Scan# 1795

Delta R.T. -0.01 min

Lab File: BN009594.D

Acq: 05 Feb 2020 09:38

Instrument :

BNA_N

ClientSampleId :

GAT55


Tot Ion:163 Resp: 126313

Ion Ratio Lower Upper

163 100

194 3.6 3.5 5.3

164 9.9 8.0 12.0

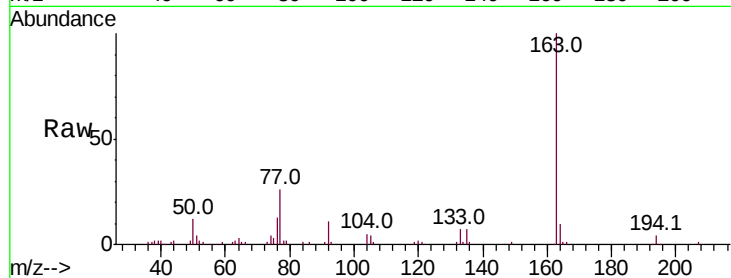

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

