

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
 Data File : BN013553.D
 Acq On : 03 Feb 2021 13:09
 Operator : CG/JU
 Sample : M1274-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Quant Time: Feb 03 13:39:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 03 12:01:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	320322	20.00	ng/ul	0.00
18) Naphthalene-d8	10.316	136	1329086	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.193	164	779852	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.945	188	1622727	20.00	ng/ul	0.00
78) Chrysene-d12	21.145	240	1646958	20.00	ng/ul	0.00
86) Perylene-d12	23.316	264	1653213	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	36292	4.87	ng/uL	0.00
5) Phenol-d5	6.734	99	154829	6.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.905	67	410481	29.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.093	132	494920	24.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.258	113	292883	15.46	ng/ul	0.00
19) Nitrobenzene-d5	8.699	128	279787	31.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.410	143	292083	31.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.940	165	545779	29.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.457	131	34000	1.54	ng/ul	0.00
44) Dimethylphthalate-d6	13.610	166	1815055	34.74	ng/ul	0.00
47) Acenaphthylene-d8	13.881	160	2384222	34.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.392	143	56229	5.55	ng/ul	0.00
58) Fluorene-d10	15.192	176	1666606	36.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.310	200	238491	27.48	ng/ul	0.00
71) Anthracene-d10	17.039	188	2619226	37.23	ng/ul	0.00
79) Pyrene-d10	19.345	212	2861168	36.56	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.180	264	3159809	39.14	ng/ul	0.00
Target Compounds						Qvalue
45) Dimethylphthalate	13.657	163	119998	2.21	ng/ul	100
69) Pentachlorophenol	16.598	266	40465	4.00	ng/ul	94
84) Bis(2-ethylhexyl)phtha...	21.086	149	106082	1.84	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
Data File : BN013553.D
Acq On : 03 Feb 2021 13:09
Operator : CG/JU
Sample : M1274-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD4

Quant Time: Feb 03 13:39:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 03 12:01:22 2021
Response via : Initial Calibration




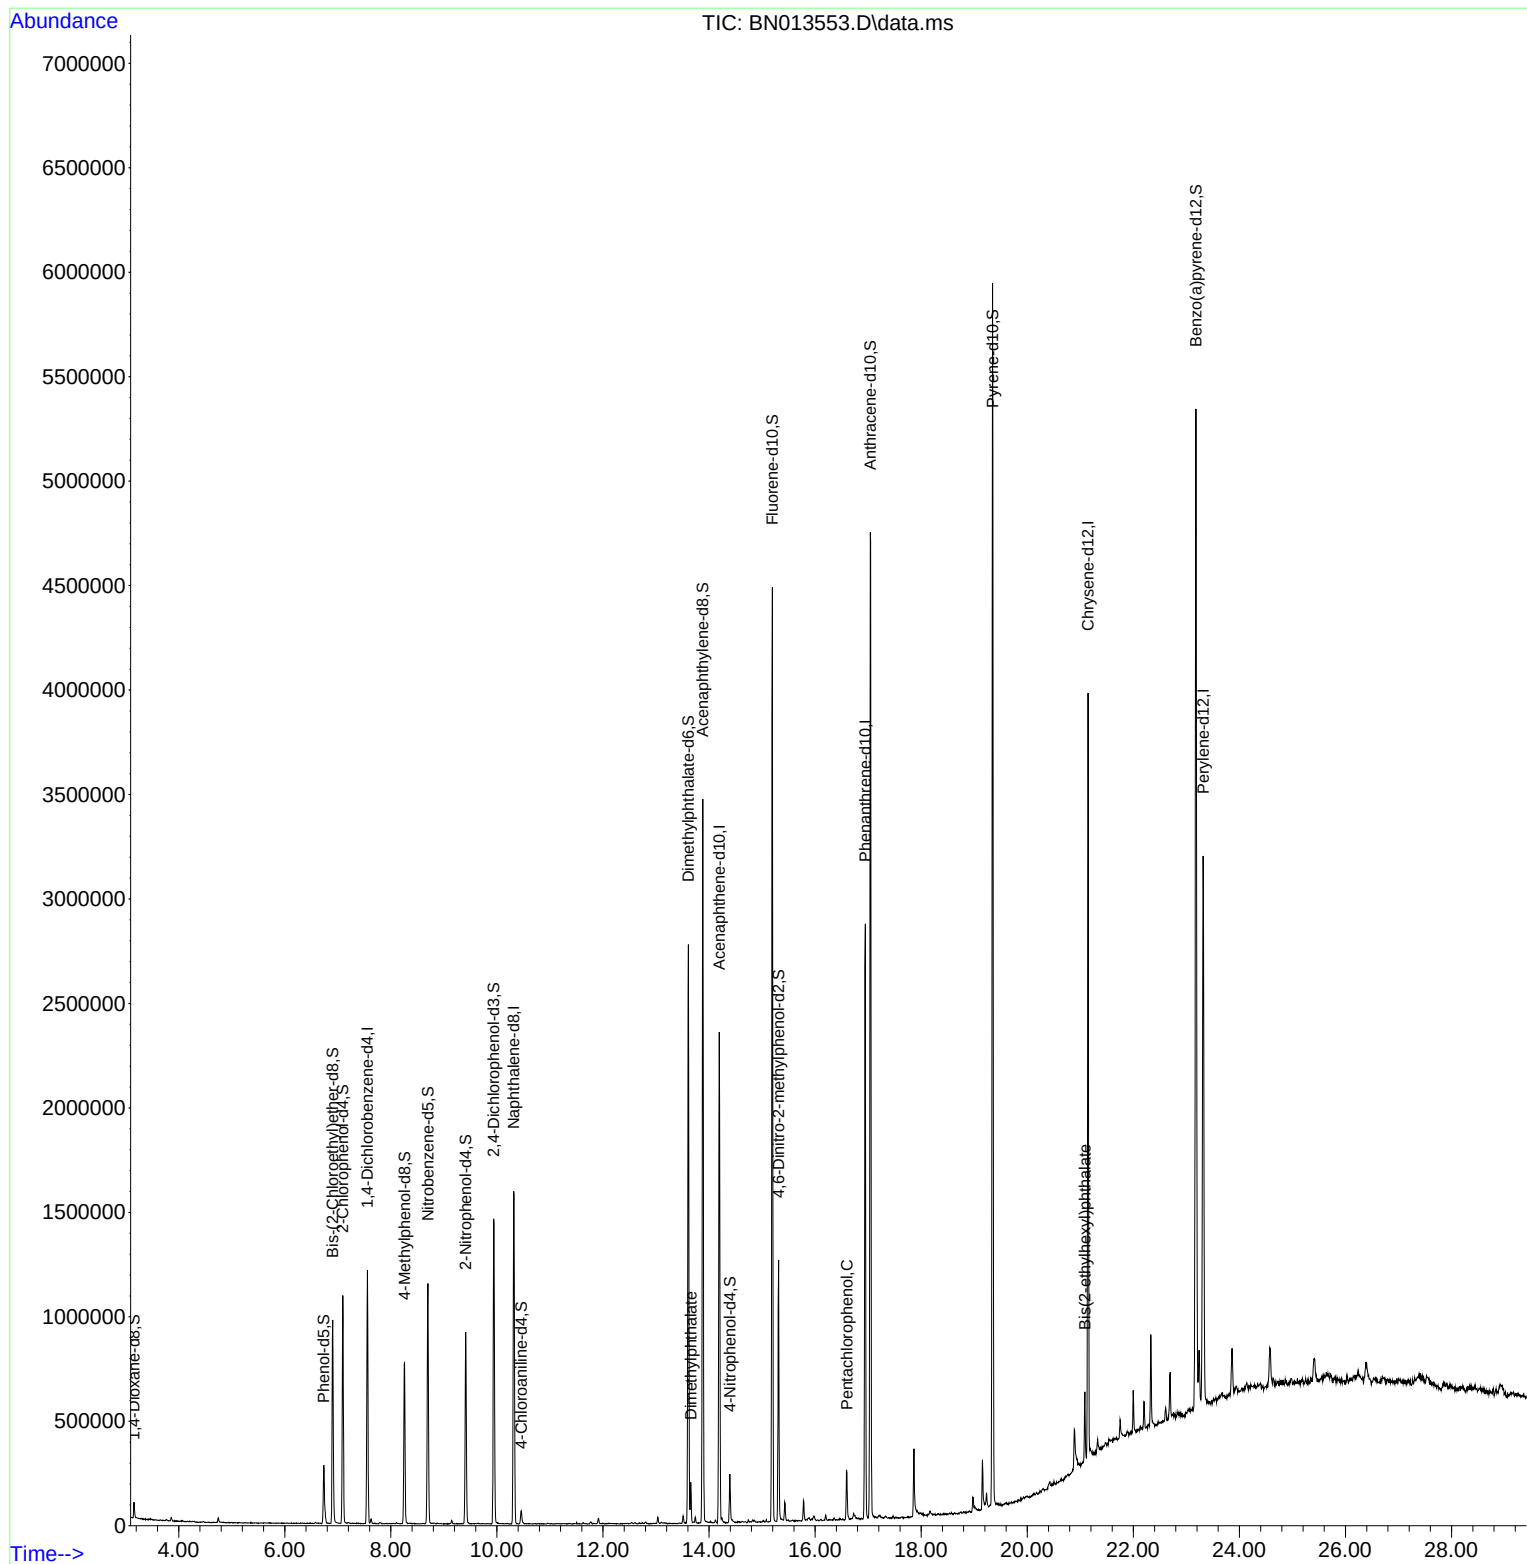


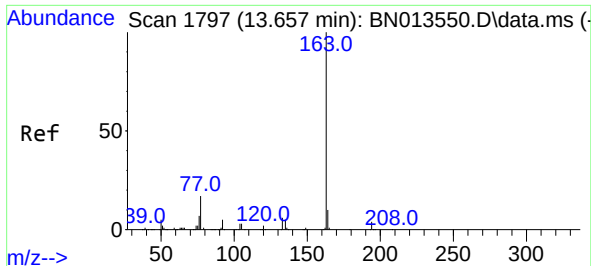

#45
Dimethylphthalate
Concen: 2.21 ng/ul
RT: 13.657 min Scan# 1797
Delta R.T. -0.000 min
Lab File: BN013553.D
Acq: 03 Feb 2021 13:09




Instrument :
BNA_N
ClientSampleId :
C0AD4


Tgt Ion:163 Resp: 119998
Ion Ratio Lower Upper
163 100
194 4.2 3.4 5.0
164 10.3 8.3 12.5

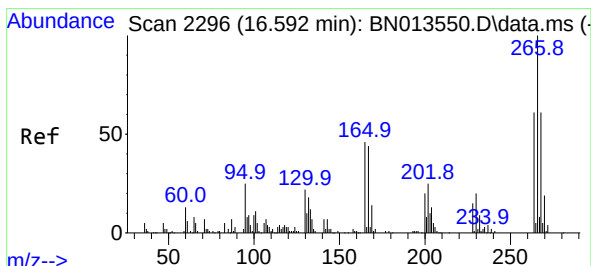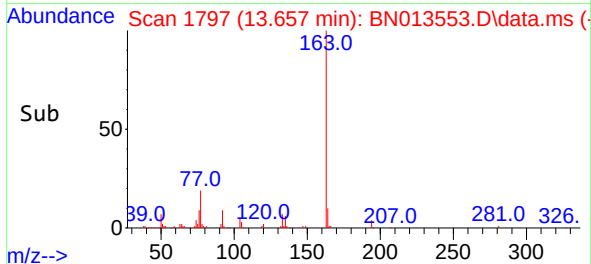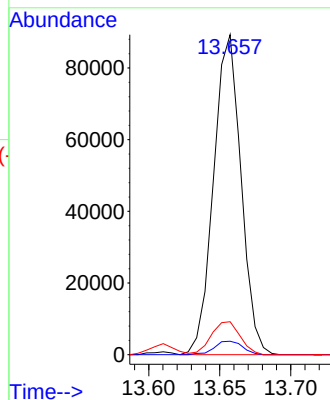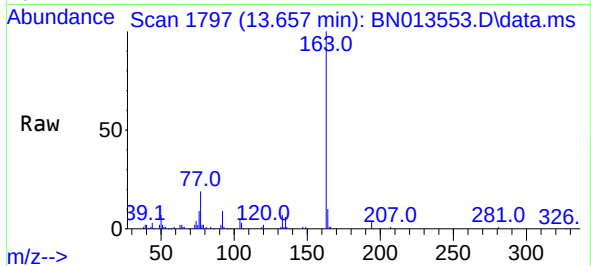

#69
Pentachlorophenol
Concen: 4.00 ng/ul
RT: 16.598 min Scan# 2297
Delta R.T. 0.006 min
Lab File: BN013553.D
Acq: 03 Feb 2021 13:09

Tgt Ion:266 Resp: 40465
Ion Ratio Lower Upper
266 100
264 66.6 47.7 71.5
268 56.9 47.5 71.3

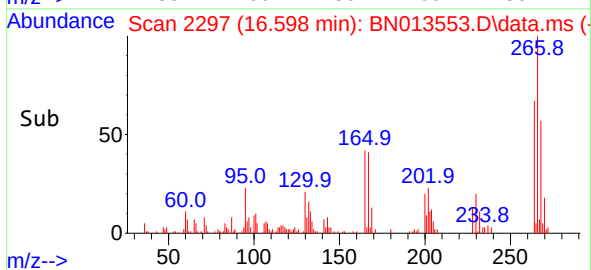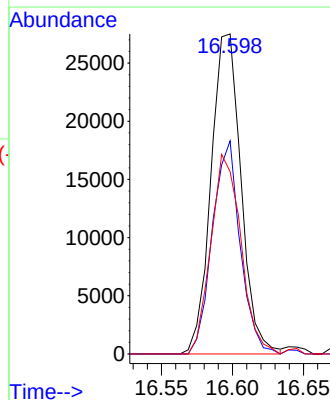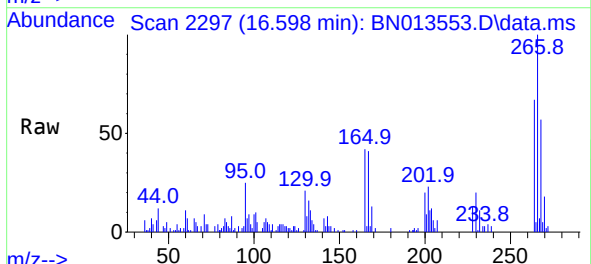

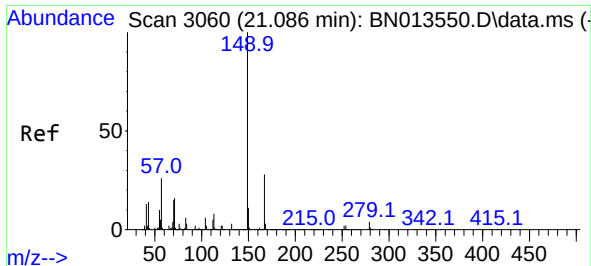

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 1.84 ng/ul
 RT: 21.086 min Scan# 3060
 Delta R.T. -0.000 min
 Lab File: BN013553.D
 Acq: 03 Feb 2021 13:09

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Tgt Ion:149 Resp: 106082

Ion	Ratio	Lower	Upper
149	100		
167	29.1	22.3	33.5
279	4.1	3.4	5.2

