

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
 Data File : BN013554.D
 Acq On : 03 Feb 2021 13:45
 Operator : CG/JU
 Sample : M1299-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CAA16

Quant Time: Feb 03 14:22:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 03 12:01:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	289337	20.00	ng/ul	0.00
18) Naphthalene-d8	10.316	136	1212068	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.193	164	737025	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.945	188	1520648	20.00	ng/ul	0.00
78) Chrysene-d12	21.145	240	1478342	20.00	ng/ul	0.00
86) Perylene-d12	23.316	264	1572766	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	36661	5.44	ng/uL	0.00
5) Phenol-d5	6.734	99	190073	8.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.905	67	459692	37.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.093	132	564968	31.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.258	113	341624	19.97	ng/ul	0.00
19) Nitrobenzene-d5	8.699	128	319148	38.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.410	143	343177	40.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.940	165	602358	35.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.457	131	49651	2.47	ng/ul	0.00
44) Dimethylphthalate-d6	13.610	166	1972913	39.96	ng/ul	0.00
47) Acenaphthylene-d8	13.881	160	2527973	38.96	ng/ul	0.00
52) 4-Nitrophenol-d4	14.393	143	62693	6.55	ng/ul	0.00
58) Fluorene-d10	15.192	176	1753541	40.53	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.310	200	262693	32.30	ng/ul	0.00
71) Anthracene-d10	17.039	188	2804328	42.53	ng/ul	0.00
79) Pyrene-d10	19.345	212	3087483	43.95	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.180	264	3268945	42.57	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.657	163	75199	1.47	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
Data File : BN013554.D
Acq On : 03 Feb 2021 13:45
Operator : CG/JU
Sample : M1299-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CAA16

Quant Time: Feb 03 14:22:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 03 12:01:22 2021
Response via : Initial Calibration

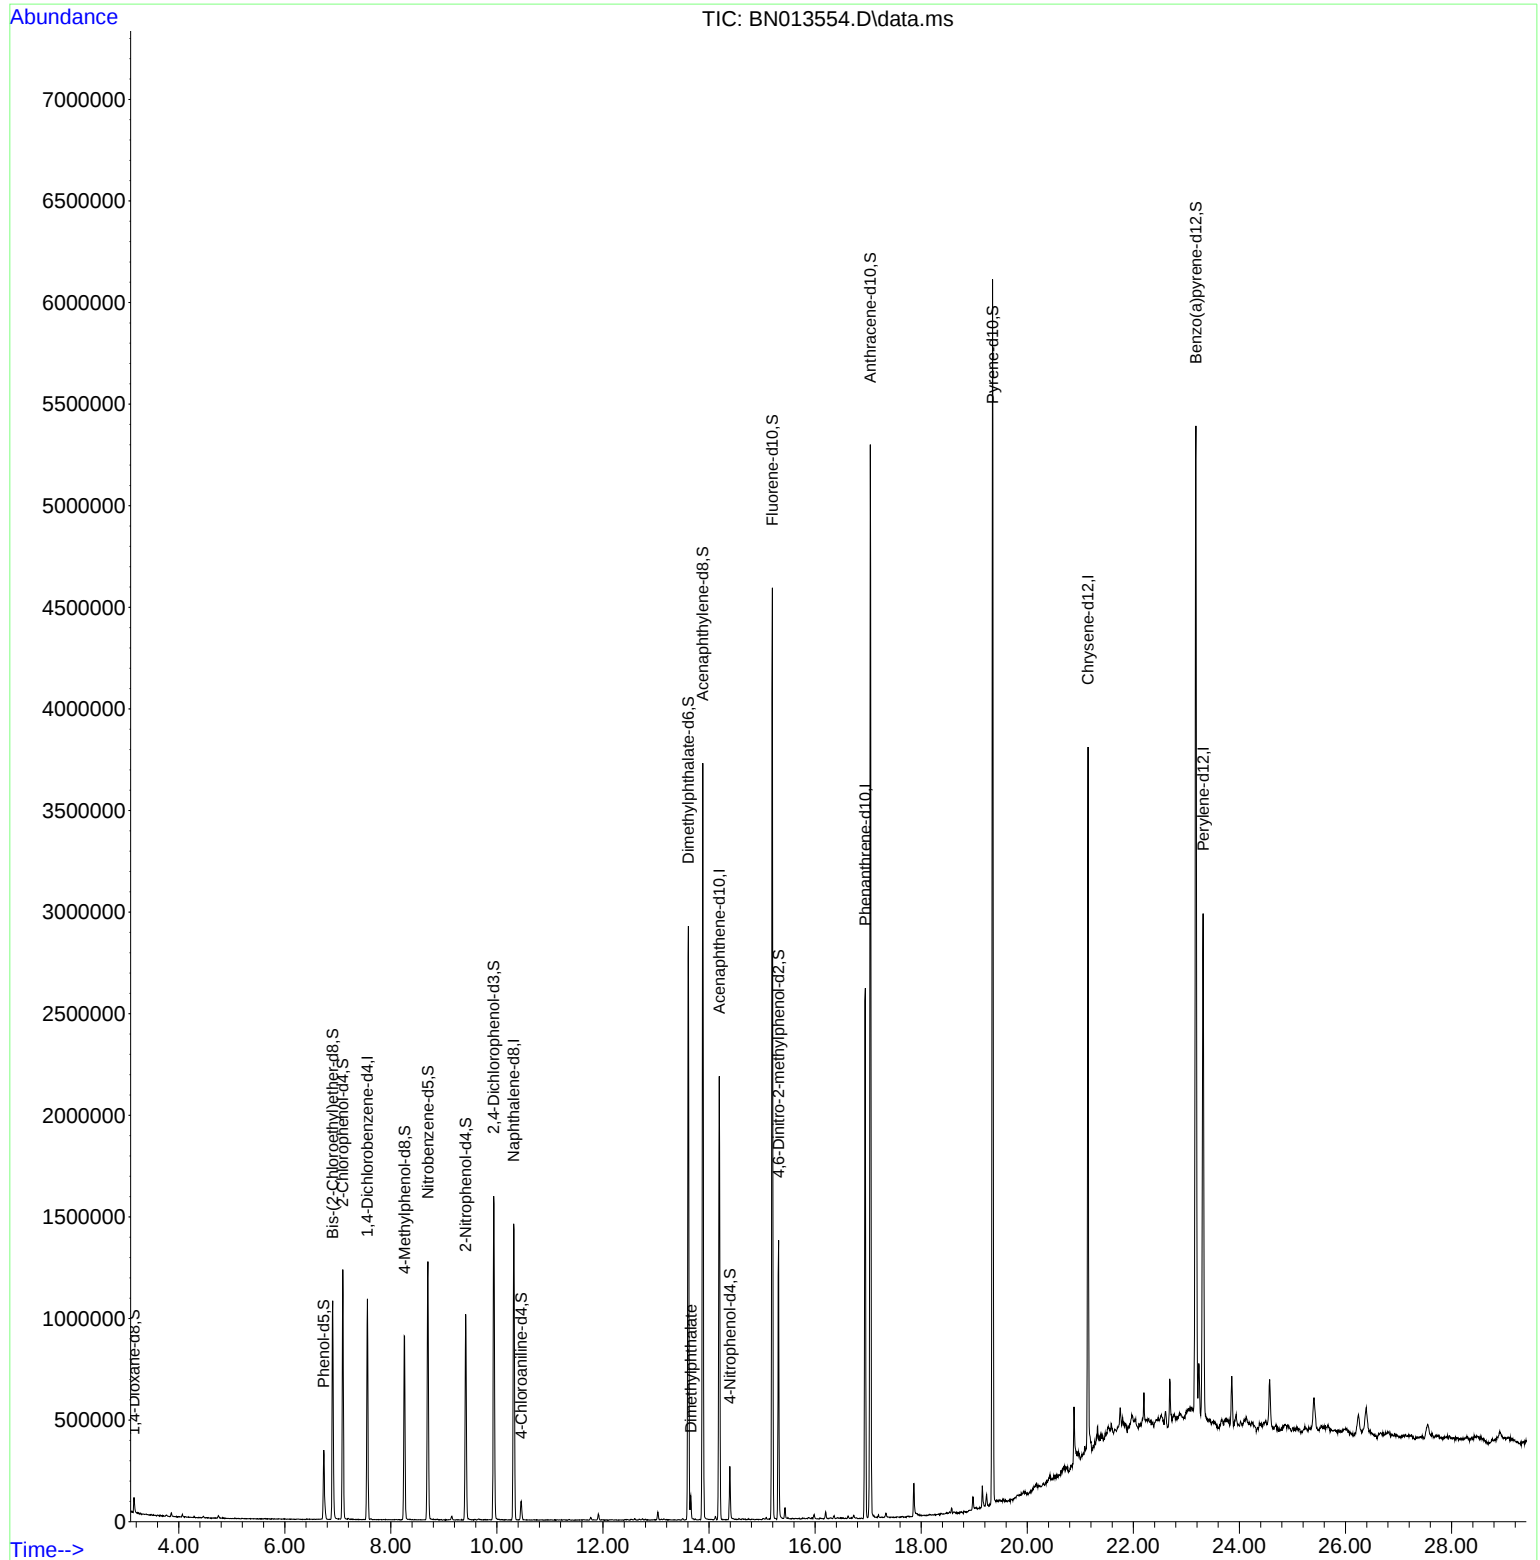

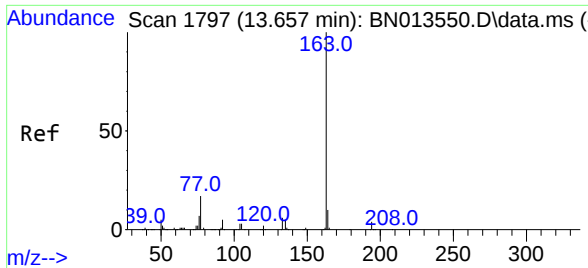

#45
 Dimethylphthalate
 Concen: 1.47 ng/ul
 RT: 13.657 min Scan# 1797
 Delta R.T. 0.000 min
 Lab File: BN013554.D
 Acq: 03 Feb 2021 13:45

Instrument :
 BNA_N
 ClientSampleId :
 CAA16

Tgt Ion:163	Resp:	75199
Ion	Ratio	Lower Upper
163	100	
194	4.3	3.4 5.0
164	10.2	8.3 12.5

