

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
 Data File : BN013555.D
 Acq On : 03 Feb 2021 14:21
 Operator : CG/JU
 Sample : M1299-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0A50

Quant Time: Feb 03 14:50:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 03 12:01:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.557	152	281362	20.00	ng/ul	0.00
18) Naphthalene-d8	10.322	136	1198805	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.192	164	715197	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.945	188	1472286	20.00	ng/ul	0.00
78) Chrysene-d12	21.145	240	1463893	20.00	ng/ul	0.00
86) Perylene-d12	23.315	264	1497543	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	33574	5.13	ng/uL	0.00
5) Phenol-d5	6.734	99	152761	7.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.904	67	378286	31.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.093	132	470467	26.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.251	113	279392	16.79	ng/ul	0.00
19) Nitrobenzene-d5	8.699	128	268248	33.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.410	143	285357	34.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.940	165	496793	29.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.457	131	46252	2.32	ng/ul	0.00
44) Dimethylphthalate-d6	13.610	166	1725739	36.02	ng/ul	0.00
47) Acenaphthylene-d8	13.881	160	2177189	34.58	ng/ul	0.00
52) 4-Nitrophenol-d4	14.392	143	54323	5.85	ng/ul	0.00
58) Fluorene-d10	15.192	176	1521892	36.25	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.310	200	238057	30.23	ng/ul	0.00
71) Anthracene-d10	17.039	188	2531341	39.66	ng/ul	0.00
79) Pyrene-d10	19.345	212	2759861	39.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.180	264	2960930	40.49	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.651	163	97444	1.96	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
Data File : BN013555.D
Acq On : 03 Feb 2021 14:21
Operator : CG/JU
Sample : M1299-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0A50

Quant Time: Feb 03 14:50:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 03 12:01:22 2021
Response via : Initial Calibration

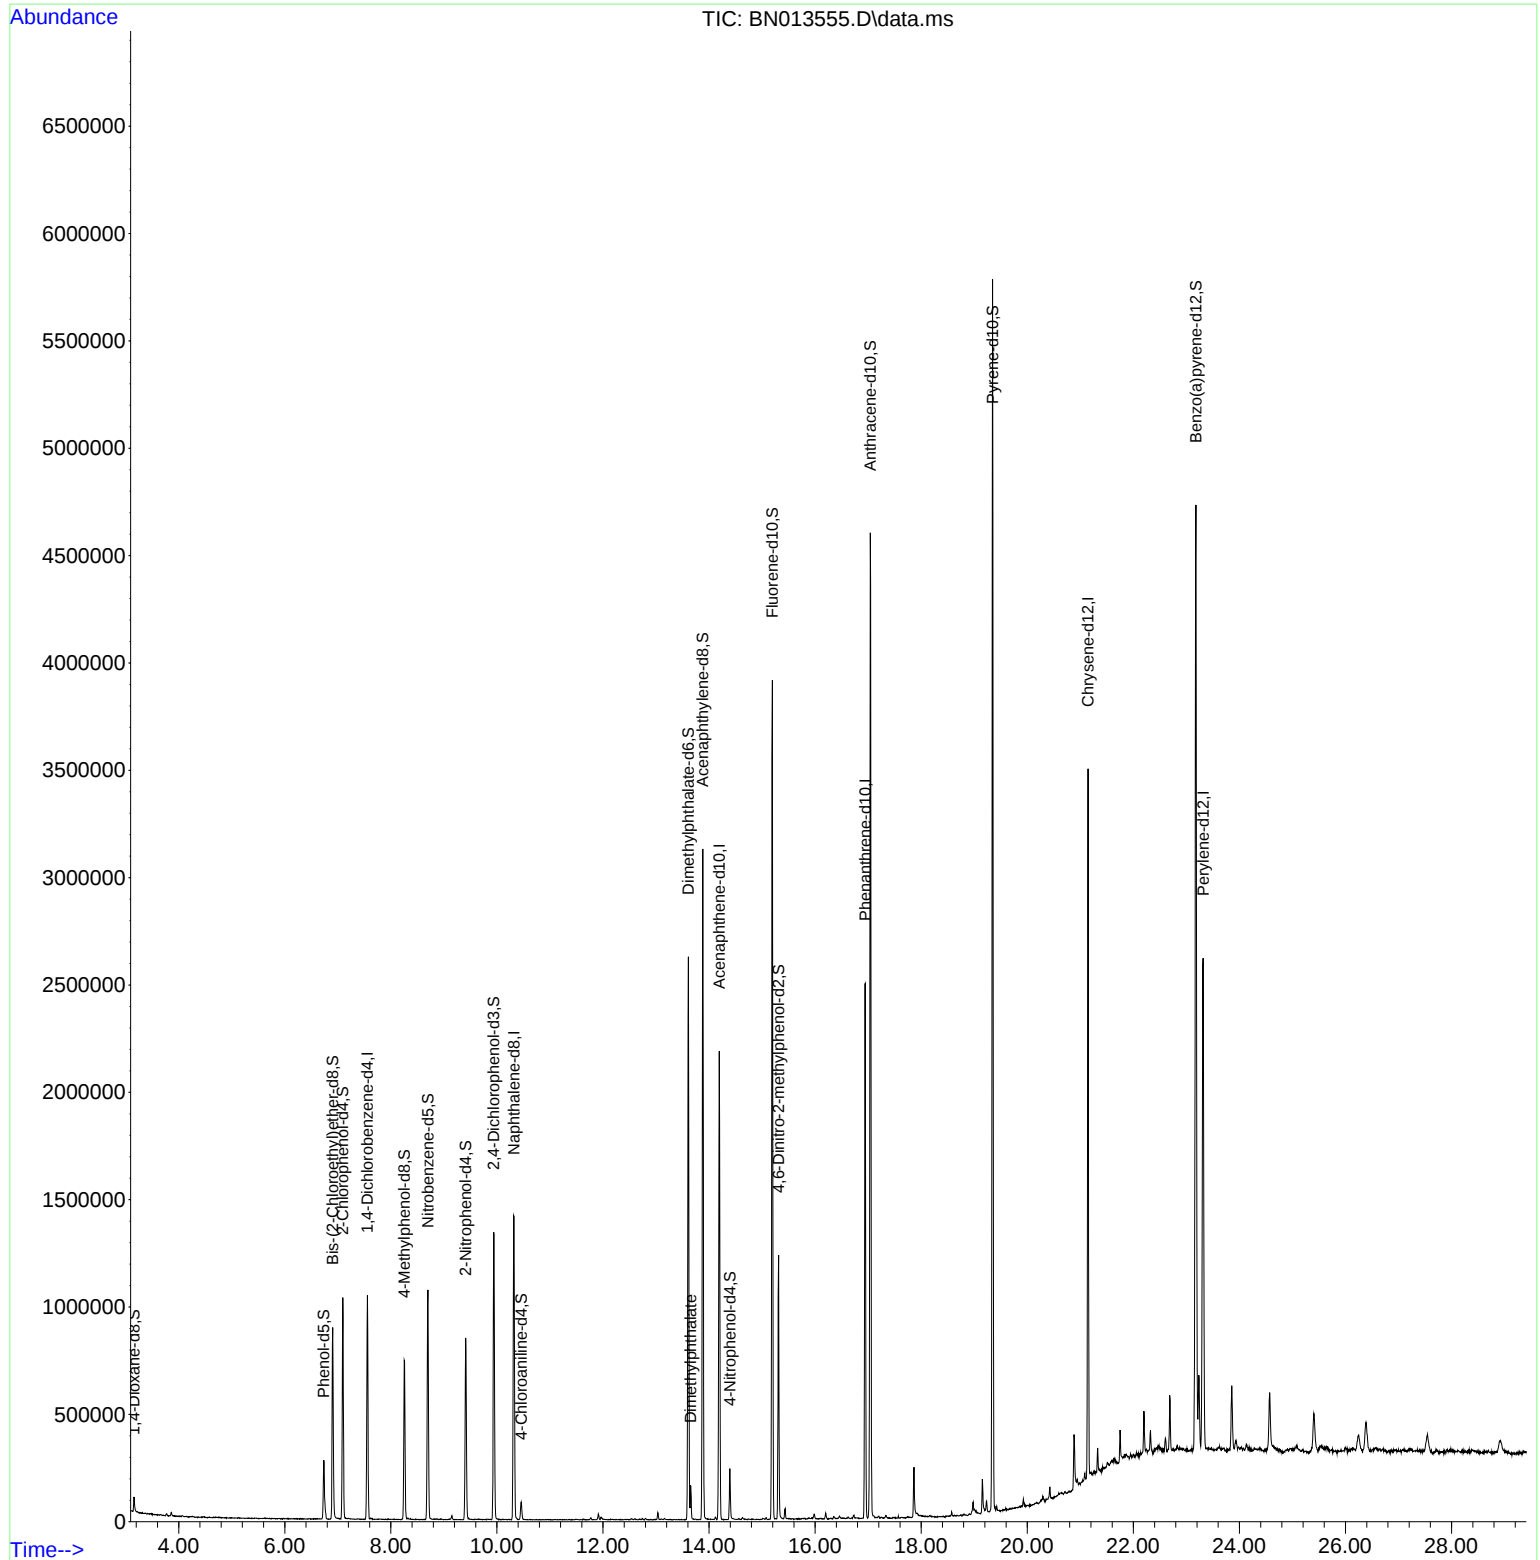

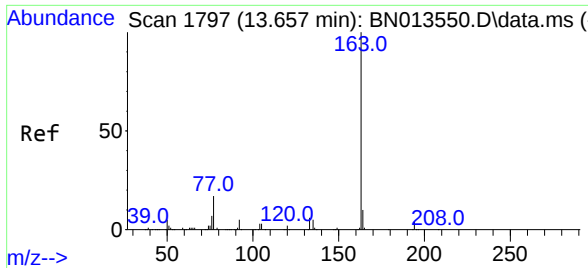

#45
Dimethylphthalate
Concen: 1.96 ng/ul
RT: 13.651 min Scan# 1796
Delta R.T. -0.006 min
Lab File: BN013555.D
Acq: 03 Feb 2021 14:21

Instrument :
BNA_N
ClientSampleId :
C0A50

Tgt Ion:163 Resp: 97444
Ion Ratio Lower Upper
163 100
194 4.3 3.4 5.0
164 10.1 8.3 12.5

