

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
 Data File : BN013558.D
 Acq On : 03 Feb 2021 16:09
 Operator : CG/JU
 Sample : M1299-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Quant Time: Feb 03 16:42:43 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 03 12:01:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.557	152	344510	20.00	ng/ul	0.00
18) Naphthalene-d8	10.316	136	1450639	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.192	164	859277	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.939	188	1757141	20.00	ng/ul	0.00
78) Chrysene-d12	21.145	240	1738965	20.00	ng/ul	0.00
86) Perylene-d12	23.315	264	1780135	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	40915	5.10	ng/uL	0.00
5) Phenol-d5	6.734	99	214628	8.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.905	67	534456	36.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.093	132	653015	30.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.252	113	398278	19.55	ng/ul	0.00
19) Nitrobenzene-d5	8.699	128	382229	38.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.410	143	417891	41.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.946	165	696694	34.76	ng/ul	0.00
29) 4-Chloroaniline-d4	10.457	131	55304	2.30	ng/ul	0.00
44) Dimethylphthalate-d6	13.610	166	2291393	39.81	ng/ul	0.00
47) Acenaphthylene-d8	13.881	160	3019671	39.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.392	143	82742	7.41	ng/ul	0.00
58) Fluorene-d10	15.192	176	2039447	40.44	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.310	200	334322	35.57	ng/ul	0.00
71) Anthracene-d10	17.039	188	3316414	43.53	ng/ul	0.00
79) Pyrene-d10	19.345	212	3606606	43.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.180	264	3857540	44.38	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.657	163	101562	1.70	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
Data File : BN013558.D
Acq On : 03 Feb 2021 16:09
Operator : CG/JU
Sample : M1299-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA5

Quant Time: Feb 03 16:42:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 03 12:01:22 2021
Response via : Initial Calibration

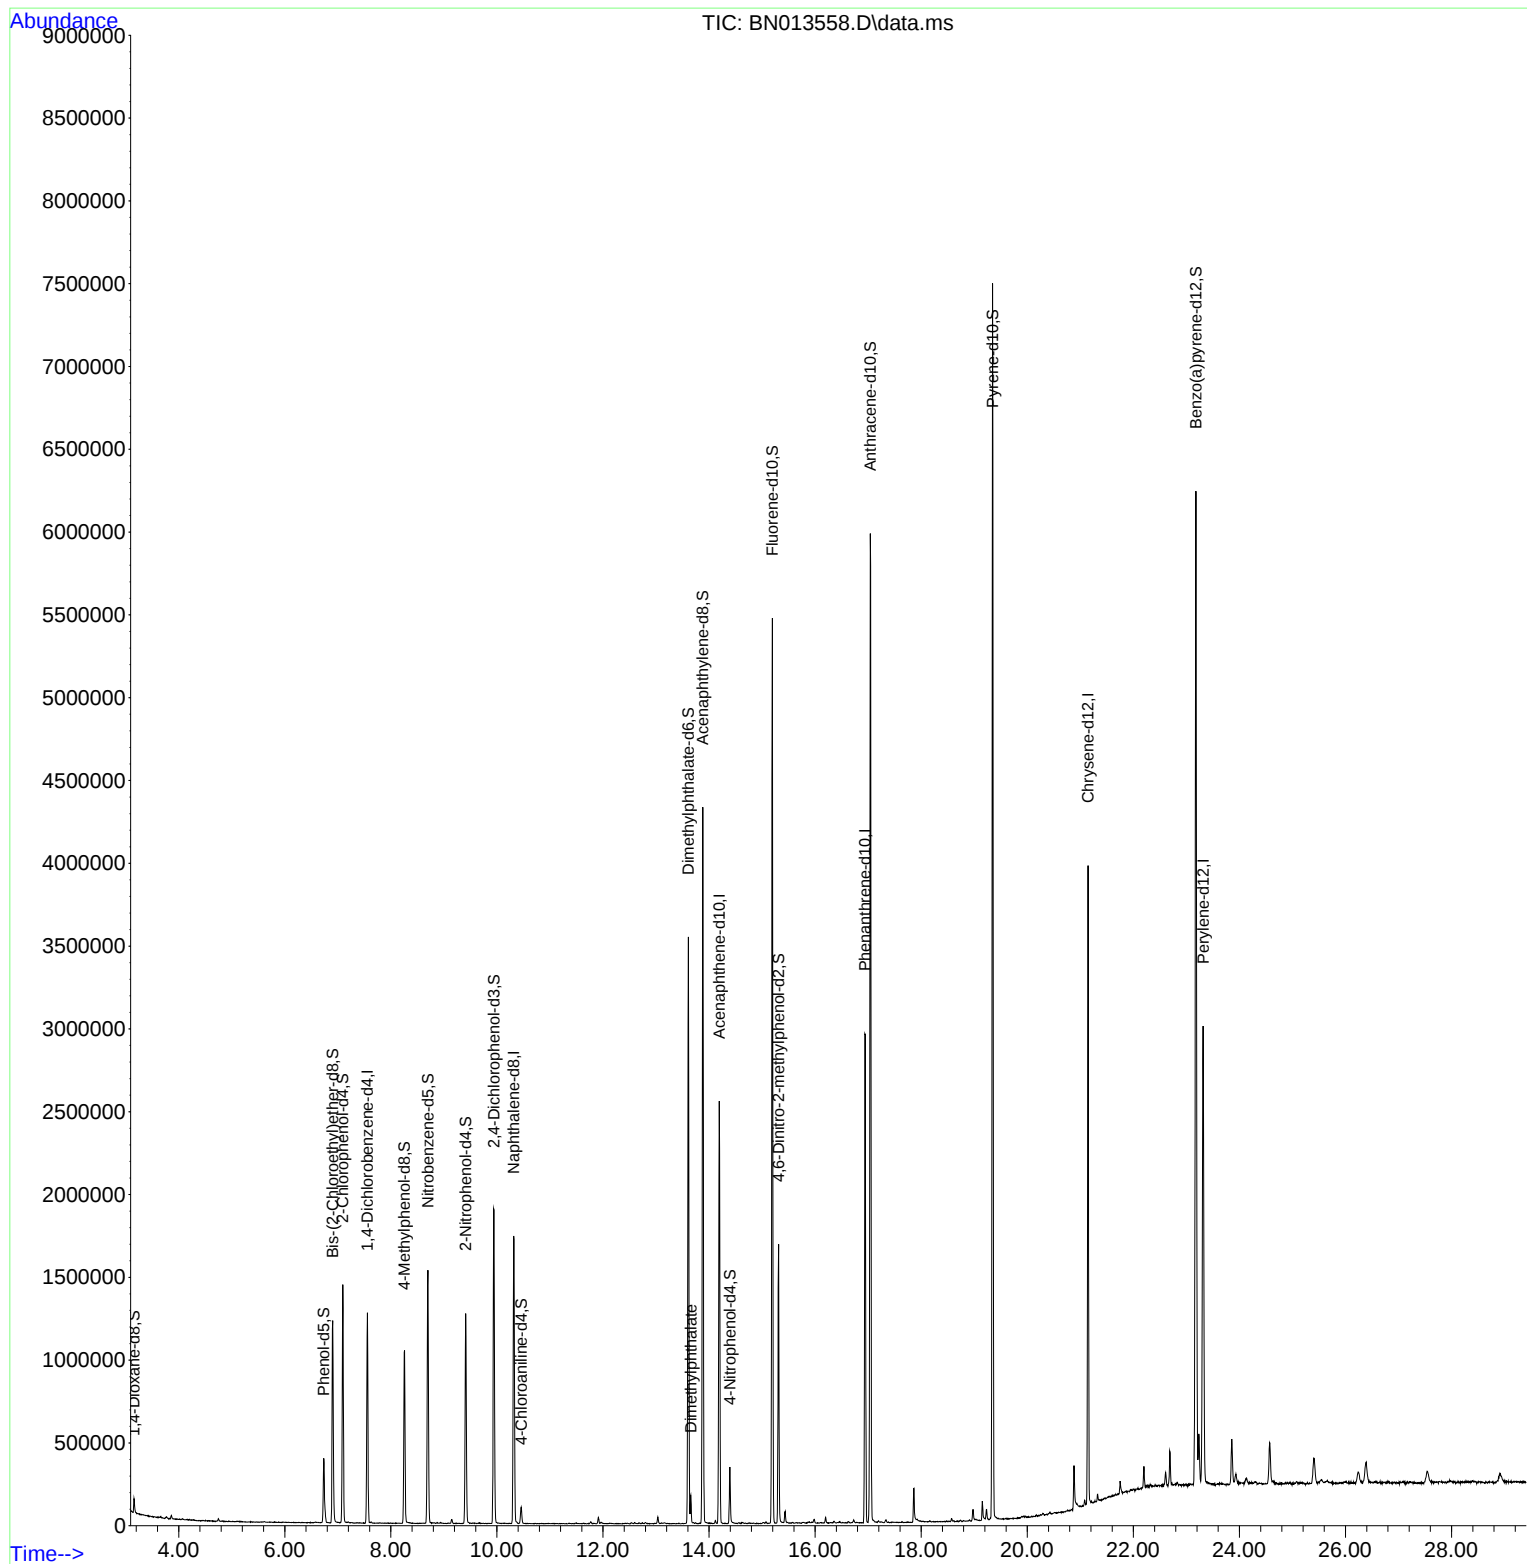

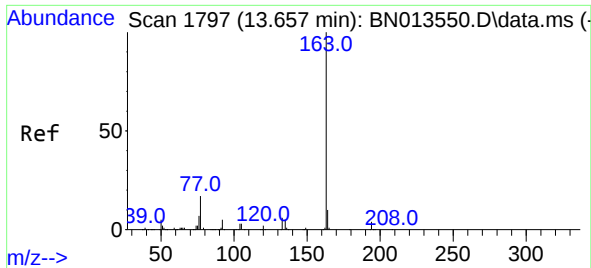

#45
Dimethylphthalate
Concen: 1.70 ng/ul
RT: 13.657 min Scan# 1797
Delta R.T. -0.000 min
Lab File: BN013558.D
Acq: 03 Feb 2021 16:09

Instrument :
BNA_N
ClientSampleId :
C0AA5

Tgt Ion:163 Resp: 101562
Ion Ratio Lower Upper
163 100
194 4.0 3.4 5.0
164 10.0 8.3 12.5

