

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
 Data File : BN013554.D
 Acq On : 03 Feb 2021 13:45
 Operator : CG/JU
 Sample : M1299-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CAA16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN013554.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	21	rVB	78388	108142	1.27%	0.140%
2	3.770	113	116	121	rVB2	6865	10758	0.13%	0.014%
3	3.864	127	132	135	rBV	19612	25904	0.30%	0.034%
4	4.070	164	167	174	rVB6	15479	21799	0.26%	0.028%
5	4.470	231	235	239	rVB2	7658	10501	0.12%	0.014%
6	4.746	278	282	290	rVB2	12996	22574	0.27%	0.029%
7	6.734	614	620	631	rVB	341005	569427	6.69%	0.738%
8	6.905	642	649	666	rBV	1076564	1688687	19.83%	2.190%
9	7.093	674	681	691	rBV	1229355	1904322	22.36%	2.469%
10	7.558	753	760	767	rBV	1086984	1644967	19.32%	2.133%
11	8.252	872	878	889	rBV	904911	1440072	16.91%	1.867%
12	8.699	946	954	966	rBV	1270334	2043996	24.00%	2.650%
13	9.152	1024	1031	1036	rVB2	18577	28792	0.34%	0.037%
14	9.410	1068	1075	1083	rBV	1012003	1645190	19.32%	2.133%
15	9.652	1110	1116	1120	rBV5	5309	10662	0.13%	0.014%
16	9.940	1158	1165	1178	rBV	1593860	2630332	30.89%	3.411%
17	10.316	1222	1229	1239	rBV	1457446	2416036	28.37%	3.133%
18	10.457	1246	1253	1259	rBV	92730	161205	1.89%	0.209%
19	11.769	1471	1476	1483	rVB4	13528	22039	0.26%	0.029%
20	11.910	1493	1500	1506	rBV	30378	49165	0.58%	0.064%
21	12.593	1613	1616	1622	rVB4	6736	10404	0.12%	0.013%
22	12.746	1637	1642	1645	rVB4	6821	9276	0.11%	0.012%
23	13.034	1685	1691	1698	rBV	39712	57940	0.68%	0.075%
24	13.504	1766	1771	1777	rBV4	7101	12520	0.15%	0.016%
25	13.610	1782	1789	1794	rVV	2922565	4078681	47.90%	5.289%
26	13.657	1794	1797	1802	rVV	118568	160113	1.88%	0.208%
27	13.881	1828	1835	1848	rBV	3724033	5222353	61.33%	6.772%
28	14.116	1869	1875	1880	rBV2	17338	26207	0.31%	0.034%
29	14.193	1880	1888	1897	rVV2	2183100	3227805	37.90%	4.185%
30	14.393	1916	1922	1929	rBV2	263010	379380	4.46%	0.492%
31	15.022	2023	2029	2034	rBV5	5955	14130	0.17%	0.018%
32	15.081	2034	2039	2043	rVV5	10329	13192	0.15%	0.017%
33	15.192	2051	2058	2066	rBV	4583412	6407611	75.24%	8.309%
34	15.310	2072	2078	2094	rBV	1372977	1788635	21.00%	2.319%
35	15.434	2094	2099	2106	rVV2	55632	89030	1.05%	0.115%
36	15.869	2170	2173	2175	rBV4	6731	8760	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
 Data File : BN013554.D
 Acq On : 03 Feb 2021 13:45
 Operator : CG/JU
 Sample : M1299-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CAA16

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
 Title : SVOA CALIBRATION

37	15.981	2188	2192	2200	rVB7	21173	30978	0.36%	0.040%
38	16.198	2223	2229	2234	rBV	36516	52996	0.62%	0.069%
39	16.357	2251	2256	2260	rVB4	14996	21271	0.25%	0.028%
40	16.622	2298	2301	2306	rVB7	12033	14020	0.16%	0.018%
41	16.728	2314	2319	2326	rBV5	15827	26455	0.31%	0.034%
42	16.945	2349	2356	2363	rBV	2611012	3680957	43.23%	4.773%
43	17.039	2364	2372	2386	rVV	5281075	7224064	84.83%	9.367%
44	17.192	2395	2398	2402	rBV6	13863	15918	0.19%	0.021%
45	17.334	2416	2422	2426	rBV8	22041	35936	0.42%	0.047%
46	17.863	2507	2512	2520	rBV	162484	260640	3.06%	0.338%
47	18.575	2629	2633	2636	rVB5	26318	34885	0.41%	0.045%
48	18.745	2659	2662	2664	rBV4	8138	10843	0.13%	0.014%
49	18.804	2670	2672	2676	rBV4	13943	20790	0.24%	0.027%
50	18.975	2697	2701	2706	rBV	64929	91911	1.08%	0.119%
51	19.151	2727	2731	2740	rBV2	108310	158883	1.87%	0.206%
52	19.233	2740	2745	2748	rBV	58664	80853	0.95%	0.105%
53	19.345	2758	2764	2775	rBV	6027022	8395413	98.59%	10.886%
54	20.880	3022	3025	3032	rBV	280749	434422	5.10%	0.563%
55	21.145	3065	3070	3082	rVB	3465359	4414049	51.83%	5.724%
56	22.198	3247	3249	3253	rVB2	135647	128089	1.50%	0.166%
57	22.686	3329	3332	3340	rBV	206724	295410	3.47%	0.383%
58	23.180	3409	3416	3422	rBV	4827993	8515734	100.00%	11.042%
59	23.233	3422	3425	3431	rVB	256693	413006	4.85%	0.536%
60	23.316	3432	3439	3449	rVB2	2485267	4428330	52.00%	5.742%
61	23.857	3528	3531	3536	rVB	244787	372776	4.38%	0.483%




Sum of corrected areas: 77119236

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
Data File : BN013554.D
Acq On : 03 Feb 2021 13:45
Operator : CG/JU
Sample : M1299-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CAA16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

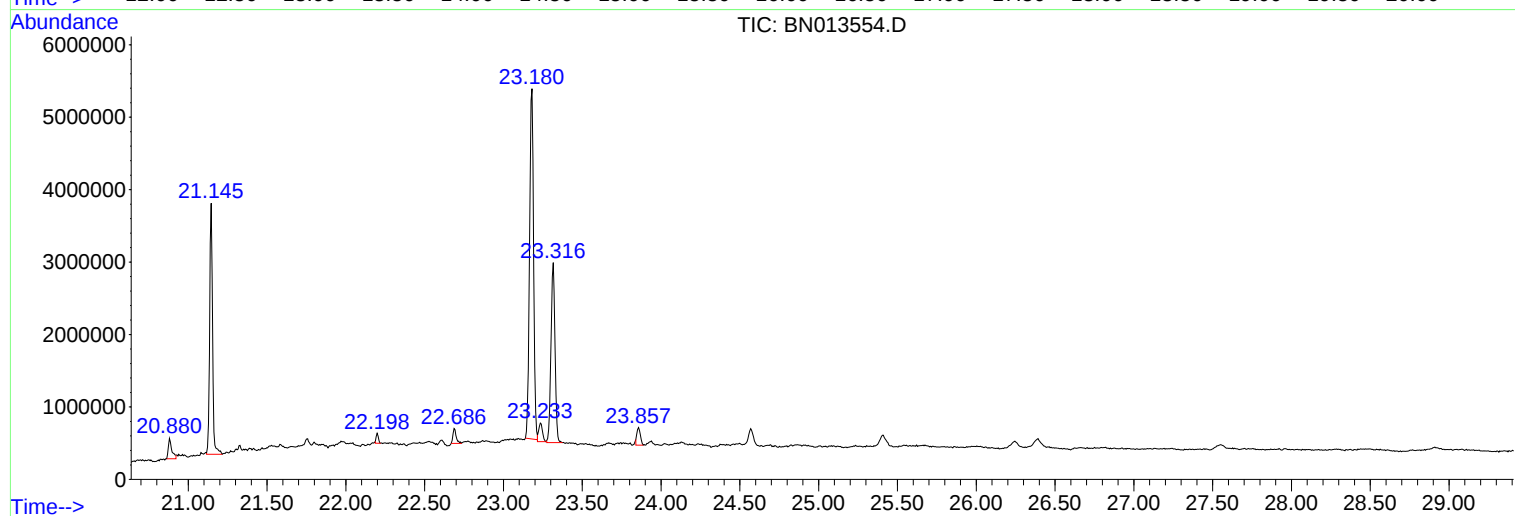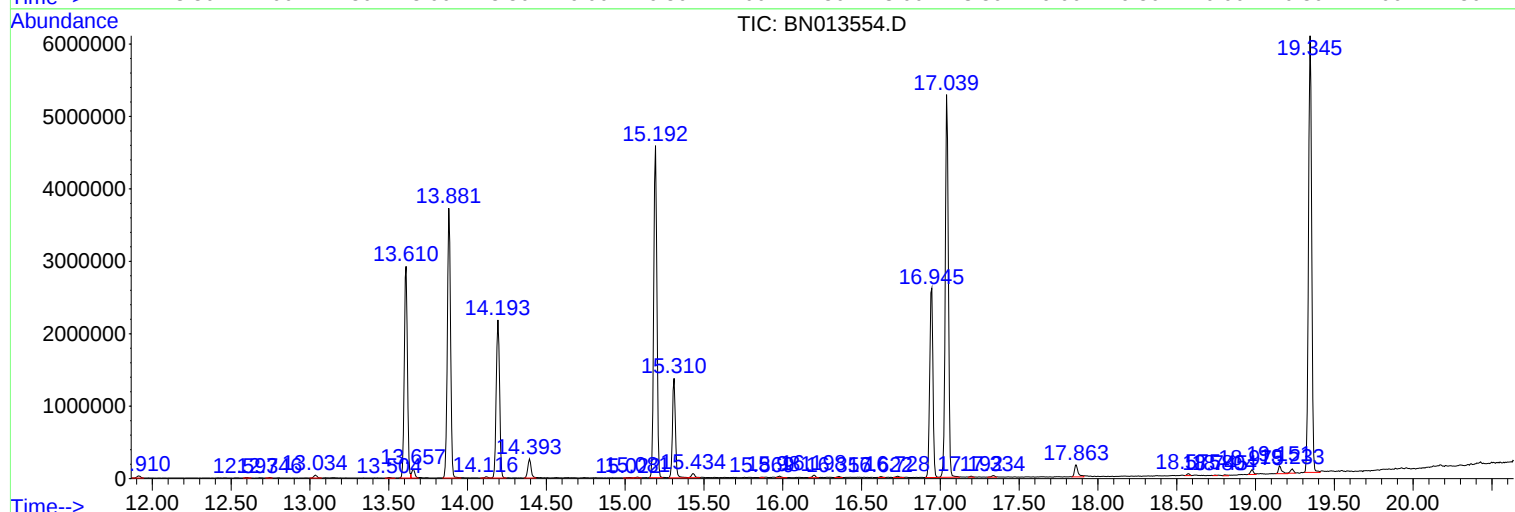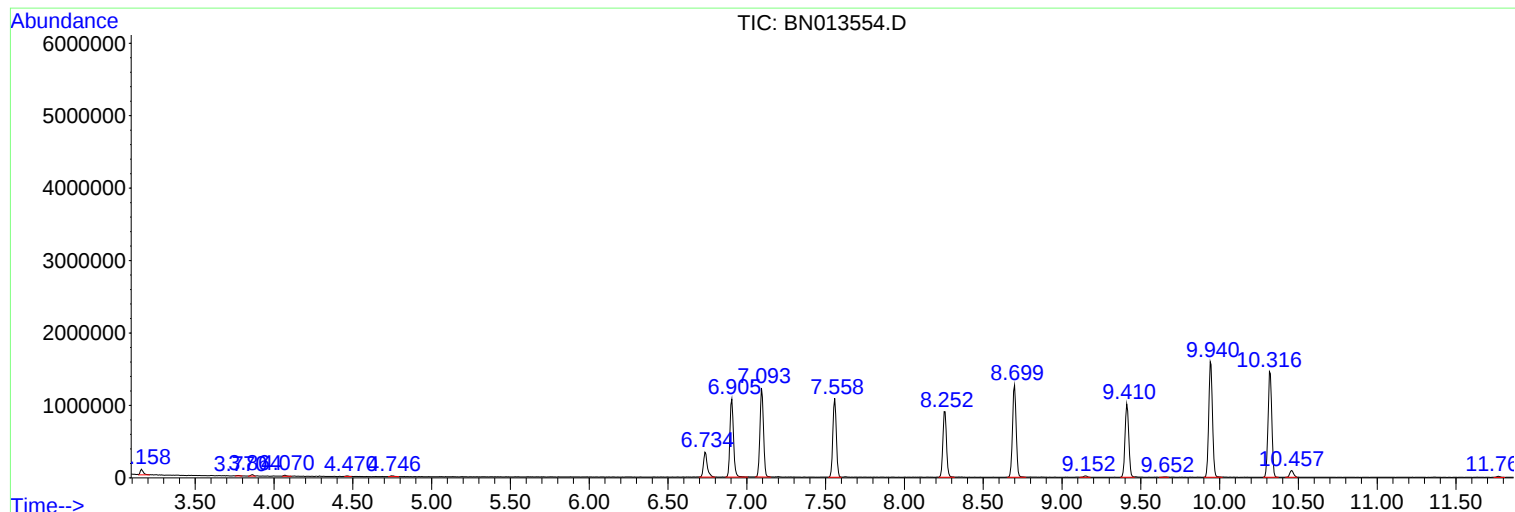

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
Data File : BN013554.D
Acq On : 03 Feb 2021 13:45
Operator : CG/JU
Sample : M1299-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CAA16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020321\
Data File : BN013554.D
Acq On : 03 Feb 2021 13:45
Operator : CG/JU
Sample : M1299-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CAA16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN012921MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
