

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
 Data File : BN036242.D
 Acq On : 03 Feb 2025 23:01
 Operator : RC/JU
 Sample : Q1197-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2999

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
 Supervised By :mohammad ahmed 02/07/2025

Quant Time: Feb 04 08:13:14 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 12:27:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	2842	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	7208	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.428	164	4445	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.175	188	9608m	0.400	ng/ul	0.00
17) Chrysene-d12	21.362	240	8518	0.400	ng/ul	# 0.00
23) Perylene-d12	23.657	264	7187m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	14341	4.609	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.173	152	3567	0.392	ng/ul	0.00
18) Fluoranthene-d10	19.207	212	10346	0.442	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.290	88	137	0.041	ng/ul#	11

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
Data File : BN036242.D
Acq On : 03 Feb 2025 23:01
Operator : RC/JU
Sample : Q1197-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2999


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
Supervised By :mohammad ahmed 02/07/2025

Quant Time: Feb 04 08:13:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

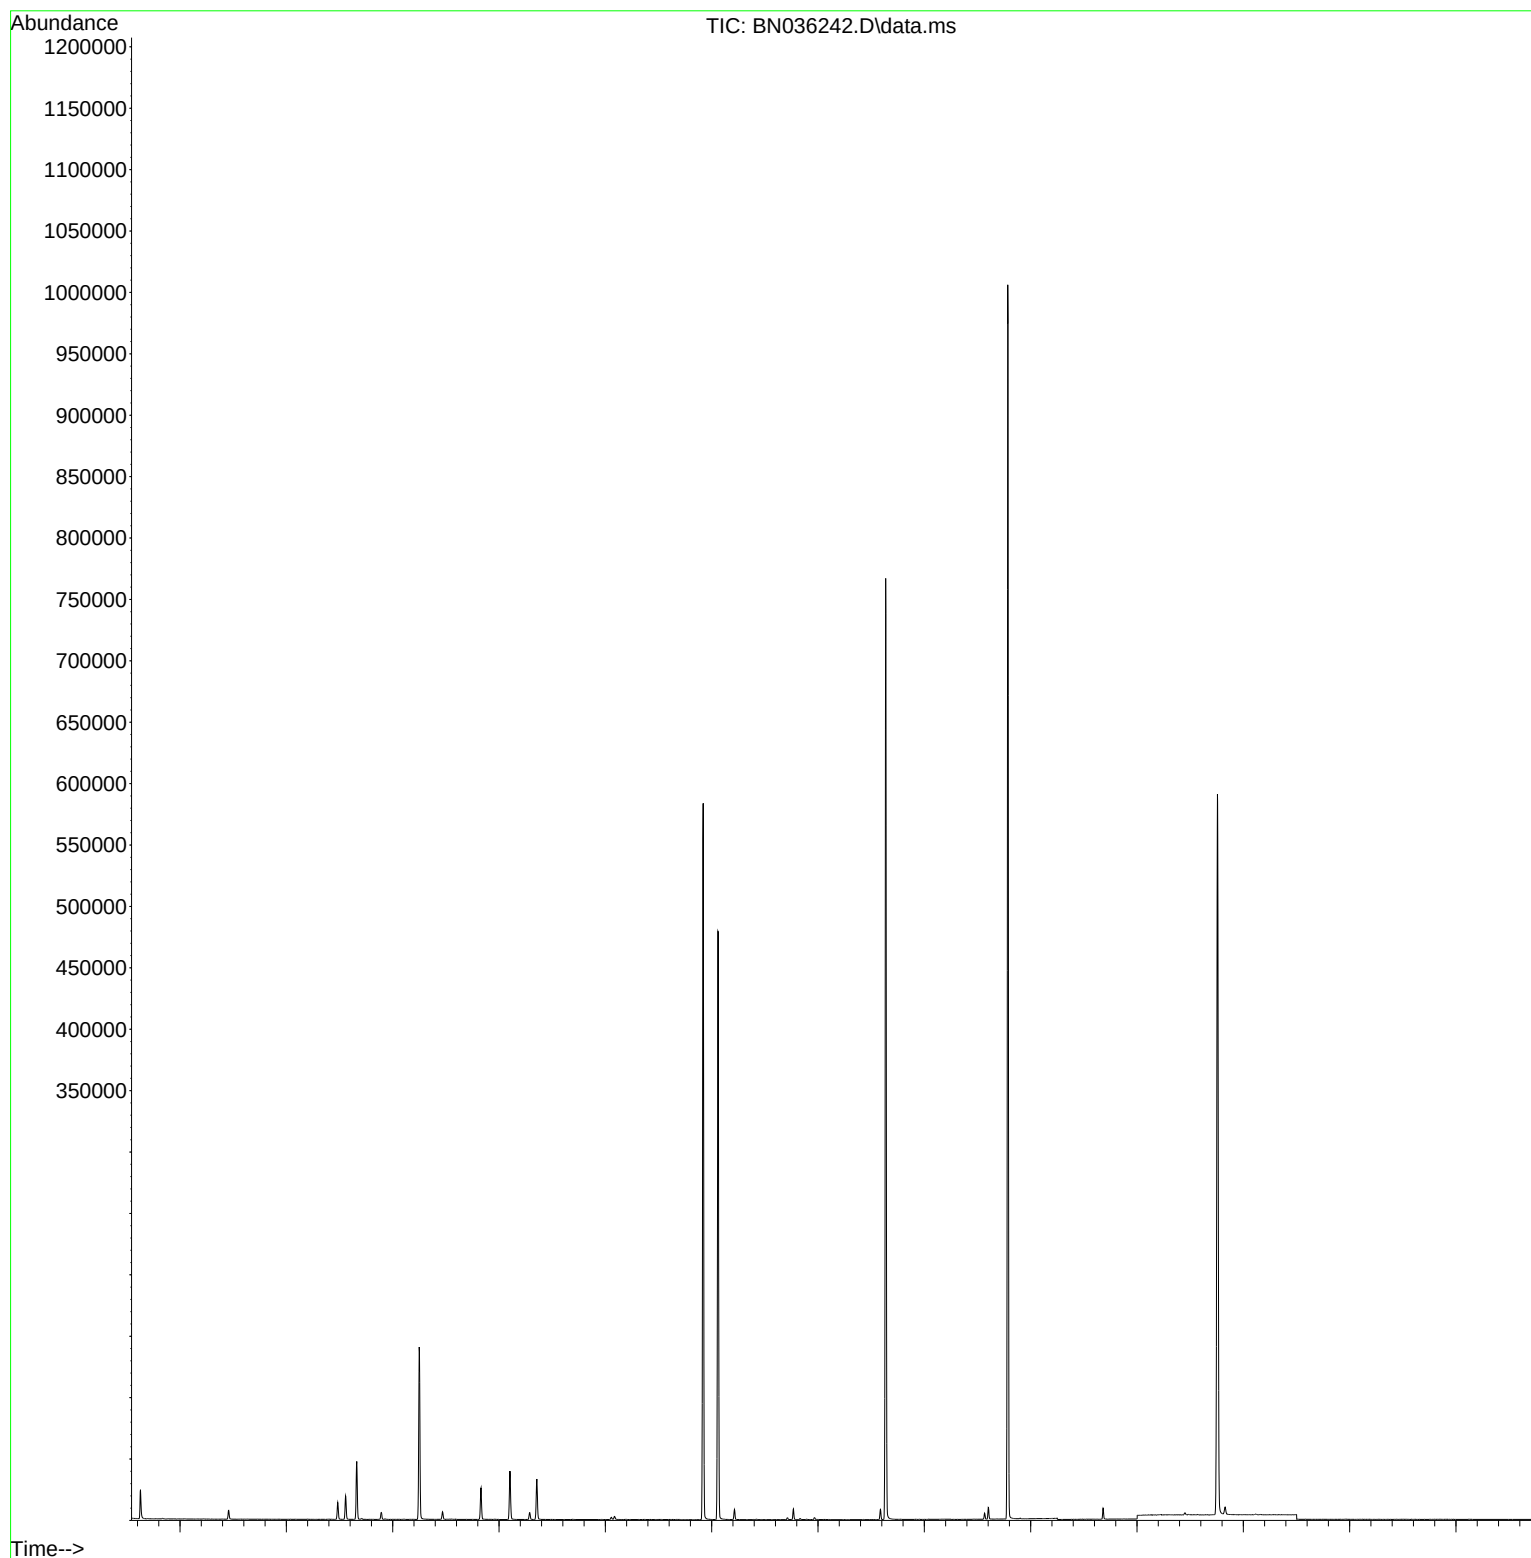

Abundance Scan 50 (3.294 min): BN036232.D\data.ms (-41)

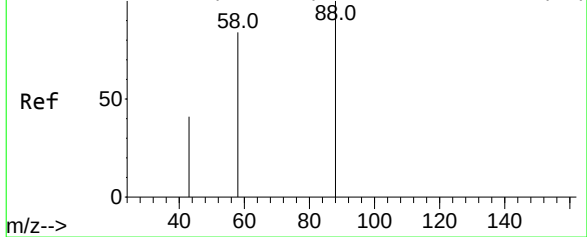

#2

1,4-Dioxane

Concen: 0.041 ng/ul

RT: 3.290 min Scan# 49

Delta R.T. -0.003 min

Lab File: BN036242.D

Acq: 03 Feb 2025 23:01


Instrument :

BNA_N

ClientSampleId :

E2999

Abundance Scan 49 (3.290 min): BN036242.D\data.ms

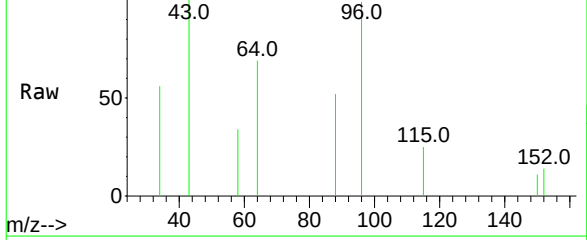

Tgt Ion: 88 Resp: 137

Ion Ratio Lower Upper

88 100

43 191.7 40.7 61.1#

58 65.1 55.2 82.8


Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025

Supervised By :mohammad ahmed 02/07/2025

Abundance Scan 49 (3.290 min): BN036242.D\data.ms (-33)

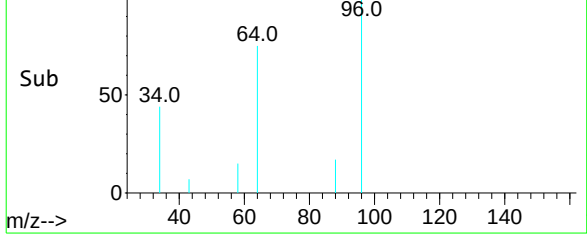

Abundance

