

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
 Data File : BN036243.D
 Acq On : 03 Feb 2025 23:37
 Operator : RC/JU
 Sample : Q1197-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2997

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
 Supervised By :mohammad ahmed 02/07/2025

Quant Time: Feb 04 08:15:54 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 12:27:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	2769	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	7044	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.428	164	4318	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.175	188	9251m	0.400	ng/ul	0.00
17) Chrysene-d12	21.362	240	8422	0.400	ng/ul	# 0.00
23) Perylene-d12	23.657	264	6825m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	15523	5.120	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.174	152	3884	0.437	ng/ul	0.00
18) Fluoranthene-d10	19.207	212	10932	0.472	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.628	128	481	0.025	ng/ul#	Qvalue 69

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
Data File : BN036243.D
Acq On : 03 Feb 2025 23:37
Operator : RC/JU
Sample : Q1197-18
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E2997

Quant Time: Feb 04 08:15:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 02/04/2025
Supervised By :mohammad ahmed 02/07/2025

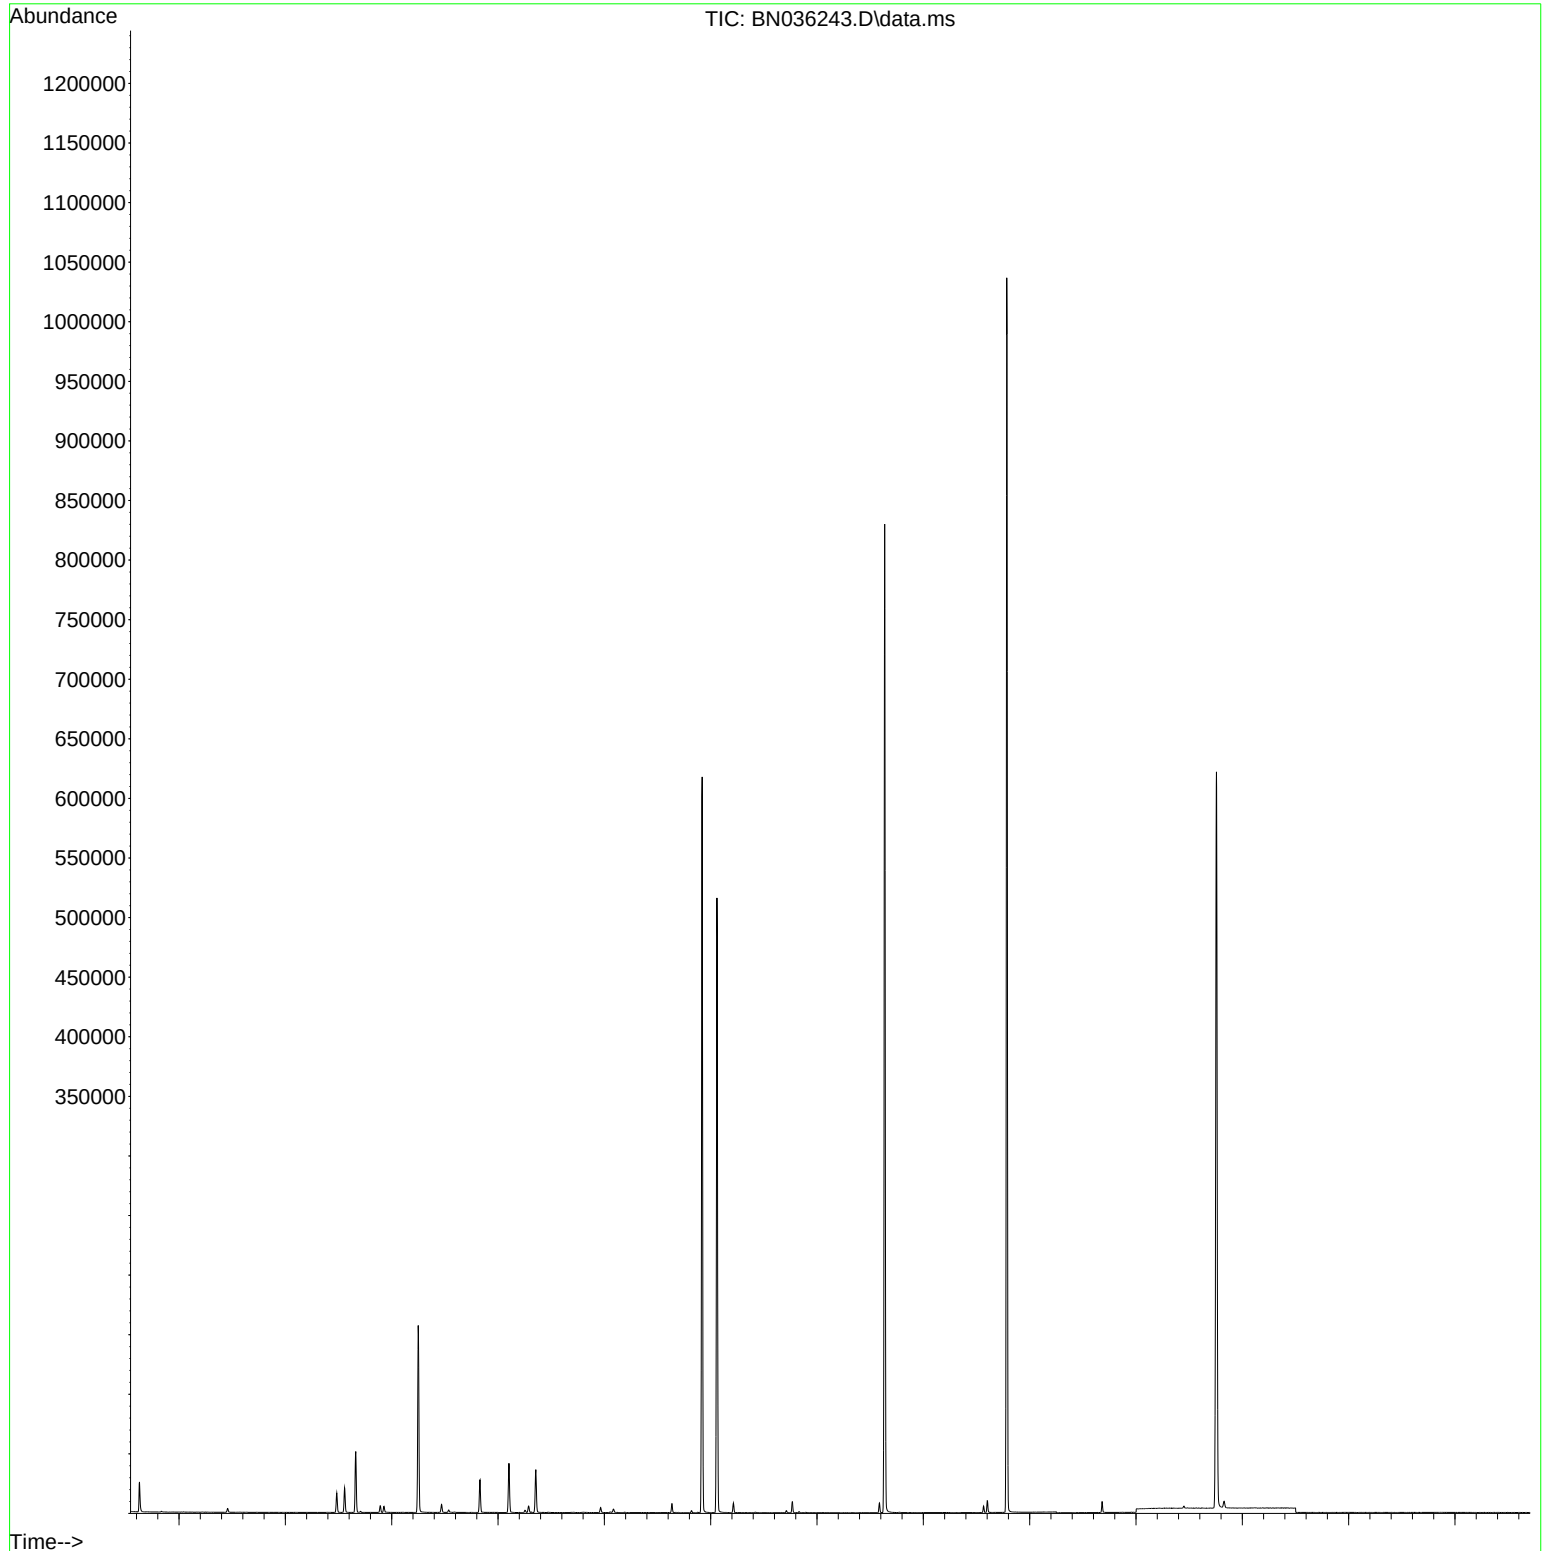

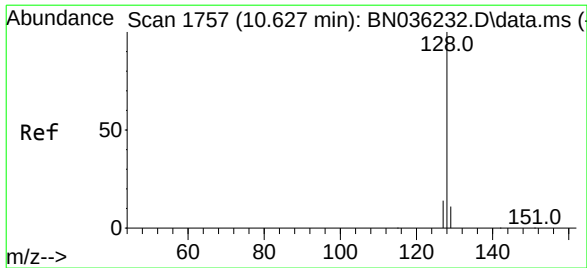

Naphthalene
 Concen: 0.025 ng/ul
 RT: 10.628 min Scan# 1757
 Delta R.T. 0.001 min
 Lab File: BN036243.D
 Acq: 03 Feb 2025 23:37

Instrument :
 BNA_N
 ClientSampleId :
 E2997

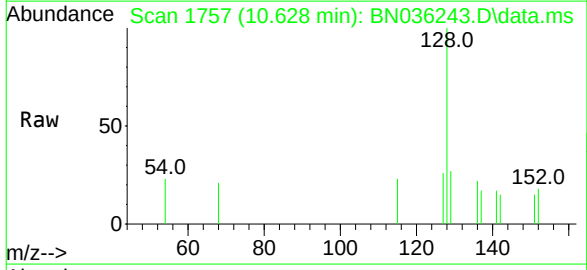

Tgt Ion:	128	Resp:	481
Ion Ratio	Lower	Upper	
128	100		
129	27.0	9.6	14.4#
127	25.6	12.0	18.0#

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
 Supervised By :mohammad ahmed 02/07/2025

