

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
 Data File : BN036245.D
 Acq On : 04 Feb 2025 00:49
 Operator : RC/JU
 Sample : Q1197-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2974

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
 Supervised By :mohammad ahmed 02/07/2025

Quant Time: Feb 04 08:21:16 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 12:27:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	3132	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	7940	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.428	164	5063	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.175	188	11195m	0.400	ng/ul	0.00
17) Chrysene-d12	21.365	240	10883	0.400	ng/ul	0.00
23) Perylene-d12	23.660	264	9692m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	14136	4.122	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.173	152	3673	0.366	ng/ul	0.00
18) Fluoranthene-d10	19.207	212	11211	0.375	ng/ul	0.00
Target Compounds						
16) Anthracene	17.306	178	2938	0.096	ng/ul#	Qvalue 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
Data File : BN036245.D
Acq On : 04 Feb 2025 00:49
Operator : RC/JU
Sample : Q1197-05
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E2974

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
Supervised By :mohammad ahmed 02/07/2025


Quant Time: Feb 04 08:21:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

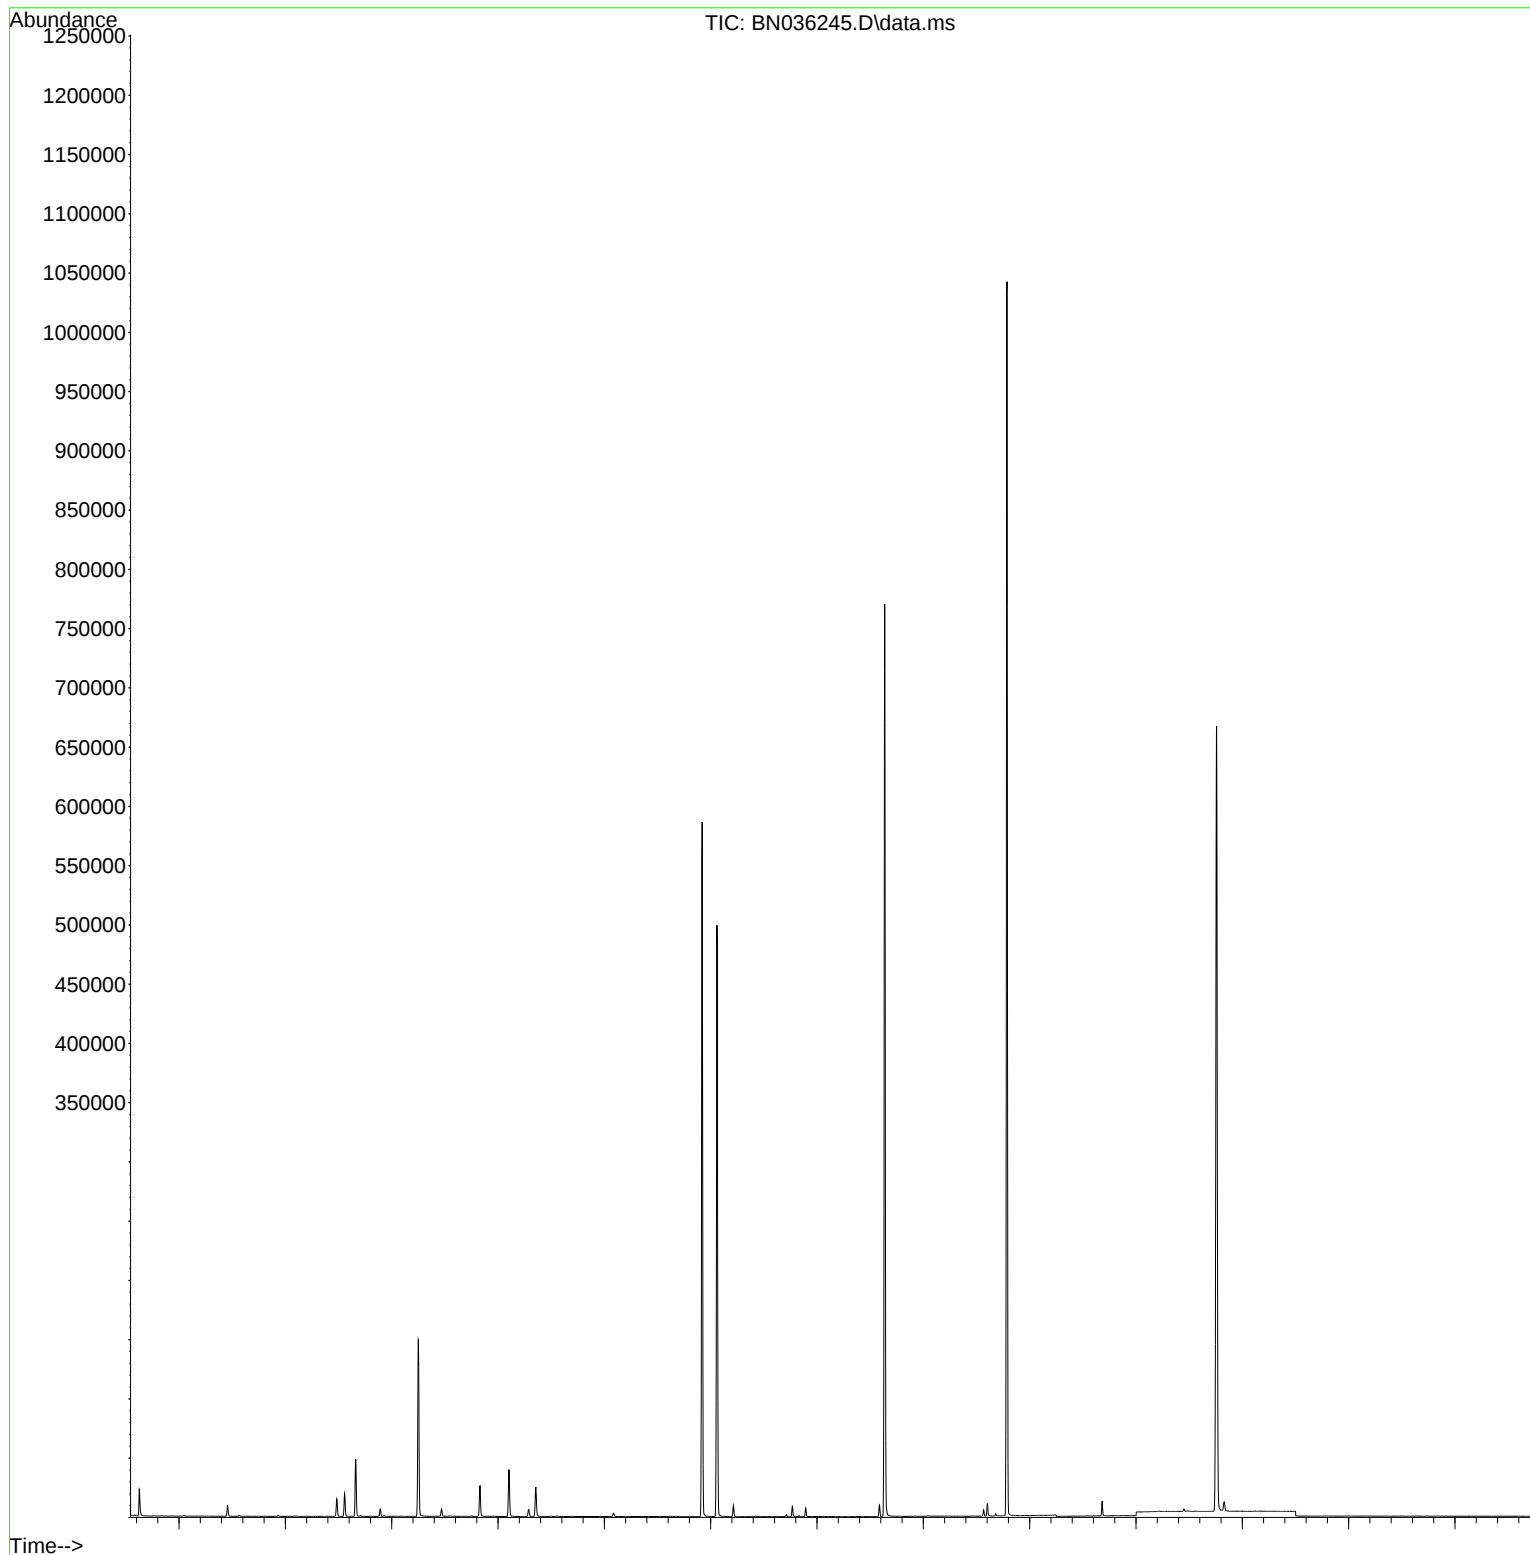

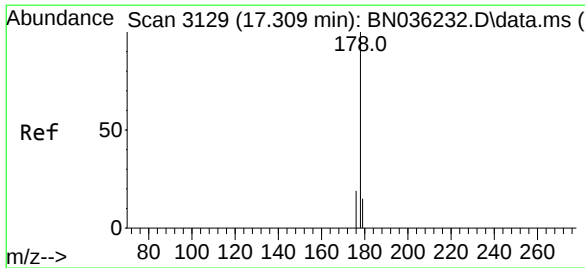

#16
Anthracene
Concen: 0.096 ng/ul
RT: 17.306 min Scan# 3128
Delta R.T. 0.001 min
Lab File: BN036245.D
Acq: 04 Feb 2025 00:49

Instrument :
BNA_N
ClientSampleId :
E2974

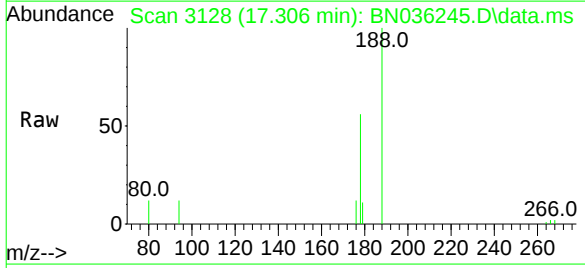

Tgt	Ion	178	Resp	2938
Ion	Ratio	100	Lower	Upper
178	100			
179	20.4	13.0	19.4	
176	22.1	15.9	23.9	

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
Supervised By :mohammad ahmed 02/07/2025

