

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
 Data File : BN036246.D
 Acq On : 04 Feb 2025 01:25
 Operator : RC/JU
 Sample : Q1197-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2981

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
 Supervised By :mohammad ahmed 02/07/2025

Quant Time: Feb 04 08:23:31 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 12:27:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.783	152	3034	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	7385	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.428	164	4338	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.175	188	8938m	0.400	ng/ul	0.00
17) Chrysene-d12	21.362	240	8247	0.400	ng/ul	# 0.00
23) Perylene-d12	23.657	264	8130m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	17079	5.141	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.174	152	3179	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.207	212	8840	0.390	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.623	128	413	0.020	ng/ul#	59

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
Data File : BN036246.D
Acq On : 04 Feb 2025 01:25
Operator : RC/JU
Sample : Q1197-06
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E2981

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
Supervised By :mohammad ahmed 02/07/2025


Quant Time: Feb 04 08:23:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

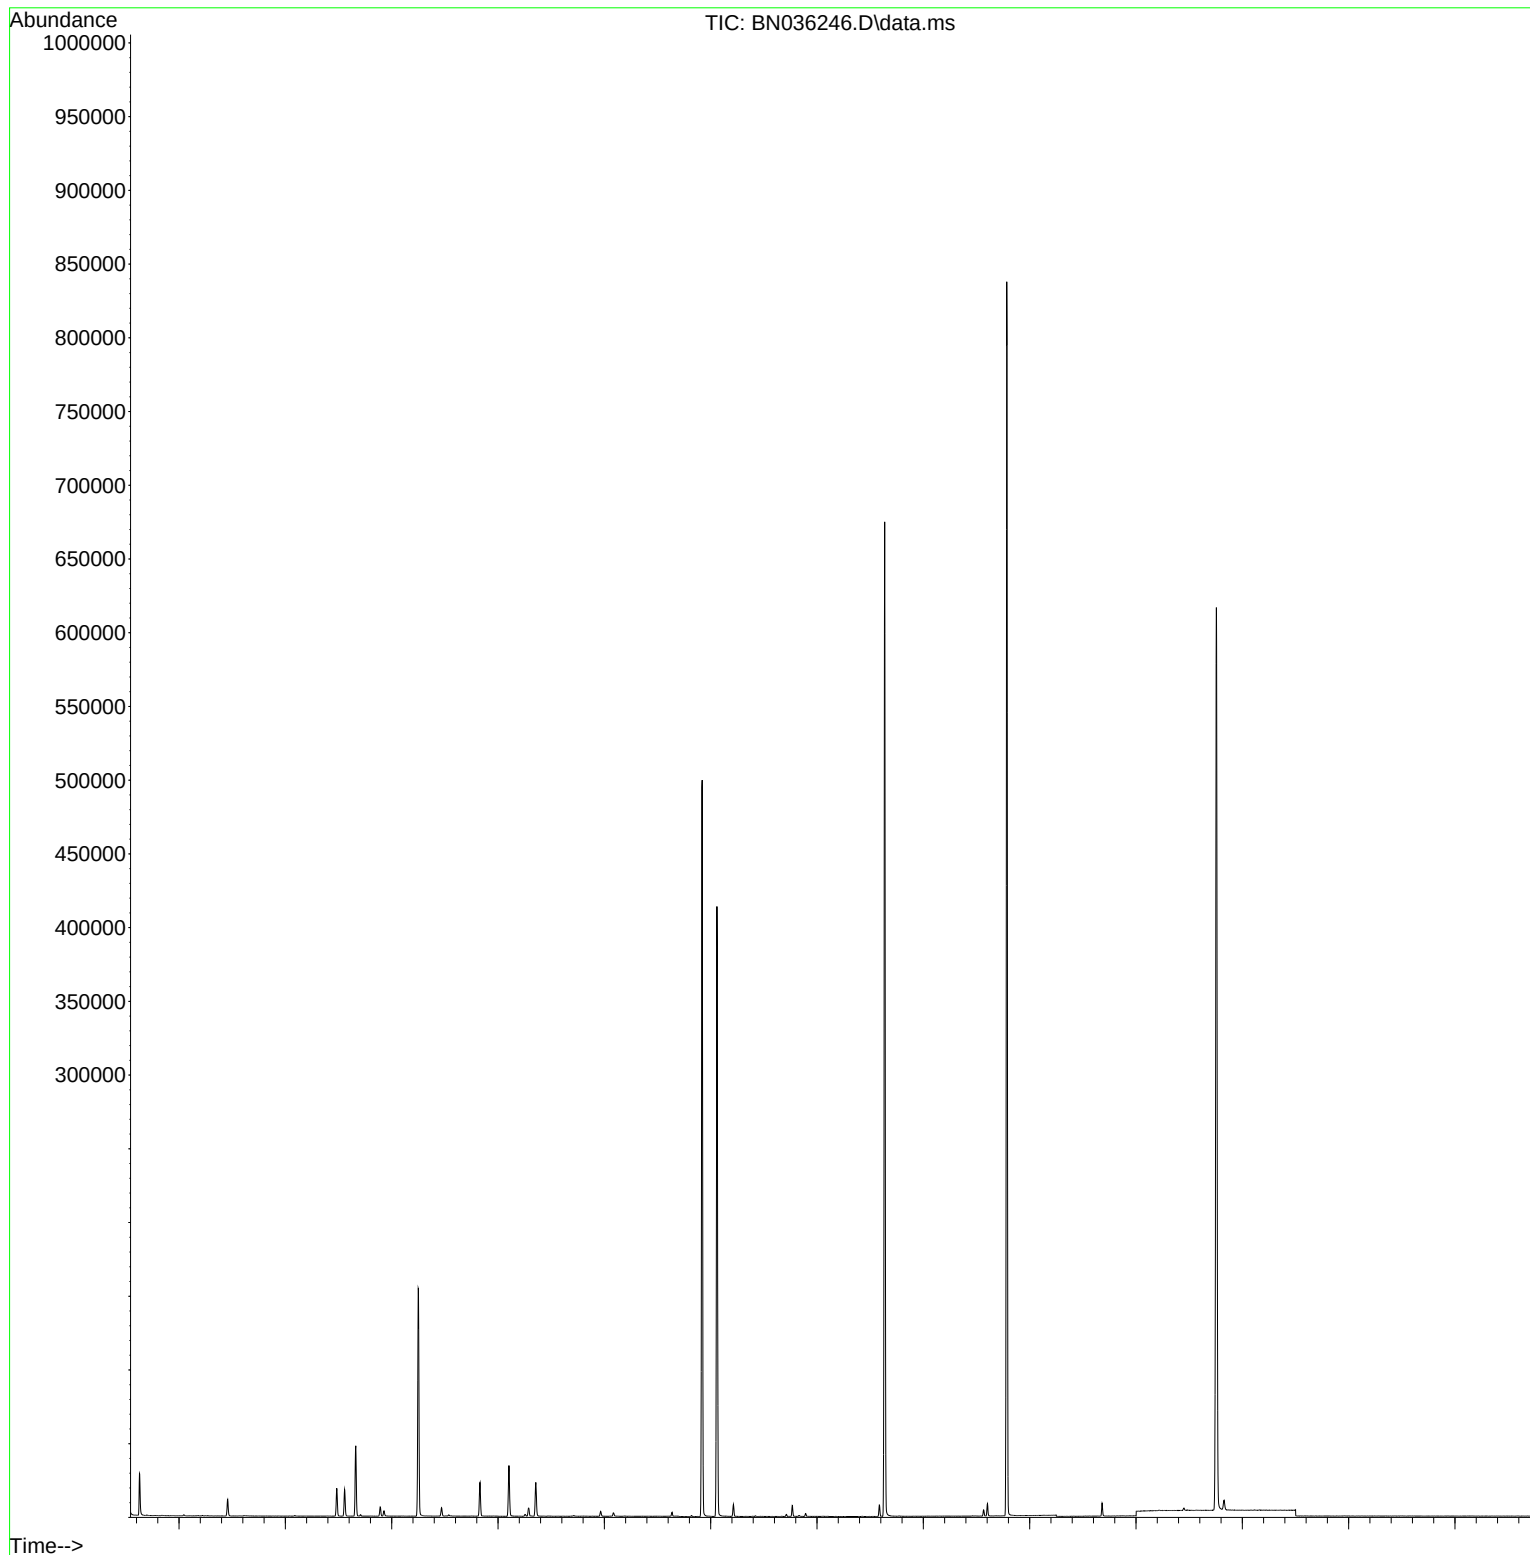

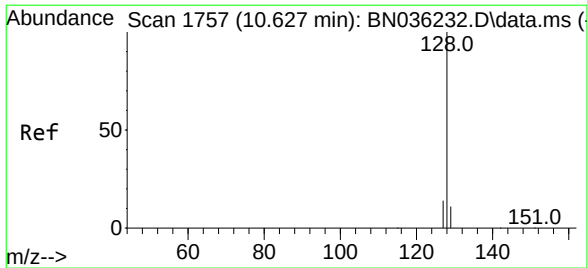

Naphthalene
 Concen: 0.020 ng/u1
 RT: 10.623 min Scan# 1756
 Delta R.T. -0.004 min
 Lab File: BN036246.D
 Acq: 04 Feb 2025 01:25

Instrument : BNA_N
 ClientSampleId : E2981

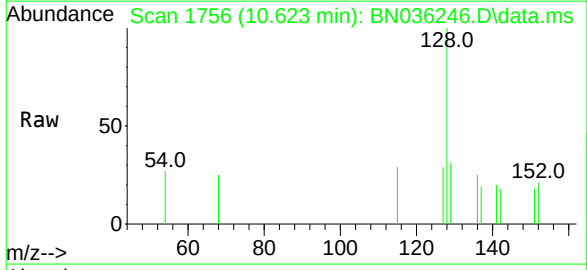

Tgt Ion:	128	Resp:	413
Ion	Ratio	Lower	Upper
128	100		
129	31.0	9.6	14.4#
127	29.1	12.0	18.0#

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
 Supervised By :mohammad ahmed 02/07/2025

