

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
 Data File : BN036247.D
 Acq On : 04 Feb 2025 02:01
 Operator : RC/JU
 Sample : Q1197-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2982

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
 Supervised By :mohammad ahmed 02/07/2025

Quant Time: Feb 04 08:26:01 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 12:27:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	2948	0.400	ng/ul	0.00
4) Naphthalene-d8	10.577	136	7291	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.426	164	4145	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.174	188	8350m	0.400	ng/ul	0.00
17) Chrysene-d12	21.363	240	7139	0.400	ng/ul	# 0.00
23) Perylene-d12	23.655	264	6793m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	14940	4.629	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.172	152	3070	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.206	212	8363	0.426	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.627	128	531	0.026	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
Data File : BN036247.D
Acq On : 04 Feb 2025 02:01
Operator : RC/JU
Sample : Q1197-07
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E2982

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
Supervised By :mohammad ahmed 02/07/2025


Quant Time: Feb 04 08:26:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

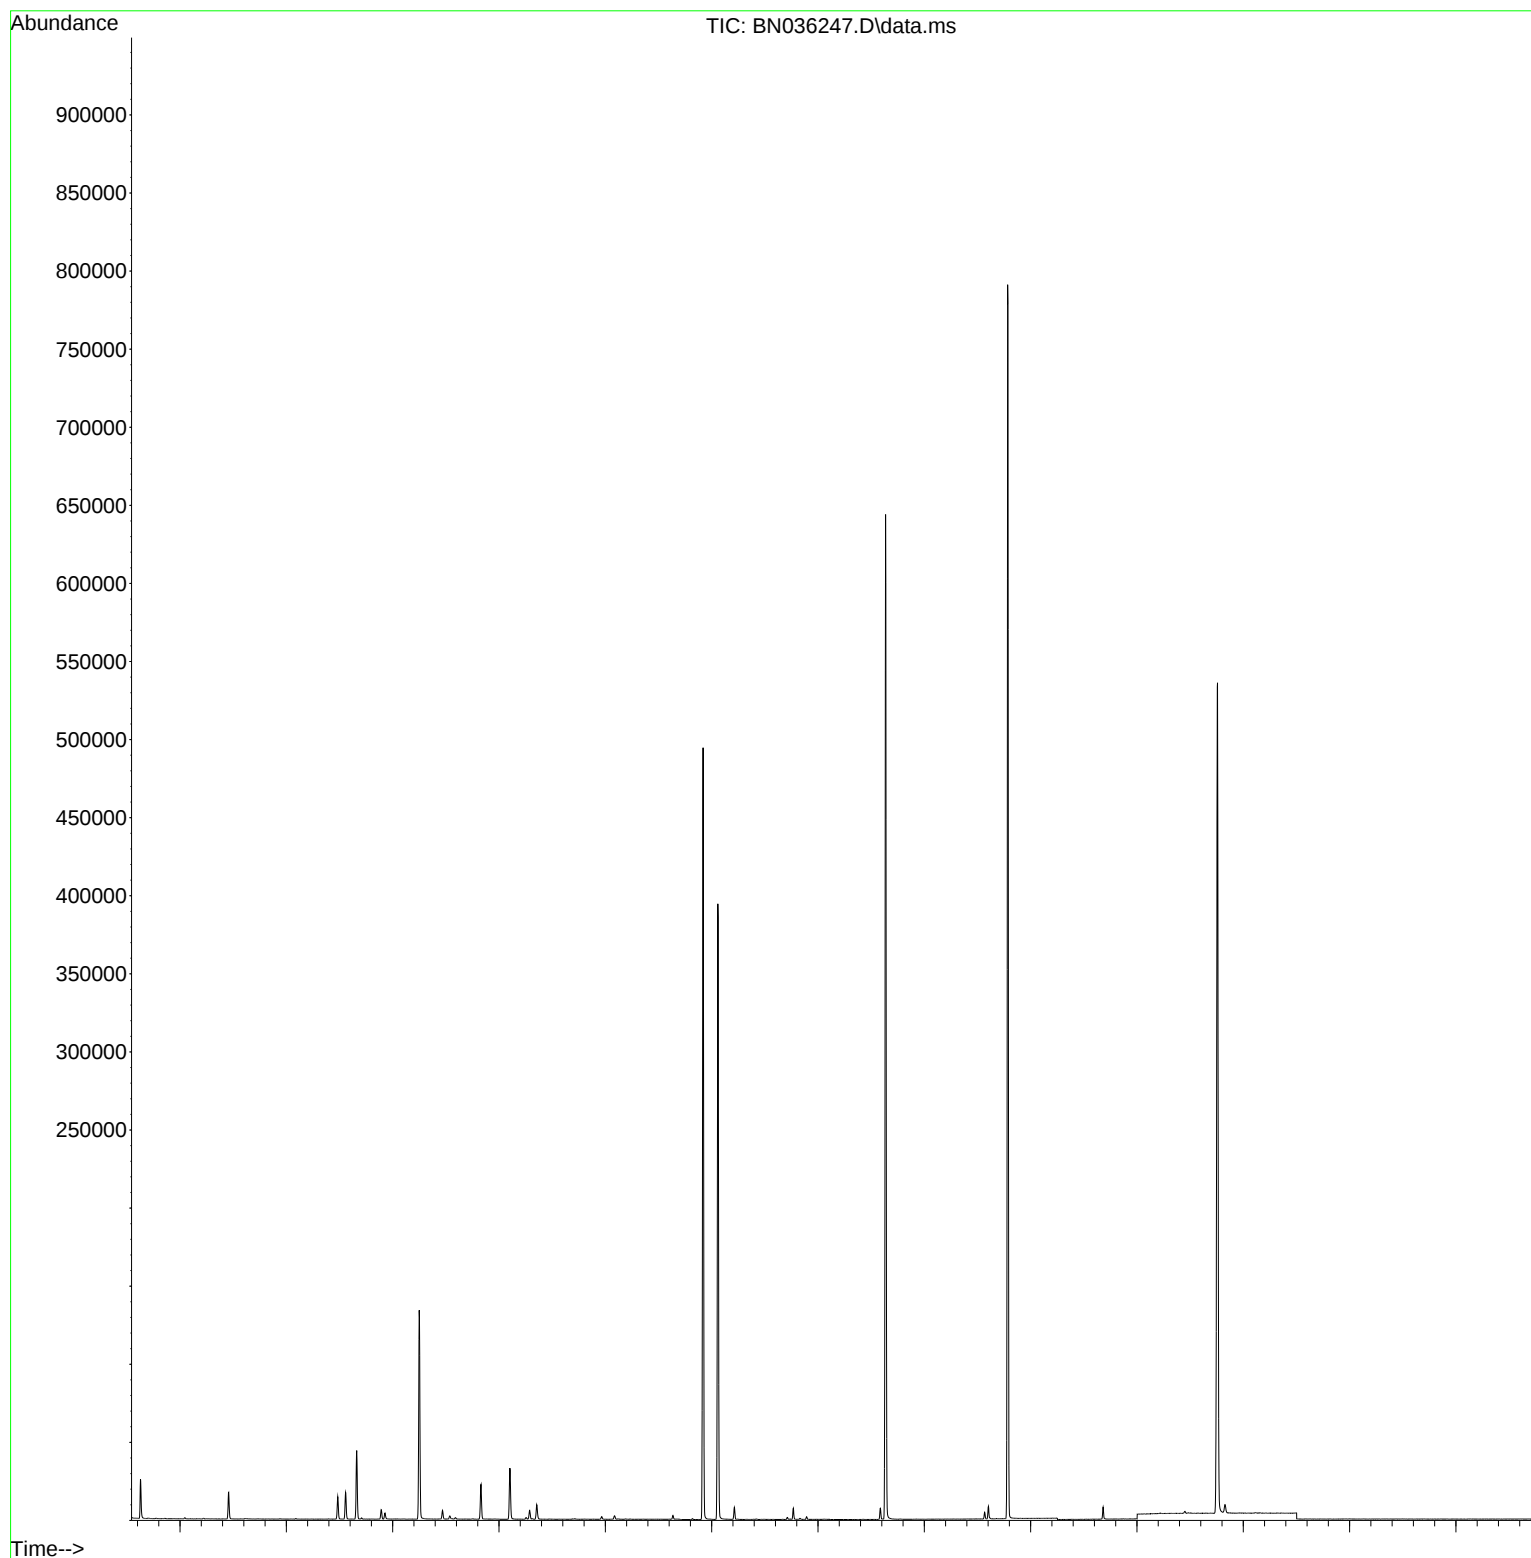

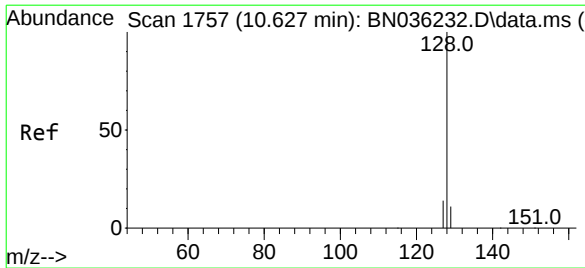

Naphthalene
Concen: 0.026 ng/u1
RT: 10.627 min Scan# 1757
Delta R.T. -0.000 min
Lab File: BN036247.D
Acq: 04 Feb 2025 02:01

Instrument :
BNA_N
ClientSampleId :
E2982

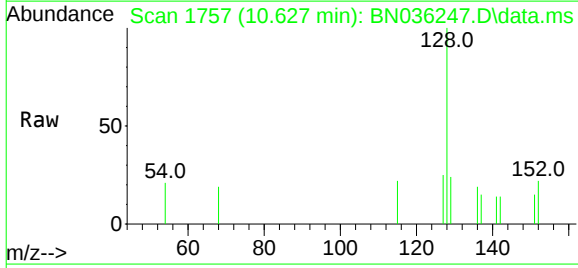

Tgt	Ion	128	Resp	531
Ion	Ratio	Lower	Upper	
128	100			
129	24.2	9.6	14.4	#
127	25.2	12.0	18.0	#

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
Supervised By :mohammad ahmed 02/07/2025

