

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
 Data File : BN036248.D
 Acq On : 04 Feb 2025 02:38
 Operator : RC/JU
 Sample : Q1197-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2983

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
 Supervised By :mohammad ahmed 02/07/2025

Quant Time: Feb 04 08:28:21 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 12:27:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.783	152	3021	0.400	ng/ul	0.00
4) Naphthalene-d8	10.577	136	7242	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.426	164	4256	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.174	188	8751m	0.400	ng/ul	0.00
17) Chrysene-d12	21.366	240	7976	0.400	ng/ul	# 0.00
23) Perylene-d12	23.657	264	7541m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	15657	4.734	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.172	152	3094	0.338	ng/ul	0.00
18) Fluoranthene-d10	19.206	212	8611	0.393	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.298	88	295m	0.084	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020325\
Data File : BN036248.D
Acq On : 04 Feb 2025 02:38
Operator : RC/JU
Sample : Q1197-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2983


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025
Supervised By :mohammad ahmed 02/07/2025

Quant Time: Feb 04 08:28:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

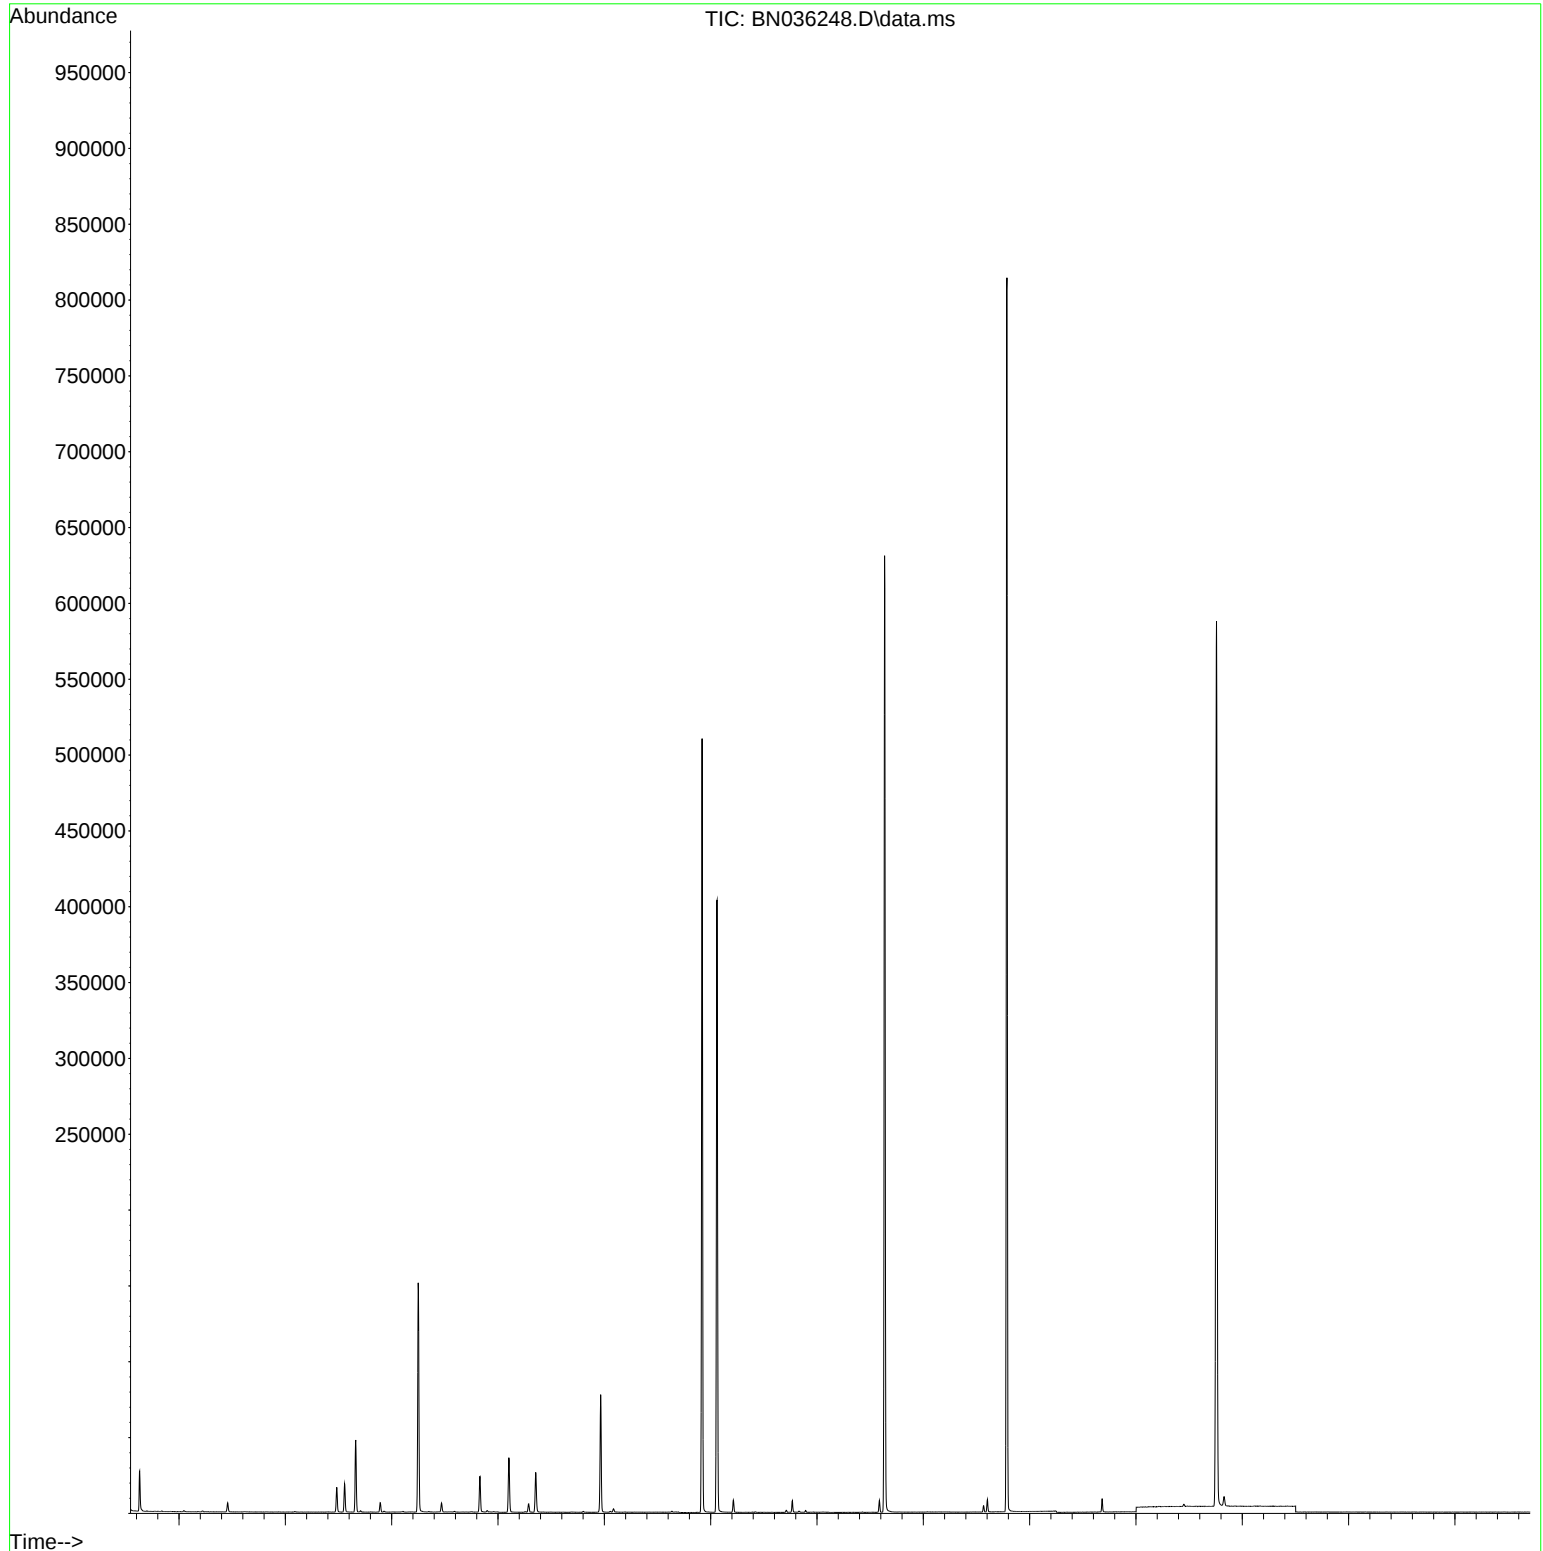

Abundance Scan 50 (3.294 min): BN036232.D\data.ms (-41)

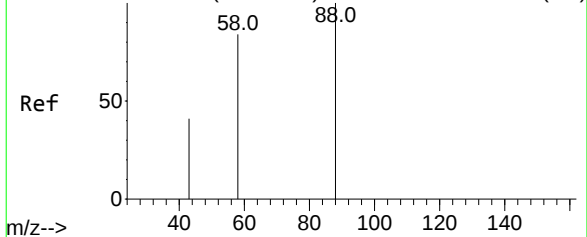

#2

1,4-Dioxane

Concen: 0.084 ng/ul m

RT: 3.298 min Scan# 51

Delta R.T. 0.005 min

Lab File: BN036248.D

Acq: 04 Feb 2025 02:38


Instrument :

BNA_N

ClientSampleId :

E2983

Abundance Scan 51 (3.298 min): BN036248.D\data.ms

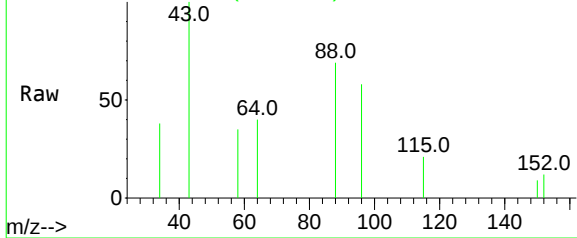

Tgt Ion: 88 Resp: 295

Ion Ratio Lower Upper

88 100

43 144.8 40.7 61.1#

58 51.3 55.2 82.8#


Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 02/04/2025

Supervised By :mohammad ahmed 02/07/2025

Abundance Scan 51 (3.298 min): BN036248.D\data.ms (-33)

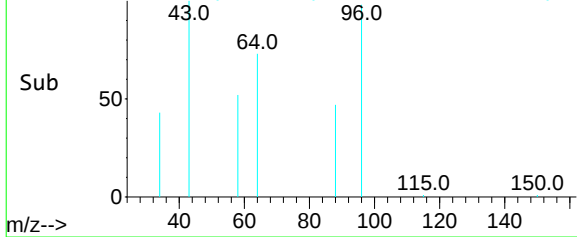

Abundance

