


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020421\
Data File : BN013574.D
Acq On : 04 Feb 2021 16:42
Operator : CG/JU
Sample : M1299-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA5

Manual Integrations
APPROVED

mohammad
2/8/2021 12:17:16 PM

Quant Time: Feb 04 17:13:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 04 14:51:05 2021
Response via : Initial Calibration

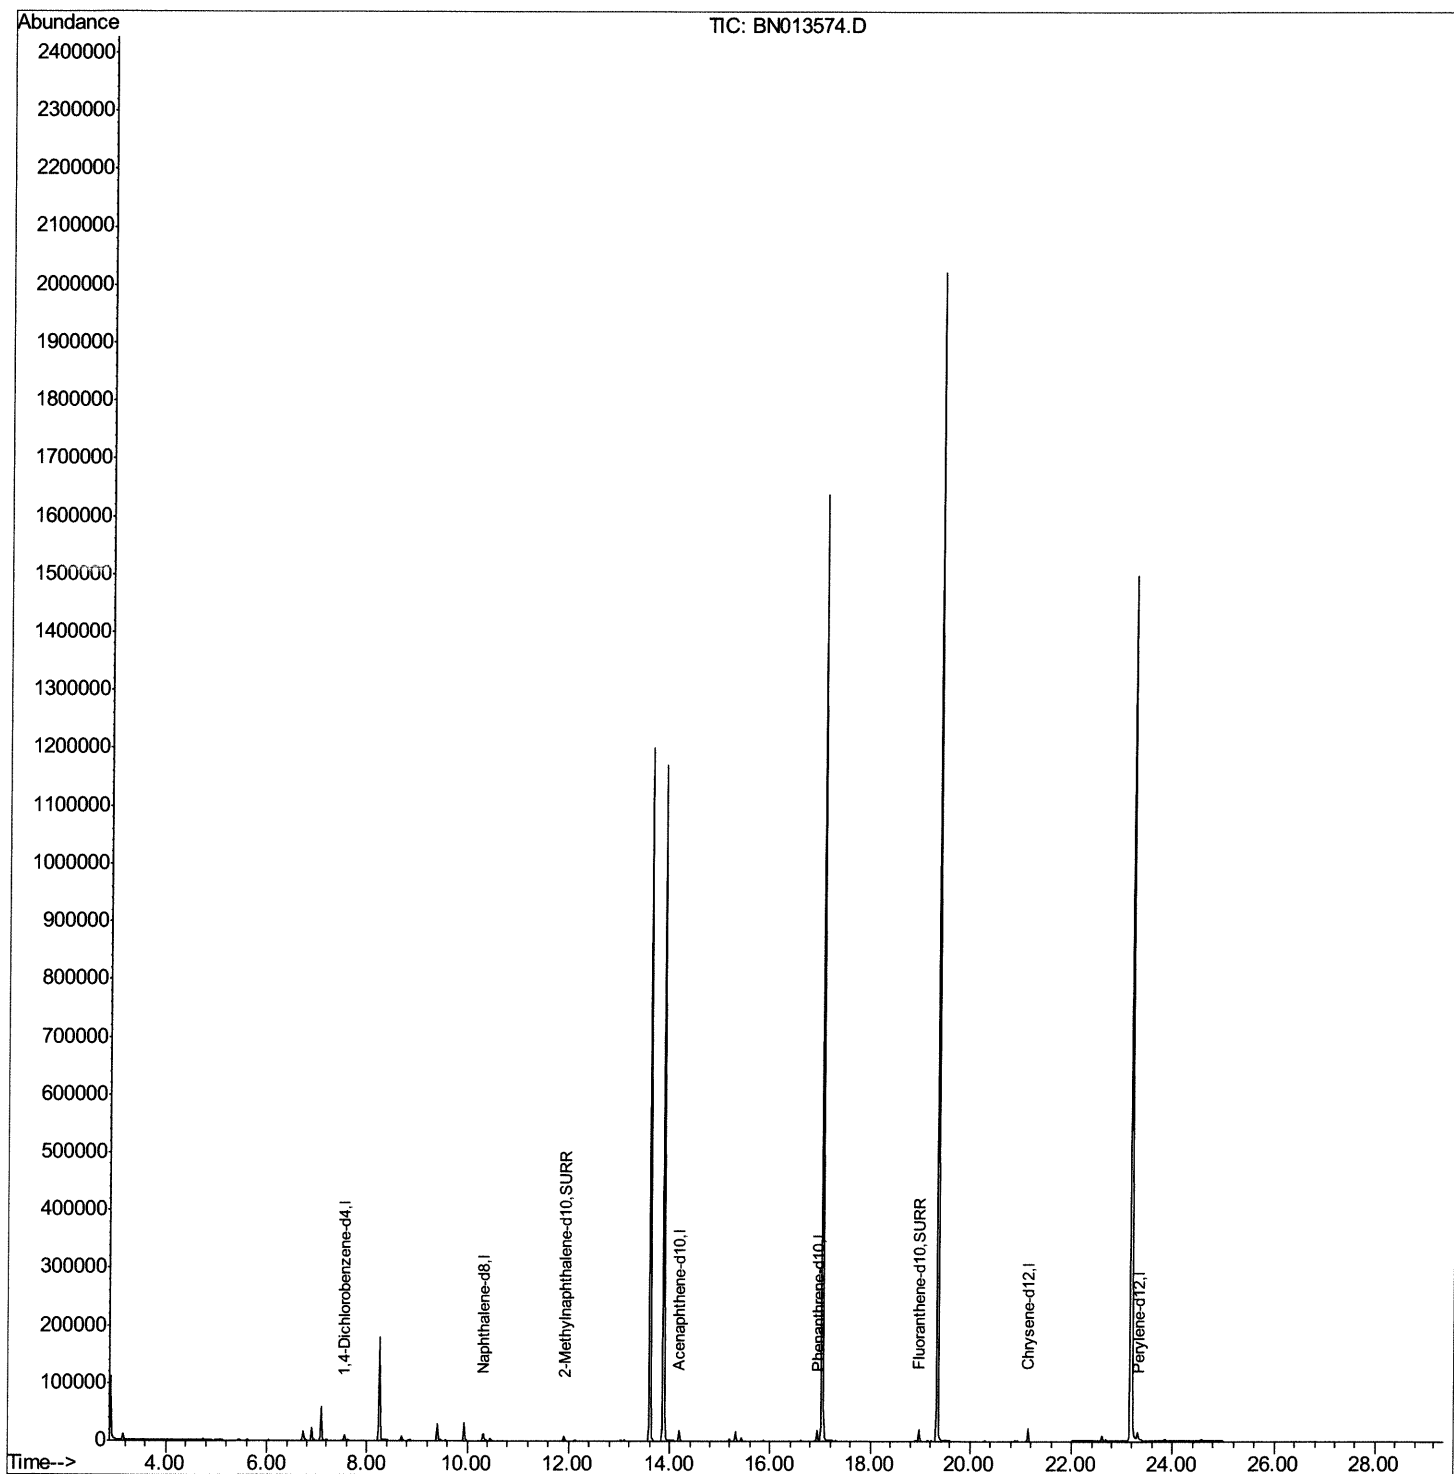

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020421\
 Data File : BN013574.D
 Acq On : 04 Feb 2021 16:42
 Operator : CG/JU
 Sample : M1299-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

mohammad
 2/8/2021 12:17:16 PM

Quant Time: Feb 04 17:12:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 04 14:51:05 2021
 Response via : Initial Calibration

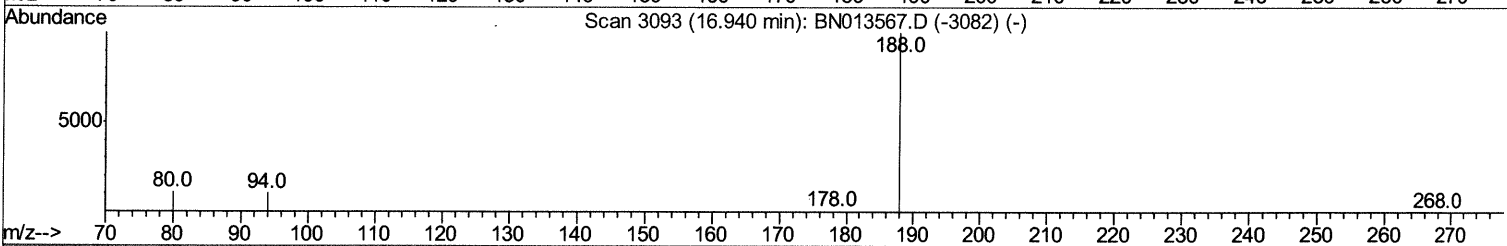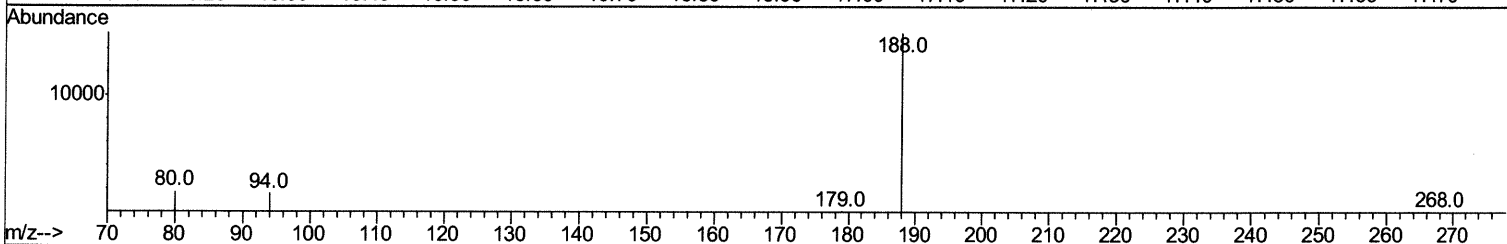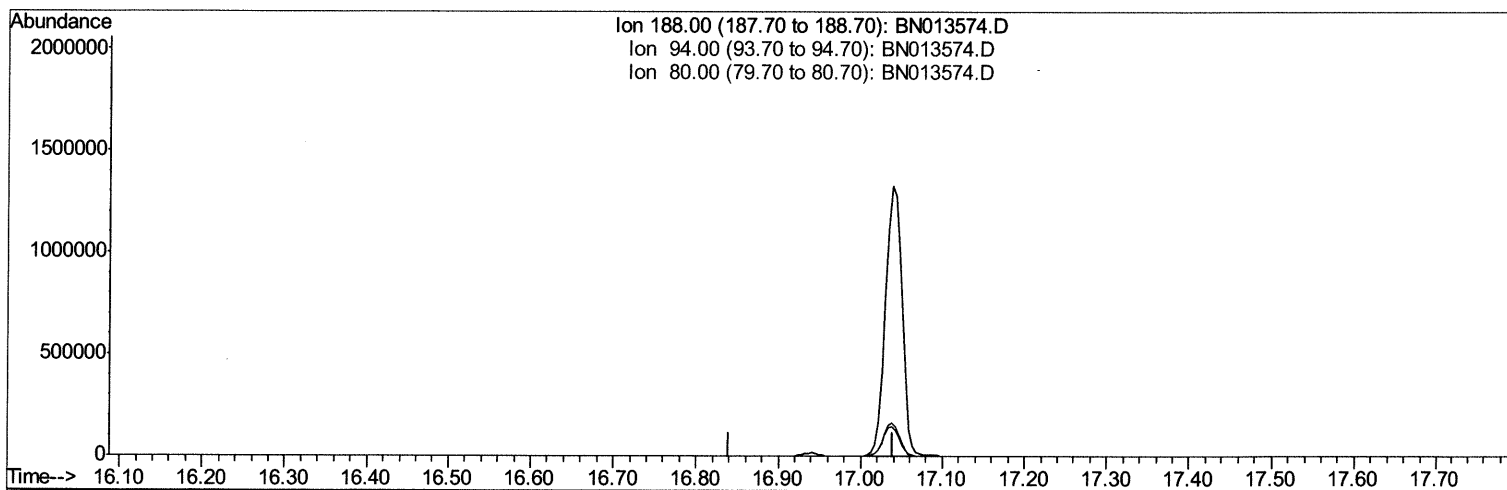

TIC: BN013574.D

(10) Phenanthrene-d10 (I)

16.940min (-16.940) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020421\
 Data File : BN013574.D
 Acq On : 04 Feb 2021 16:42
 Operator : CG/JU
 Sample : M1299-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

mohammad
 2/8/2021 12:17:16 PM

Quant Time: Feb 04 17:12:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 04 14:51:05 2021
 Response via : Initial Calibration

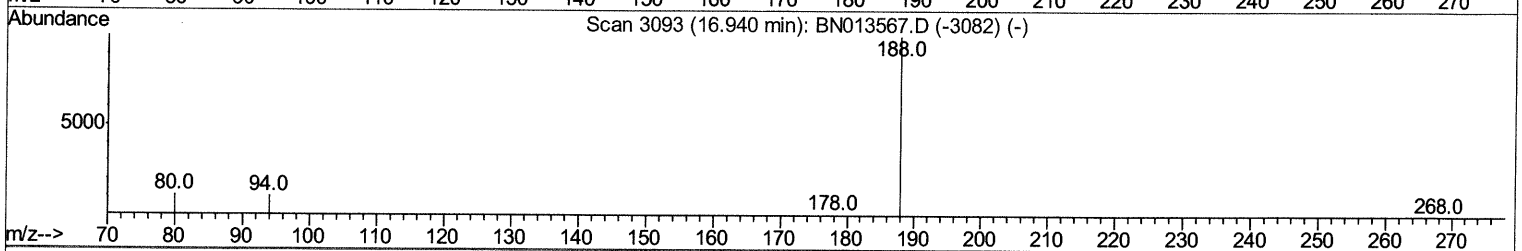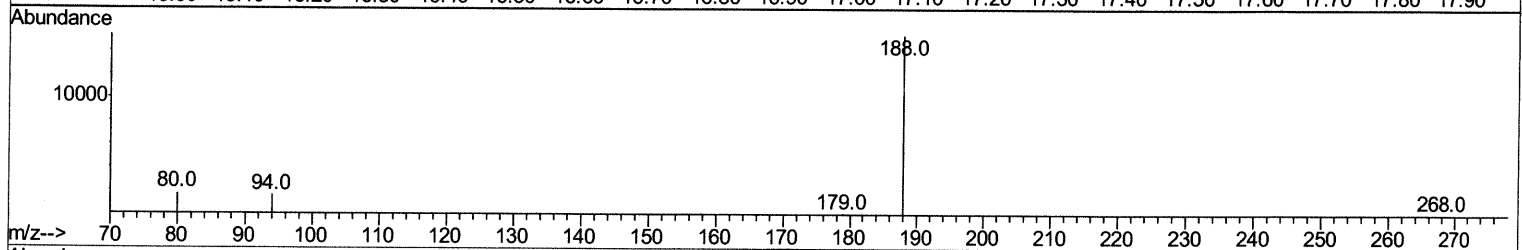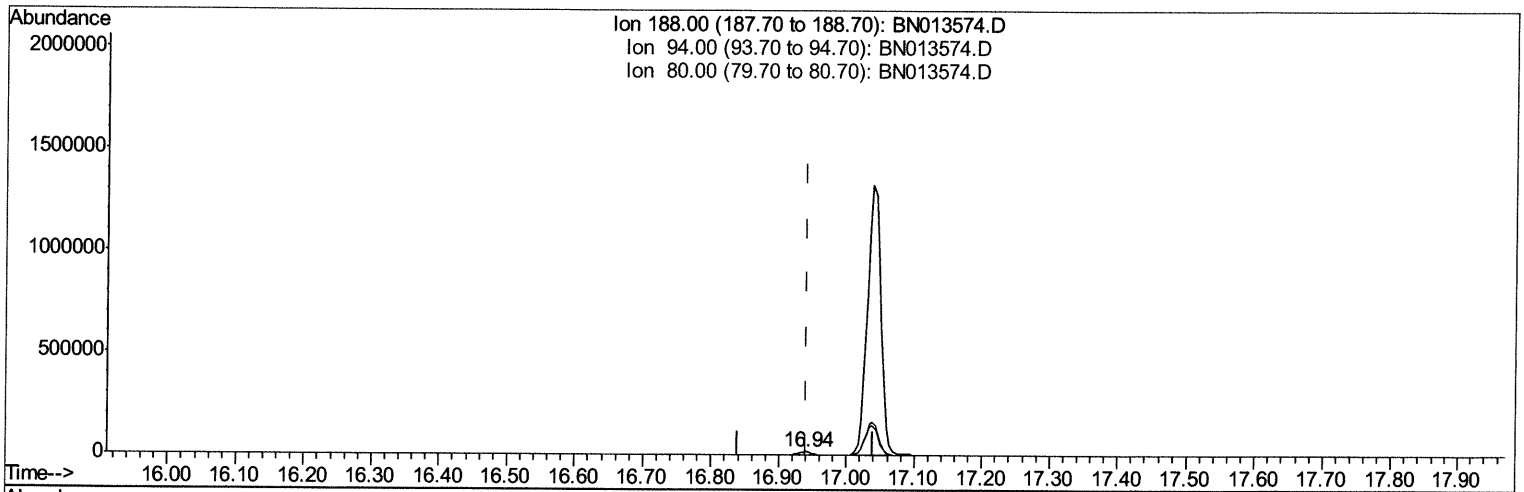

TIC: BN013574.D

(10) Phenanthrene-d10 (I)

16.941min (+0.001) 0.40ng/ul m 02/08/21 JU

response 21147

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	10.52
80.00	11.30	11.36
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020421\
 Data File : BN013574.D
 Acq On : 04 Feb 2021 16:42
 Operator : CG/JU
 Sample : M1299-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

mohammad
 2/8/2021 12:17:16 PM

Quant Time: Feb 04 17:13:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 04 14:51:05 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	4510	0.40	ng/ul	0.00
2) Naphthalene-d8	10.32	136	17182	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	10258	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	21147m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.15	240	19365	0.40	ng/ul	0.00
20) Perylene-d12	23.31	264	18642	0.40	ng/ul	0.00

02/08/21 JY

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.91	152	10067	0.41	ng/ul	0.00
14) Fluoranthene-d10	18.98	212	23150	0.45	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed