

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020421\
 Data File : BN013573.D
 Acq On : 04 Feb 2021 16:06
 Operator : CG/JU
 Sample : M1299-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CAA16

Manual Integrations
 APPROVED

mohammad
 2/8/2021 12:17:13 PM

Quant Time: Feb 04 16:55:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 04 14:51:05 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	5304	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	20500	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	11943	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	24265m	0.40	ng/ul	0.00
16) Chrysene-d12	21.14	240	21435	0.40	ng/ul	0.00
20) Perylene-d12	23.31	264	20078	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.91	152	11139	0.38	ng/ul	0.00
14) Fluoranthene-d10	18.98	212	23616	0.40	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.59	266	79	0.027	ng/ul	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN020421\
Data File : BN013573.D
Acq On : 04 Feb 2021 16:06
Operator : CG/JU
Sample : M1299-10
Misc :
ALS Vial : 10 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
CAA16

Manual Integrations
APPROVED

mohammad
2/8/2021 12:17:13 PM

Quant Time: Feb 04 16:55:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 04 14:51:05 2021
Response via : Initial Calibration

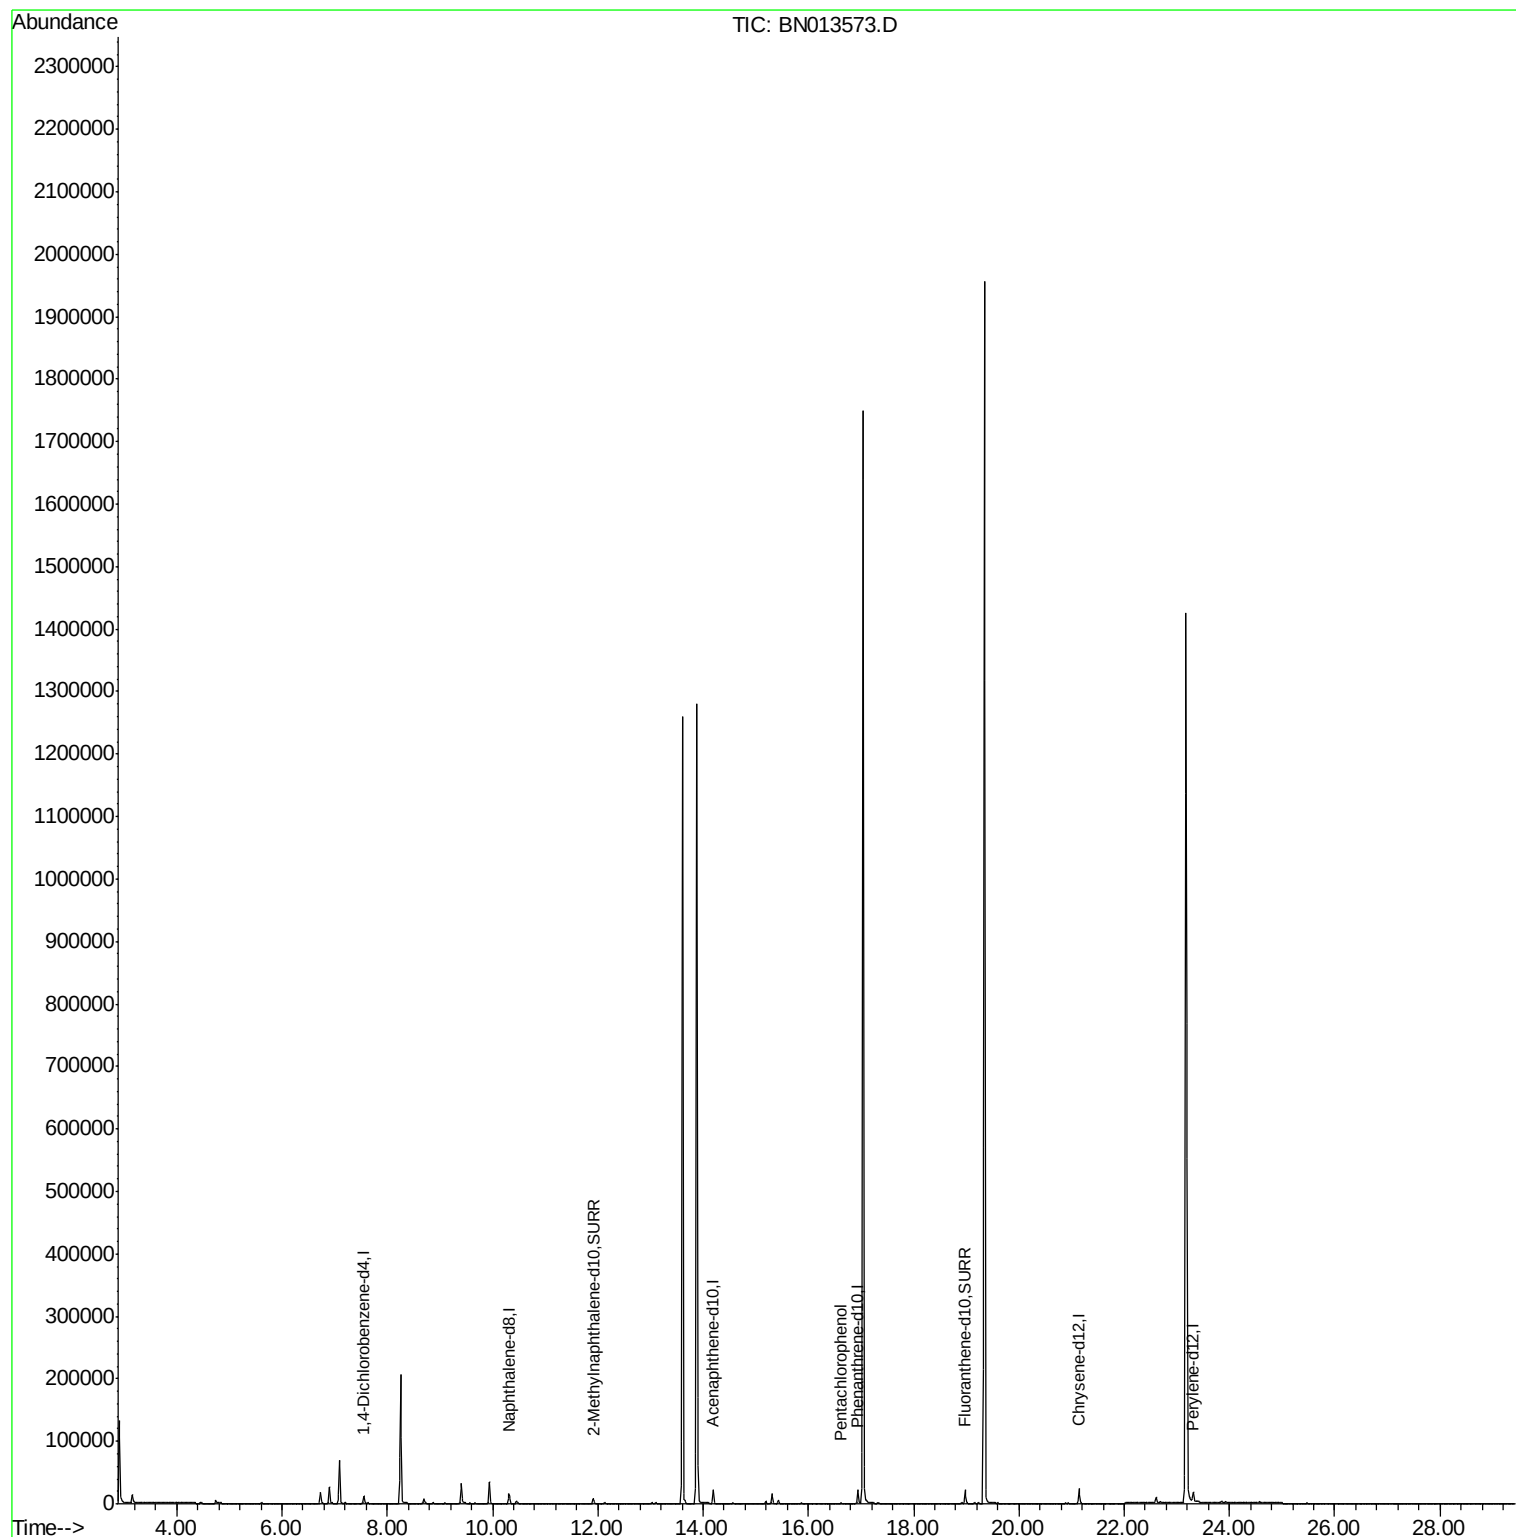

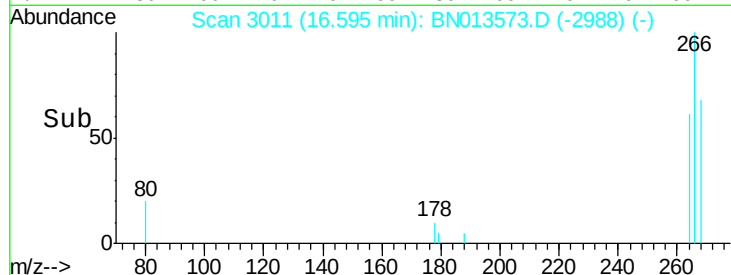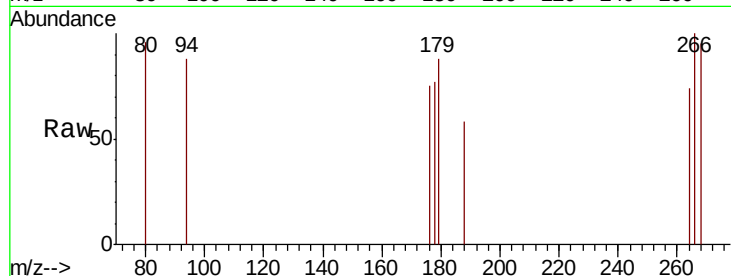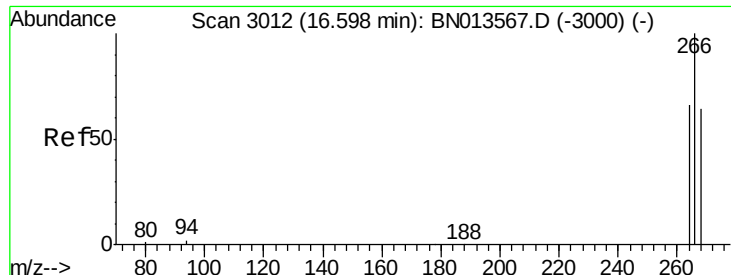

#11
 Pentachlorophenol
 Concen: 0.027 ng/ul
 RT: 16.59 min Scan# 3011
 Delta R.T. -0.00 min
 Lab File: BN013573.D
 Acq: 04 Feb 2021 16:06

Instrument :
 BNA_N
 ClientSampleId :
 CAA16

Tot Ion:	266	Resp:	79
Ion Ratio	Lower	Upper	
266	100		
264	50.6	49.9	74.9
268	64.6	51.2	76.8

Manual Integrations
 APPROVED

mohammad
 2/8/2021 12:17:13 PM

