

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020422\
 Data File : BN018578.D
 Acq On : 04 Feb 2022 11:45
 Operator : CG/JU
 Sample : N1307-18
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0Q61

Quant Time: Feb 04 12:19:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 02 14:08:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	634	0.400	ng/u1	0.00
4) Naphthalene-d8	10.728	136	2291	0.400	ng/u1 #	0.00
9) Acenaphthene-d10	14.553	164	1324	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.294	188	2592	0.400	ng/u1 #	0.00
17) Chrysene-d12	21.467	240	2125	0.400	ng/u1 #	0.00
23) Perylene-d12	23.864	264	2148	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	2452	3.368	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.317	152	1062	0.340	ng/u1	0.00
18) Fluoranthene-d10	19.318	212	2617	0.431	ng/u1	0.00
Target Compounds						
14) Pentachlorophenol	16.943	266	398	0.824	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020422\
Data File : BN018578.D
Acq On : 04 Feb 2022 11:45
Operator : CG/JU
Sample : N1307-18
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0Q61

Quant Time: Feb 04 12:19:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN020222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 02 14:08:46 2022
Response via : Initial Calibration

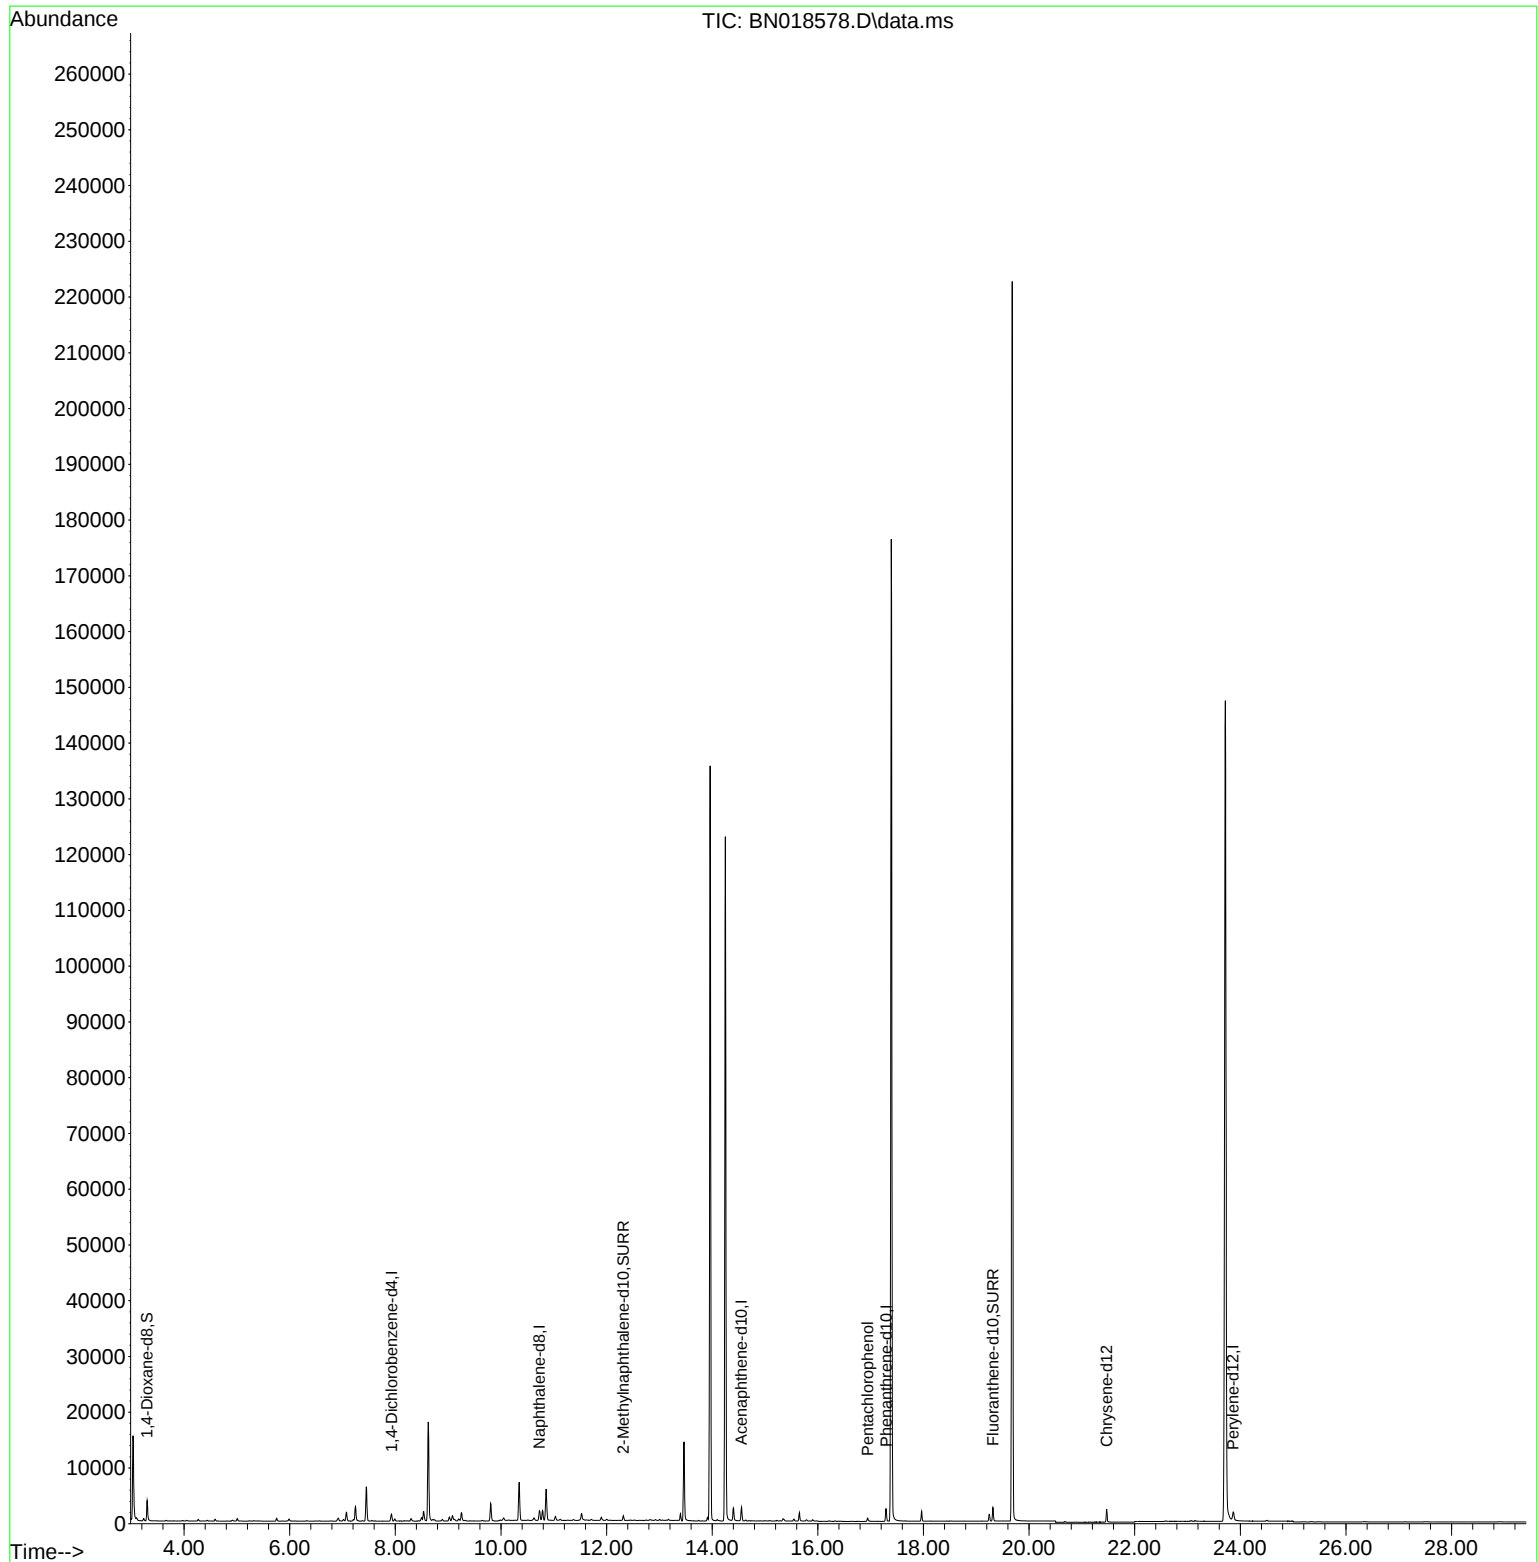

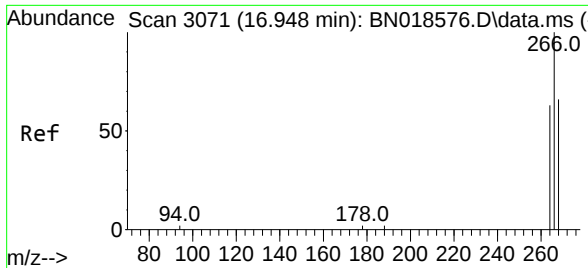

#14
 Pentachlorophenol
 Concen: 0.824 ng/ul
 RT: 16.943 min Scan# 3070
 Delta R.T. -0.004 min
 Lab File: BN018578.D
 Acq: 04 Feb 2022 11:45

Instrument :
 BNA_N
 ClientSampleId :
 C0Q61

Tgt Ion:	266	Resp:	398
Ion	Ratio	Lower	Upper
266	100		
264	61.6	49.9	74.9
268	63.3	51.7	77.5

