




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
Data File : BN036263.D
Acq On : 04 Feb 2025 16:56
Operator : RC/JU
Sample : Q1248-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6326

Manual IntegrationsAPPROVED

Quant Time: Feb 05 07:48:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/05/2025
Supervised By :mohammad ahmed 02/06/2025

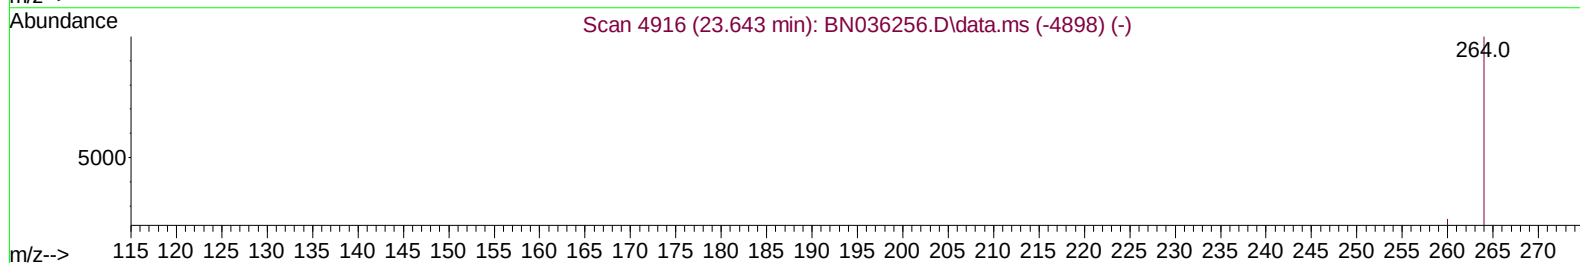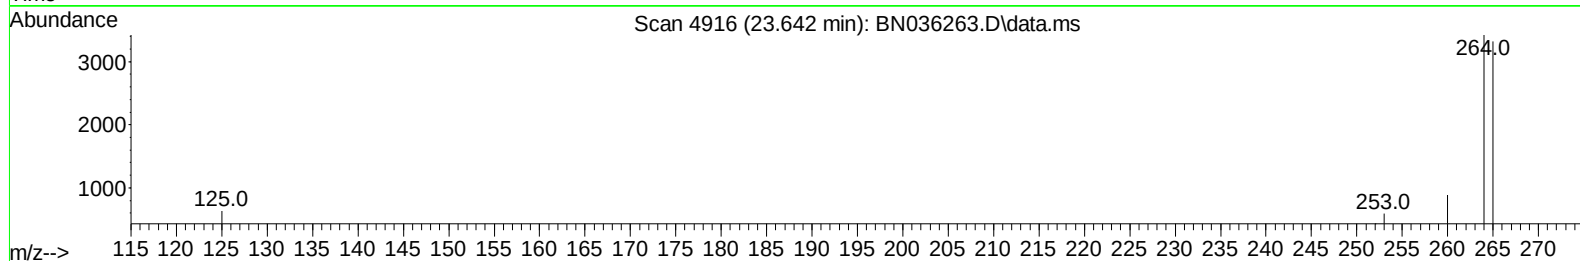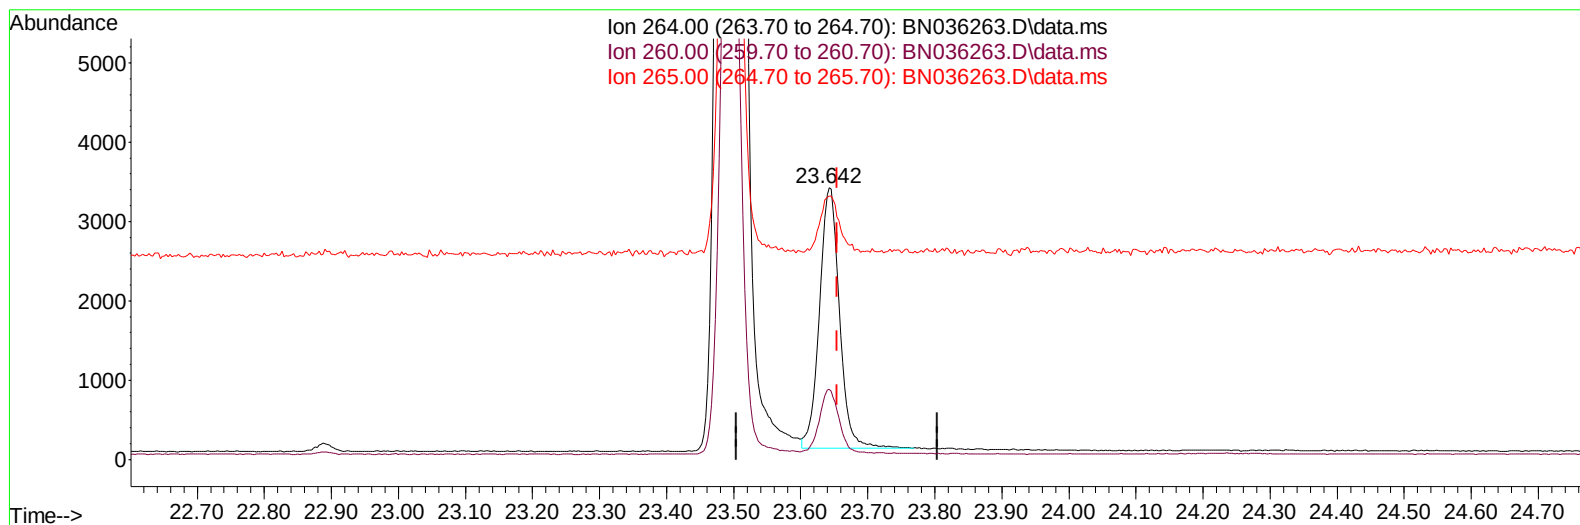

TIC: BN036263.D\data.ms

(23) Perylene-d12 (I)

23.642min (-0.012) 0.40 ng/u1

response 6754

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.83
265.00	53.20	96.93#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
Data File : BN036263.D
Acq On : 04 Feb 2025 16:56
Operator : RC/JU
Sample : Q1248-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6326

Manual IntegrationsAPPROVED

Quant Time: Feb 05 07:48:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/05/2025
Supervised By :mohammad ahmed 02/06/2025

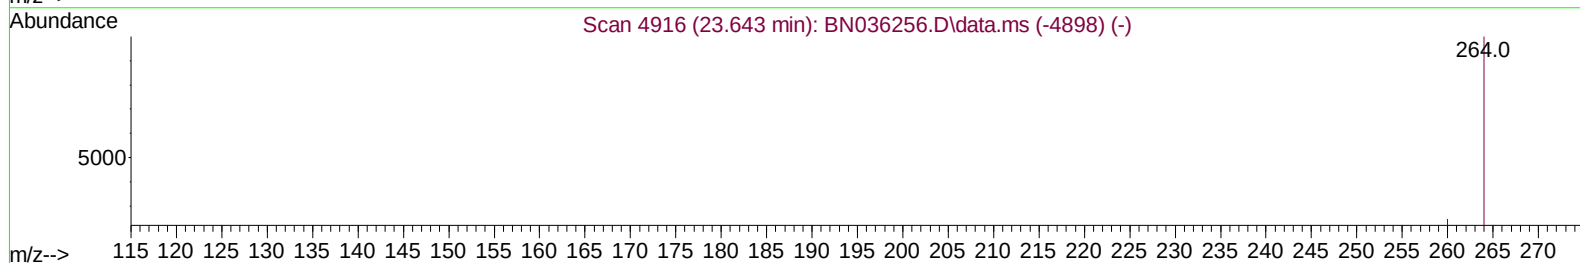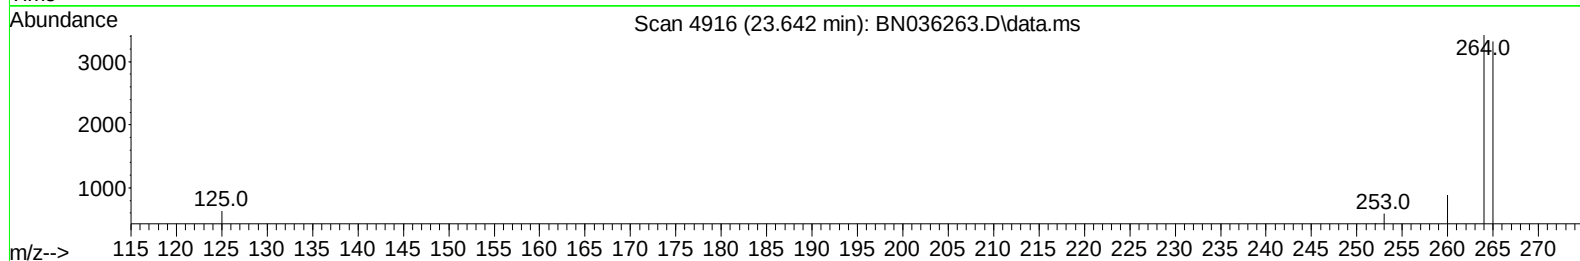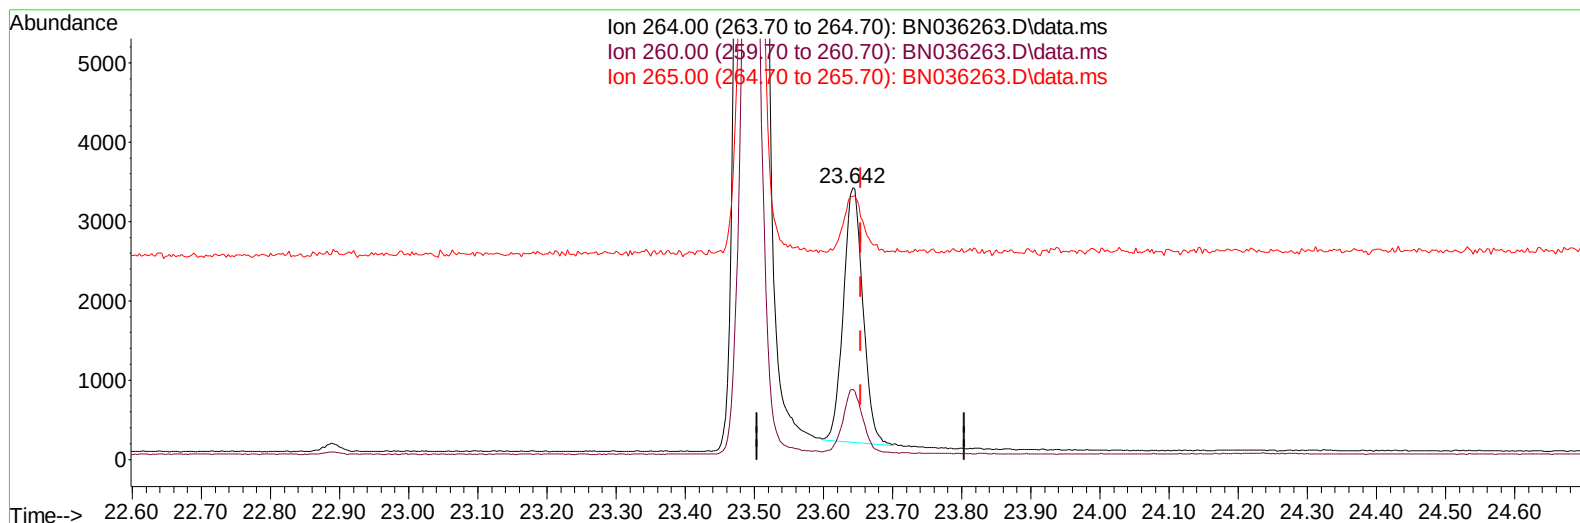

TIC: BN036263.D\data.ms

(23) Perylene-d12 (I)

23.642min (-0.012) 0.40 ng/ul m

response 6262

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	25.83
265.00	53.20	96.93#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
 Data File : BN036263.D
 Acq On : 04 Feb 2025 16:56
 Operator : RC/JU
 Sample : Q1248-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A6326

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/05/2025
 Supervised By :mohammad ahmed 02/06/2025

Quant Time: Feb 05 07:48:56 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 12:27:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.779	152	3266	0.400	ng/ul	0.00
4) Naphthalene-d8	10.568	136	8114	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.419	164	4462	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.163	188	7904	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.354	240	5992	0.400	ng/ul	# 0.00
23) Perylene-d12	23.642	264	6262m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	7984	2.233	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.163	152	2120	0.207	ng/ul	0.00
18) Fluoranthene-d10	19.193	212	3005	0.182	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
Data File : BN036263.D
Acq On : 04 Feb 2025 16:56
Operator : RC/JU
Sample : Q1248-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6326

Manual IntegrationsAPPROVED

Quant Time: Feb 05 07:48:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/05/2025
Supervised By :mohammad ahmed 02/06/2025

