




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
Data File : BN036266.D
Acq On : 04 Feb 2025 18:44
Operator : RC/JU
Sample : Q1248-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6333

Manual IntegrationsAPPROVED

Quant Time: Feb 05 07:54:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/05/2025
Supervised By :mohammad ahmed 02/06/2025

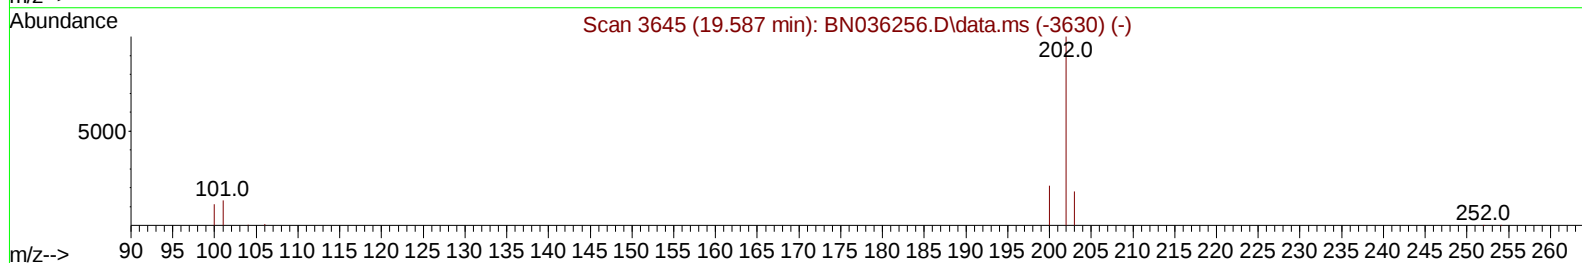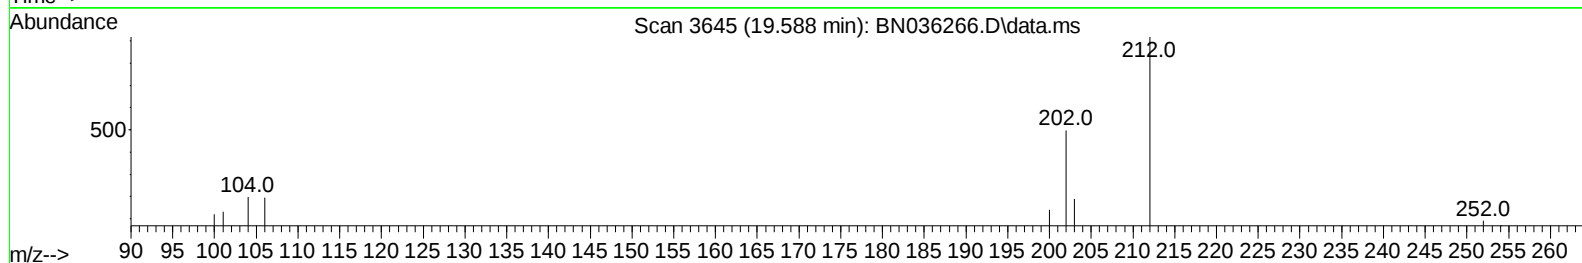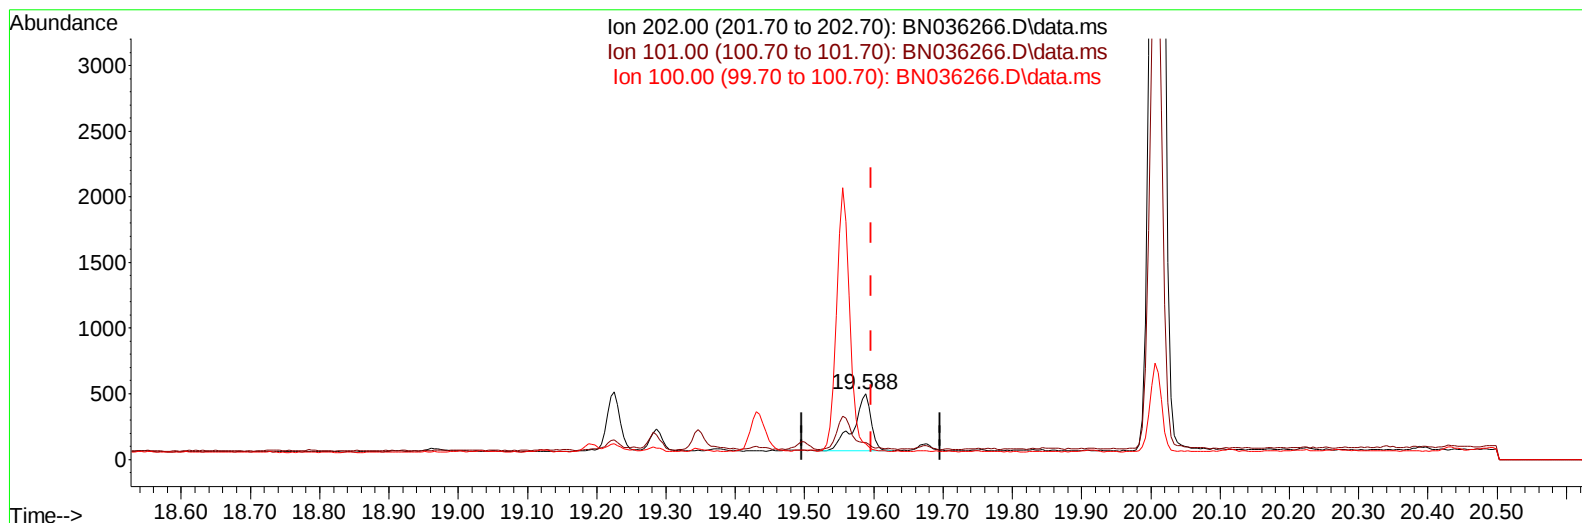

TIC: BN036266.D\data.ms

(20) Pyrene

19.588min (-0.008) 0.02 ng/u1

response 764

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	26.31#
100.00	9.40	24.30#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
Data File : BN036266.D
Acq On : 04 Feb 2025 18:44
Operator : RC/JU
Sample : Q1248-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6333

Manual IntegrationsAPPROVED

Quant Time: Feb 05 07:54:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/05/2025
Supervised By :mohammad ahmed 02/06/2025

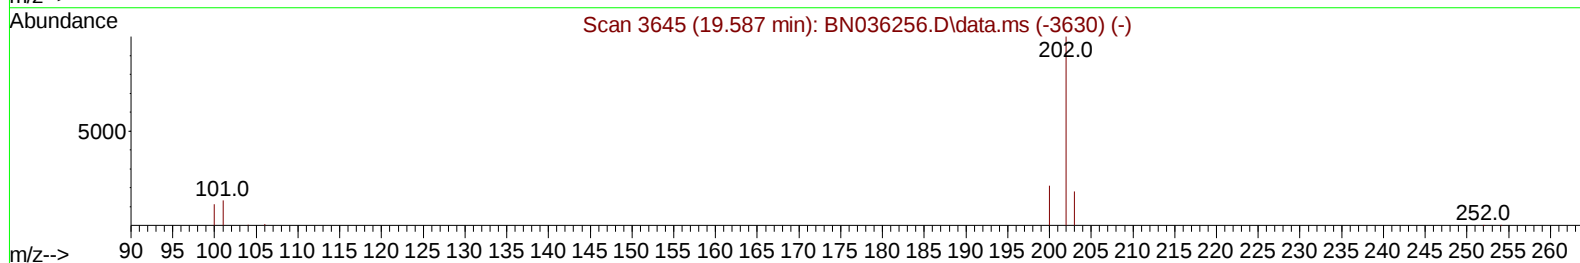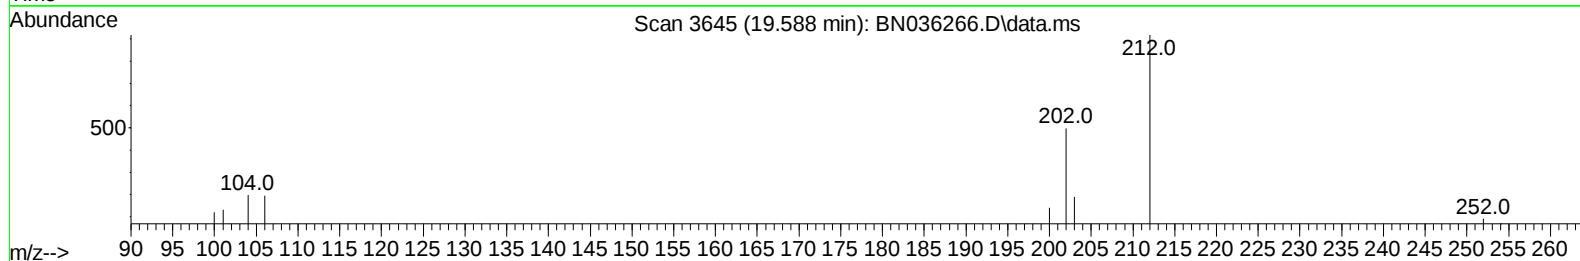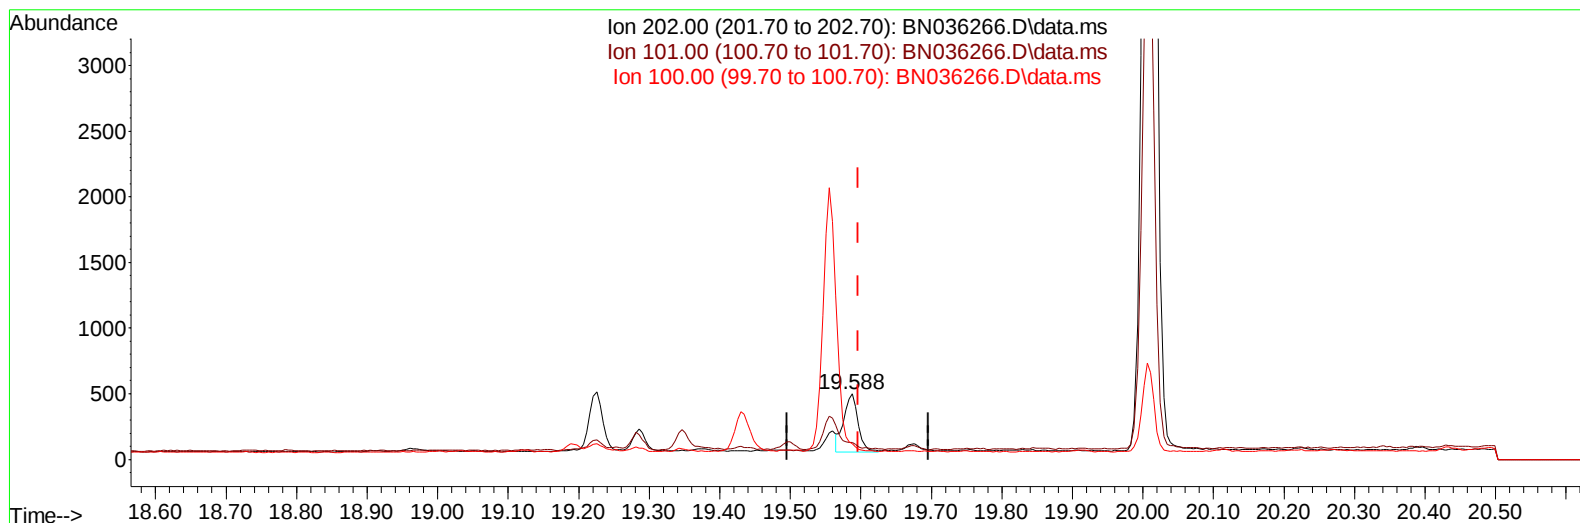

TIC: BN036266.D\data.ms

(20) Pyrene

19.588min (-0.008) 0.02 ng/u1 m

response 633

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	26.31#
100.00	9.40	24.30#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
 Data File : BN036266.D
 Acq On : 04 Feb 2025 18:44
 Operator : RC/JU
 Sample : Q1248-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A6333

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/05/2025
 Supervised By :mohammad ahmed 02/06/2025

Quant Time: Feb 05 07:54:10 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 12:27:24 2025
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.779	152		3038	0.400	ng/ul	0.00
4) Naphthalene-d8	10.568	136		7320	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.418	164		4211	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.163	188		8557	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.353	240		7930	0.400	ng/ul	# 0.00
23) Perylene-d12	23.639	264		8749	0.400	ng/ul	#-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.256	96		7691	2.312	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.162	152		2179	0.236	ng/ul	0.00
18) Fluoranthene-d10	19.193	212		3805	0.175	ng/ul	0.00
Target Compounds							Qvalue
20) Pyrene	19.588	202		633m	0.020	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
Data File : BN036266.D
Acq On : 04 Feb 2025 18:44
Operator : RC/JU
Sample : Q1248-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A6333

Manual IntegrationsAPPROVED

Quant Time: Feb 05 07:54:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/05/2025
Supervised By :mohammad ahmed 02/06/2025

