

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
 Data File : BN036266.D
 Acq On : 04 Feb 2025 18:44
 Operator : RC/JU
 Sample : Q1248-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A6333

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/05/2025
 Supervised By :mohammad ahmed 02/06/2025

Quant Time: Feb 05 07:54:10 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 12:27:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.779	152	3038	0.400	ng/u1	0.00
4) Naphthalene-d8	10.568	136	7320	0.400	ng/u1	-0.01
9) Acenaphthene-d10	14.418	164	4211	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.163	188	8557	0.400	ng/u1	#-0.01
17) Chrysene-d12	21.353	240	7930	0.400	ng/u1	# 0.00
23) Perylene-d12	23.639	264	8749	0.400	ng/u1	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	7691	2.312	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.162	152	2179	0.236	ng/u1	0.00
18) Fluoranthene-d10	19.193	212	3805	0.175	ng/u1	0.00
Target Compounds						Qvalue
20) Pyrene	19.588	202	633m	0.020	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
Data File : BN036266.D
Acq On : 04 Feb 2025 18:44
Operator : RC/JU
Sample : Q1248-07
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A6333

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/05/2025
Supervised By :mohammad ahmed 02/06/2025


Quant Time: Feb 05 07:54:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

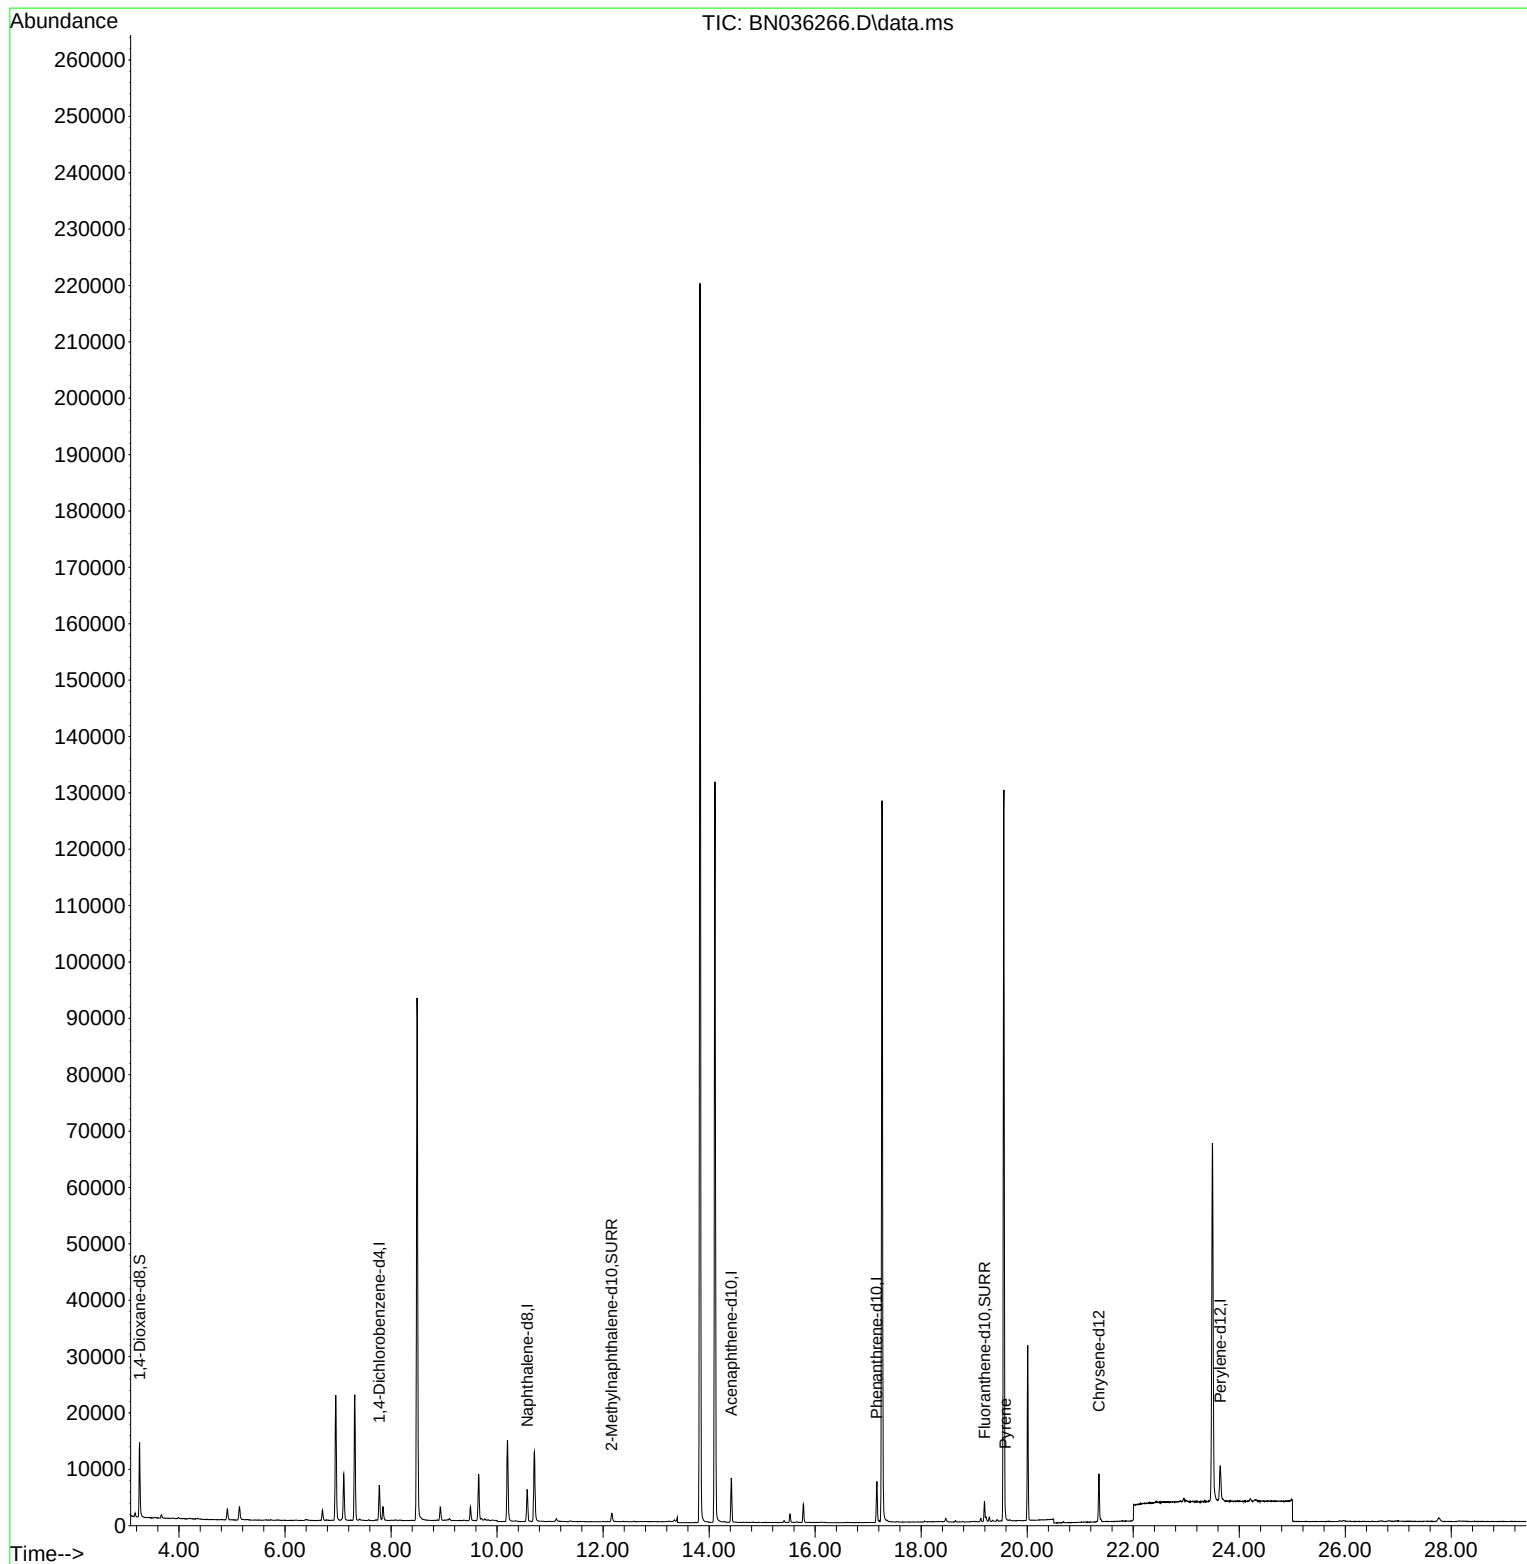

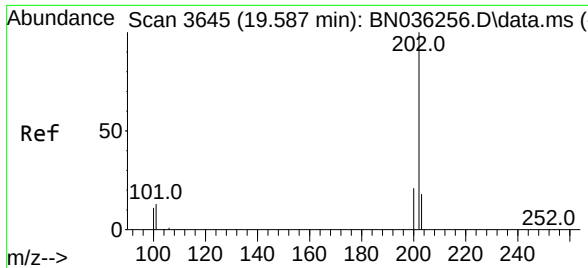

#20
Pyrene
Concen: 0.020 ng/ul m
RT: 19.588 min Scan# 30
Delta R.T. -0.008 min
Lab File: BN036266.D
Acq: 04 Feb 2025 18:44

Instrument :
BNA_N
ClientSampleId :
A6333

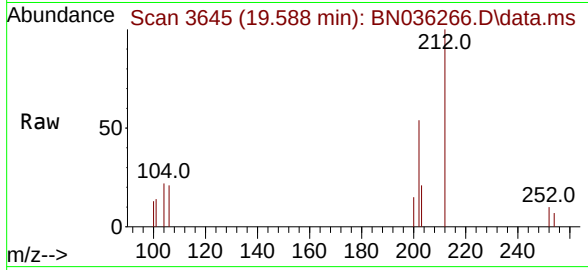

Tgt Ion:202 Resp: 63

Ion	Ratio	Lower	Upper
202	100		
101	26.3	9.3	13.9
100	24.3	7.5	11.3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/05/2025
Supervised By :mohammad ahmed 02/06/2025

