

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
 Data File : BN036276.D
 Acq On : 05 Feb 2025 01:19
 Operator : RC/JU
 Sample : Q1202-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2975

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/05/2025
 Supervised By :mohammad ahmed 02/06/2025

Quant Time: Feb 05 08:13:11 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 12:27:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.779	152	2691	0.400	ng/ul	0.00
4) Naphthalene-d8	10.568	136	6149	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.419	164	3375	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.163	188	6451m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.351	240	5906	0.400	ng/ul	#-0.01
23) Perylene-d12	23.633	264	5849m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	14350	4.870	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.163	152	2439	0.314	ng/ul	0.00
18) Fluoranthene-d10	19.193	212	5989	0.369	ng/ul	0.00
Target Compounds						Qvalue
16) Anthracene	17.294	178	2315	0.132	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020425\
Data File : BN036276.D
Acq On : 05 Feb 2025 01:19
Operator : RC/JU
Sample : Q1202-01
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E2975

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/05/2025
Supervised By :mohammad ahmed 02/06/2025


Quant Time: Feb 05 08:13:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 03 12:27:24 2025
Response via : Initial Calibration

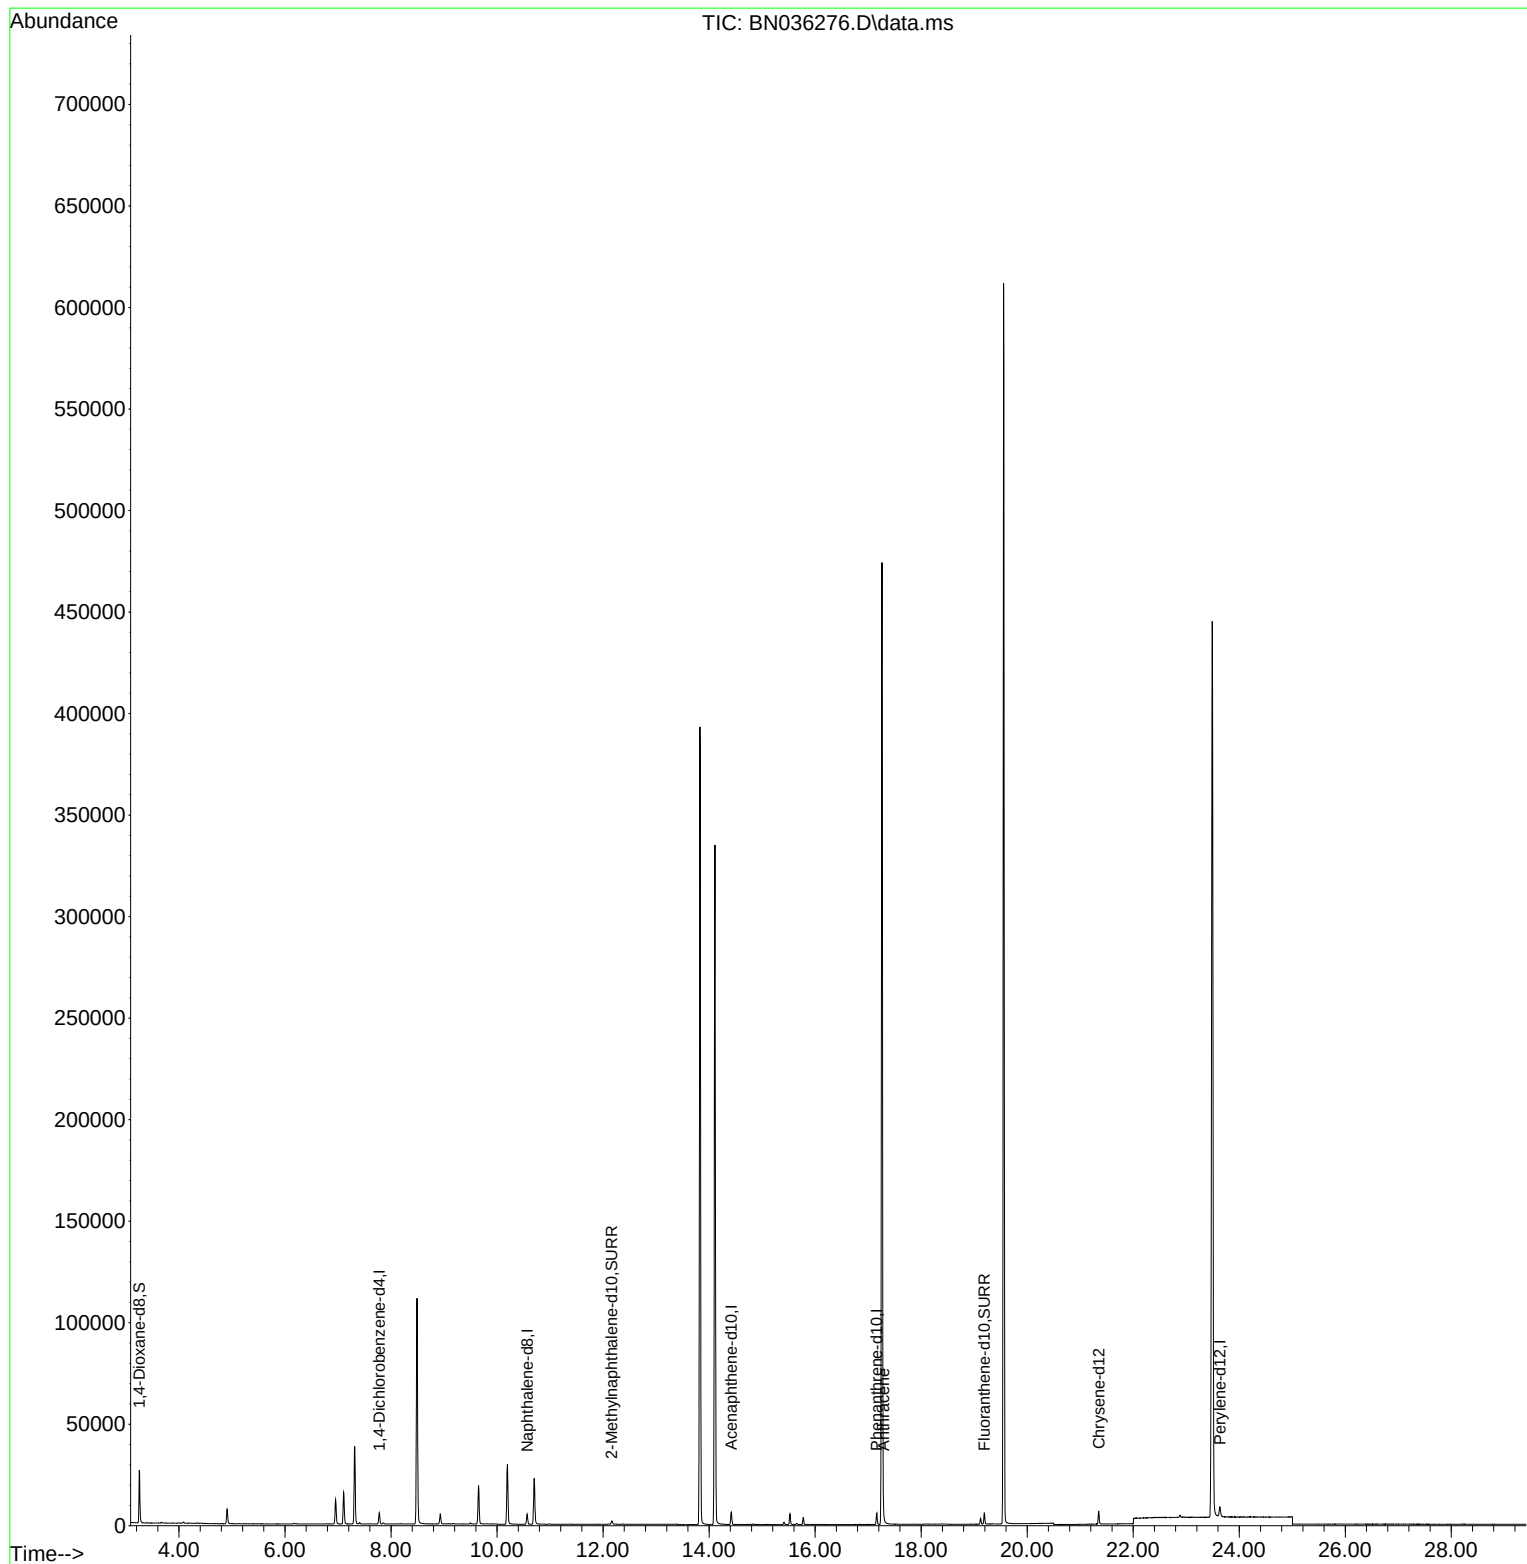

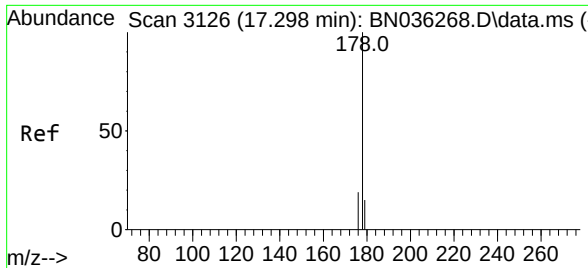

#16
 Anthracene
 Concen: 0.132 ng/ul
 RT: 17.294 min Scan# 3125
 Delta R.T. -0.012 min
 Lab File: BN036276.D
 Acq: 05 Feb 2025 01:19

Instrument :
 BNA_N
 ClientSampleId :
 E2975

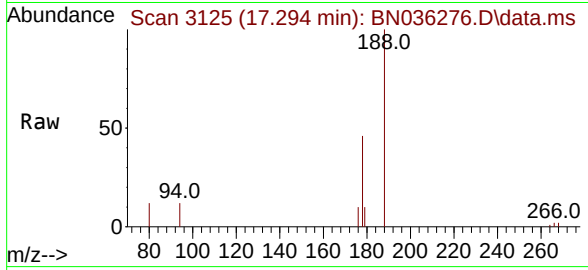

Tgt Ion:178 Resp: 2315

Ion	Ratio	Lower	Upper
178	100		
179	21.3	13.0	19.4
176	22.8	15.9	23.9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/05/2025
 Supervised By :mohammad ahmed 02/06/2025

