
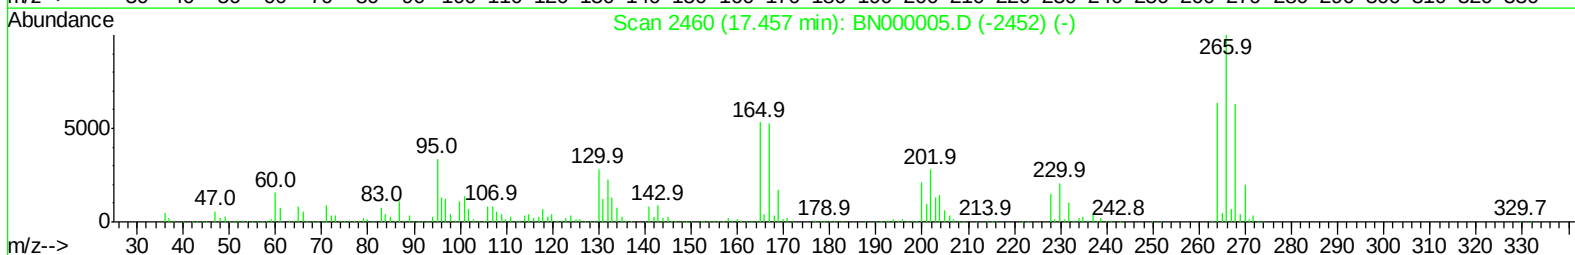
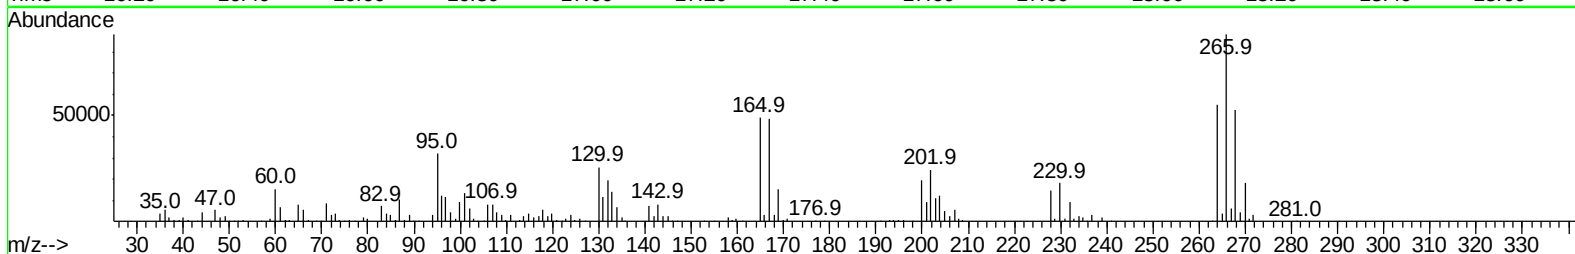


Data Path : U:\HPCHEM1\BNA N\DATA\BN020518\
Data File : BN000010.D
Acq On : 05 Feb 2018 09:14
Operator :
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 06:06:24 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 19:48:39 2018
Response via : Initial Calibration

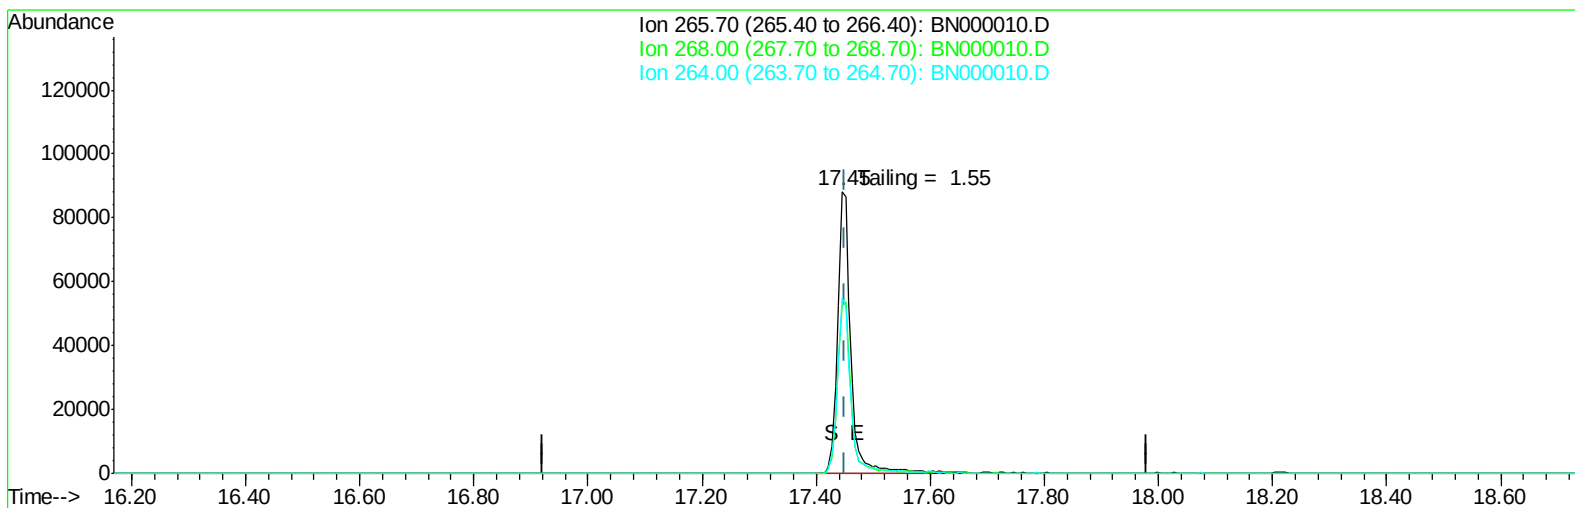

TIC: BN000010.D

(69) Pentachlorophenol (C)




17.445min (-0.006) 13678.26ng

response 140688

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.56
264.00	62.00	62.26
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA N\DATA\BN020518\
 Data File : BN000010.D
 Acq On : 05 Feb 2018 09:14
 Operator :
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 06:06:24 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 19:48:39 2018
 Response via : Initial Calibration

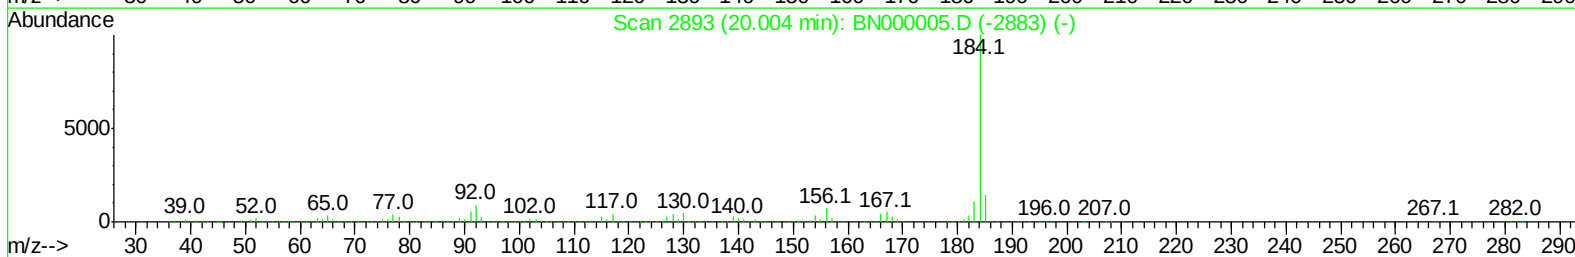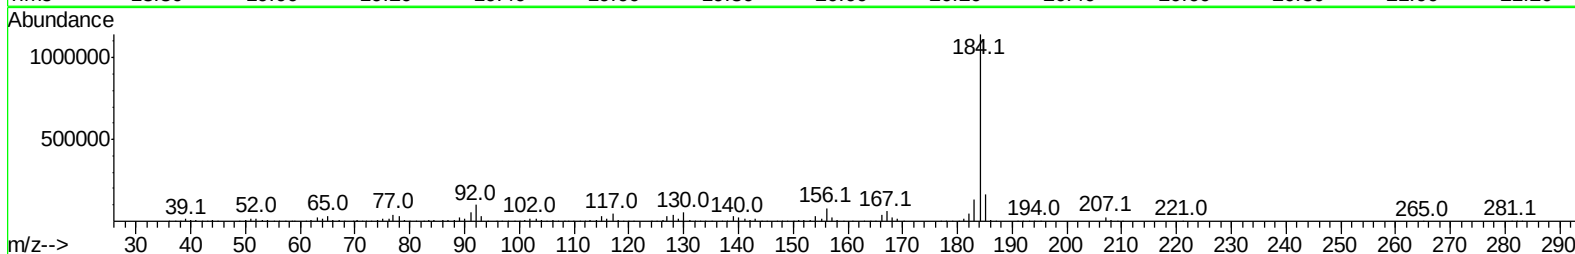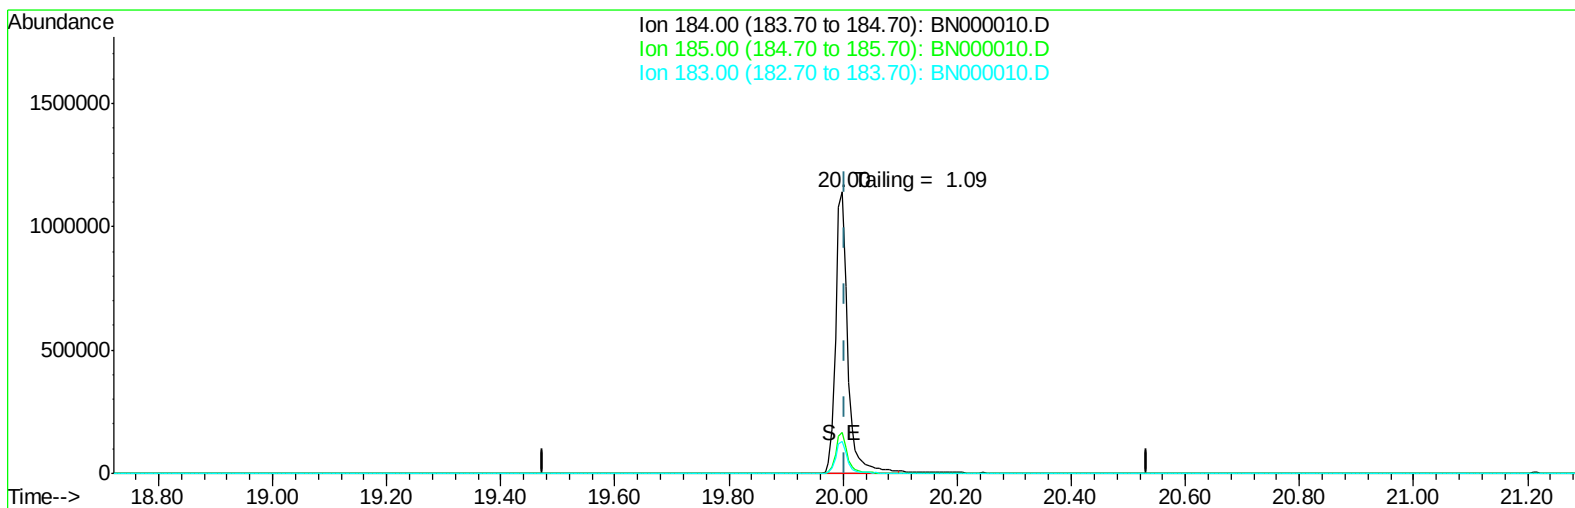

TIC: BN000010.D

(76) Benzidine

19.998min (-0.006) 0.00ng

response 1694130

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.36
183.00	13.30	11.47
0.00	0.00	0.00