


Data Path : Z:\HPCHEM1\BNA N\Data\BN020518\
 Data File : BN000010.D
 Acq On : 05 Feb 2018 09:14
 Operator :
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 06 15:24:10 2018

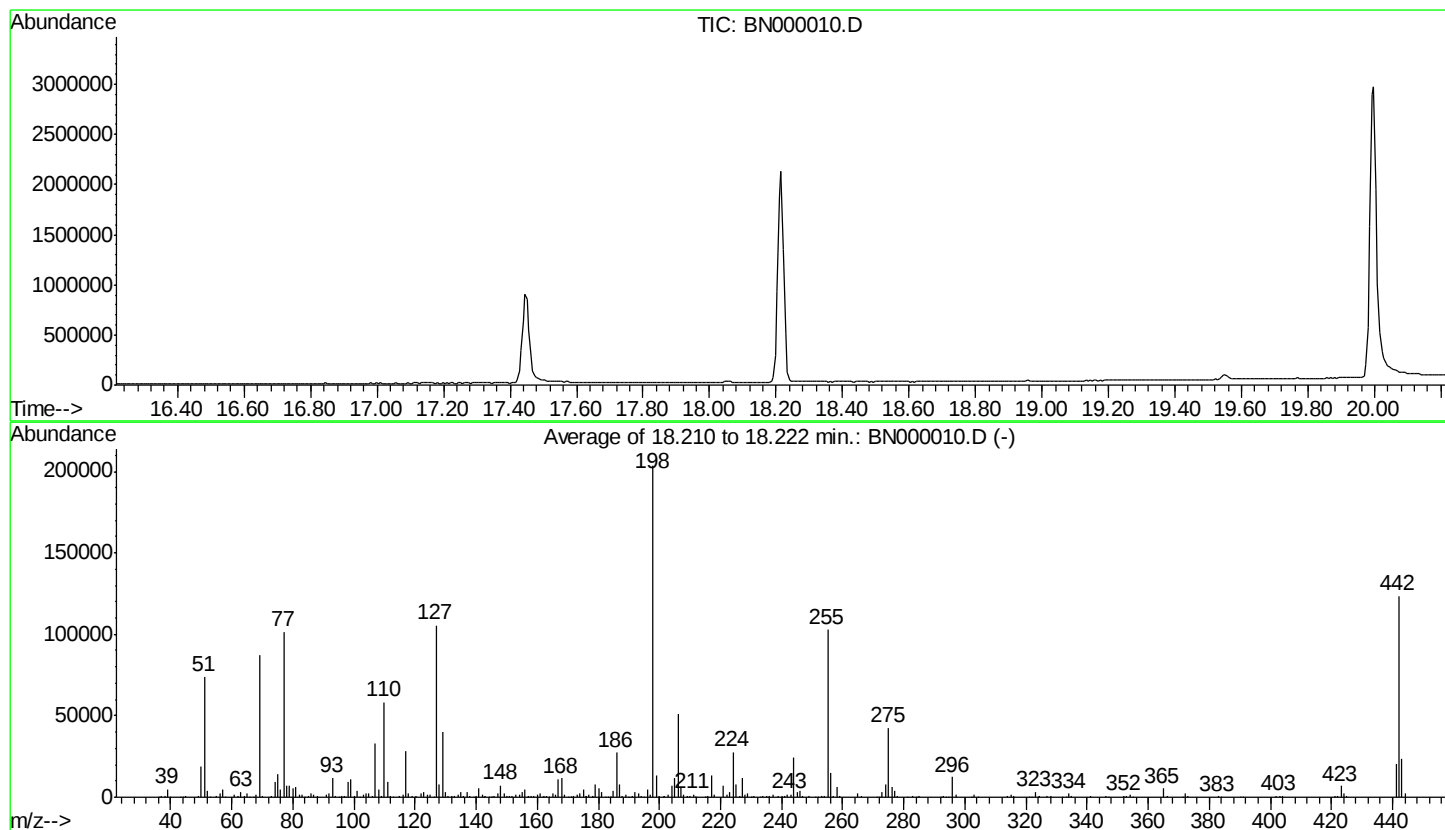

AutoFind: Scans 2588, 2589, 2590; Background Corrected with Scan 2581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	73885	PASS
68	69	0.00	2	1.8	1590	PASS
69	198	0.00	100	42.7	86864	PASS
70	69	0.00	2	0.7	624	PASS
127	198	10	80	51.8	105498	PASS
197	198	0.00	2	0.6	1267	PASS
198	198	100	100	100.0	203562	PASS
199	198	5	9	6.7	13674	PASS
275	198	10	60	21.0	42773	PASS
365	198	1	100	2.6	5225	PASS
441	443	0.01	100	86.2	20245	PASS
442	198	50	100	60.7	123600	PASS
443	442	15	24	19.0	23488	PASS