
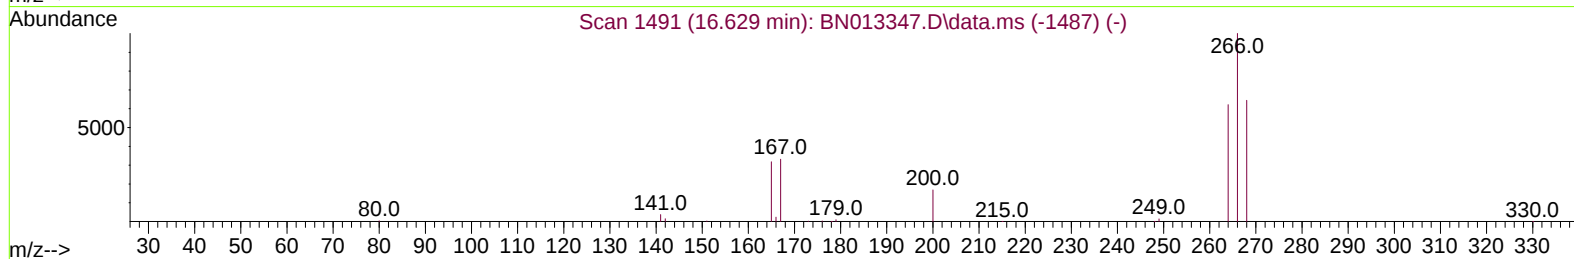
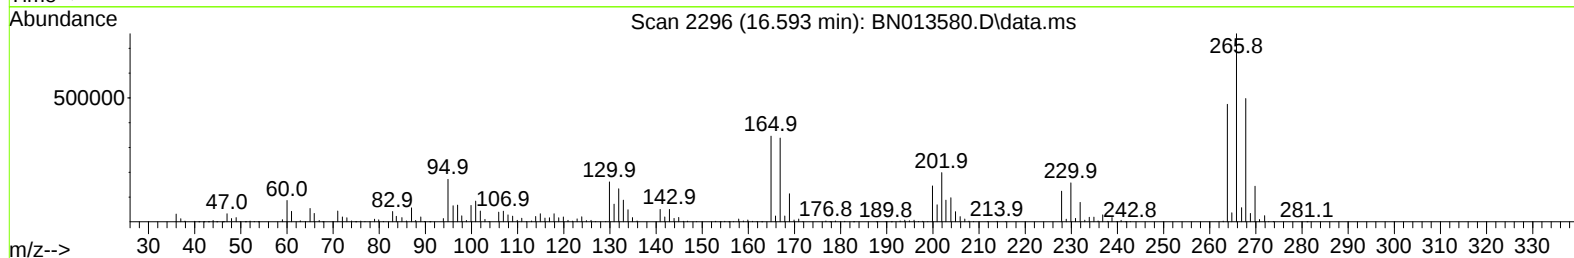


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020521\
 Data File : BN013580.D
 Acq On : 05 Feb 2021 09:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 04:13:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 05 11:21:14 2021
 Response via : Initial Calibration

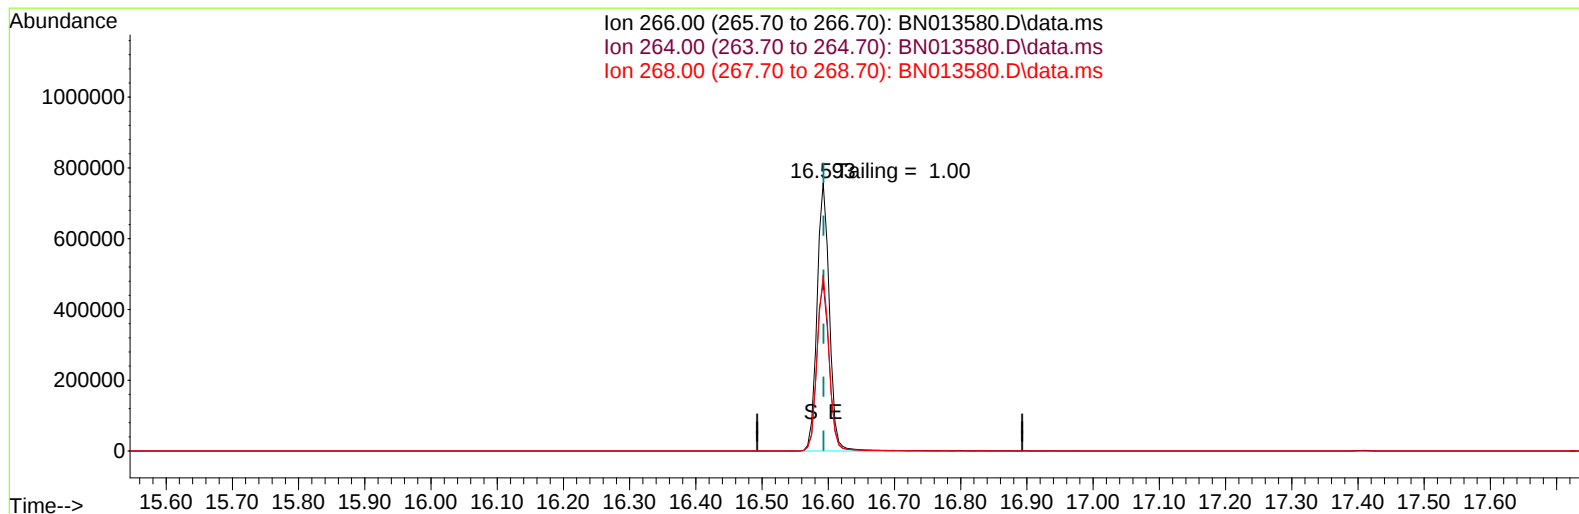

TIC: BN013580.D\data.ms

(24) Pentachlorophenol

16.593min (-0.000) 0.00 ng

response 980712

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	63.01
268.00	68.30	64.37
0.00	0.00	0.00