


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020521\
 Data File : BN013580.D
 Acq On : 05 Feb 2021 09:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 05 11:21:14 2021

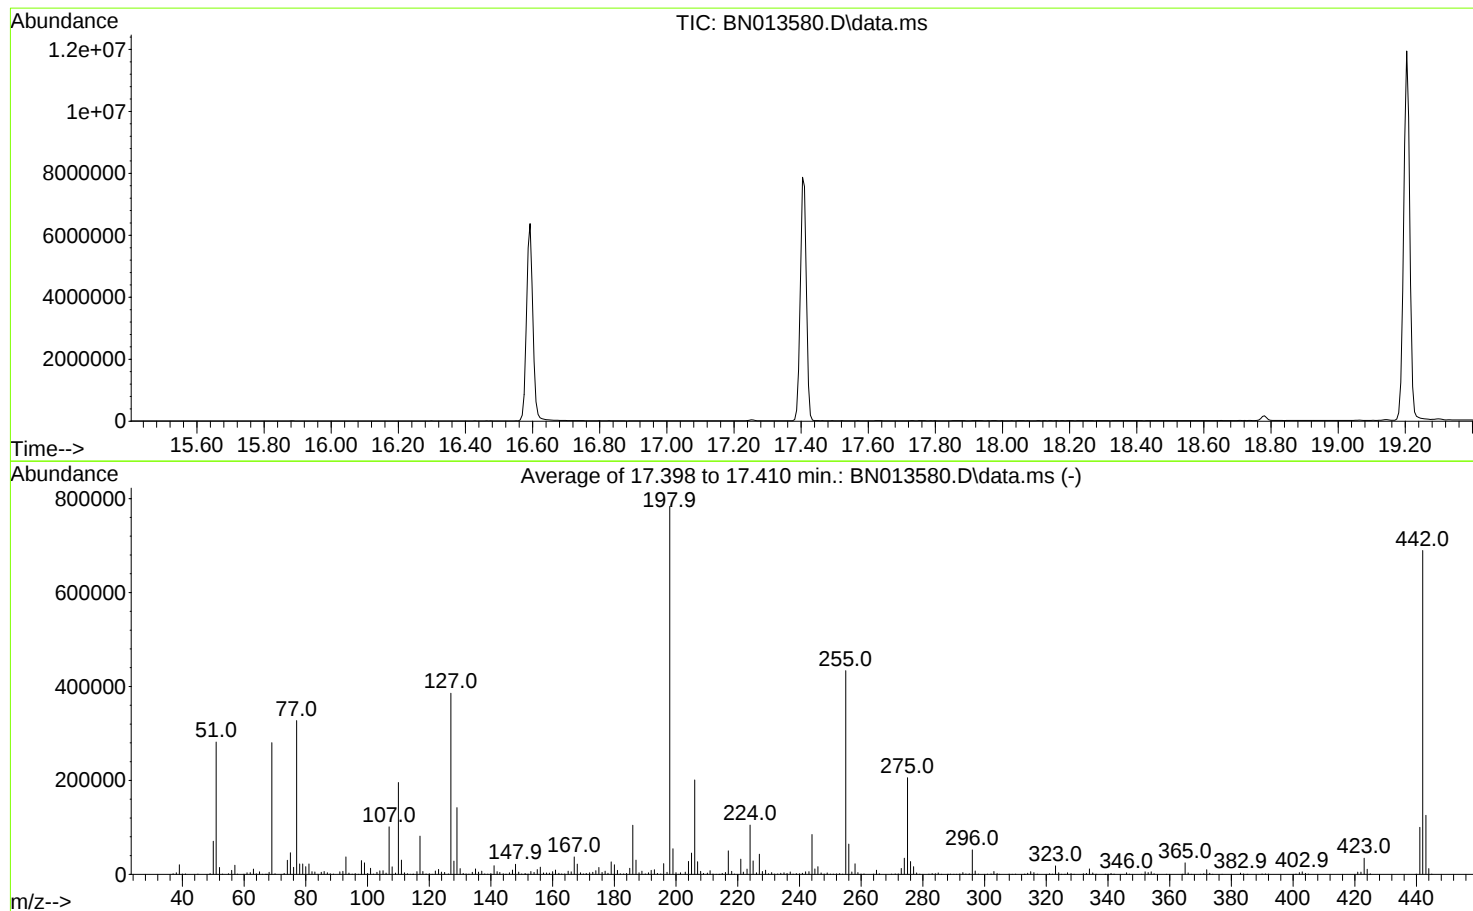

AutoFind: Scans 2433, 2434, 2435; Background Corrected with Scan 2426

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	281857	PASS
68	69	0.00	2	1.6	4541	PASS
69	198	0.00	100	35.8	280235	PASS
70	69	0.00	2	0.5	1483	PASS
127	198	10	80	49.3	385749	PASS
197	198	0.00	2	0.6	4432	PASS
198	198	100	100	100.0	783189	PASS
199	198	5	9	6.9	54376	PASS
275	198	10	60	26.3	205675	PASS
365	198	1	100	3.1	24610	PASS
441	198	0.01	100	12.8	100267	PASS
442	442	50	100	100.0	689515	PASS
443	442	15	24	18.2	125664	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/5/2021	BNA_N	<u>BN013580.D</u>
Compound Name	Response	Retention Time
DDT	2869043	20.451
DDD	22460	20.004
DDE	3053	19.492
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25513	2894556	0.88

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020521\
 Data File : BN013580.D
 Acq On : 05 Feb 2021 09:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Feb 06 04:13:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 05 11:21:14 2021
 Response via : Initial Calibration

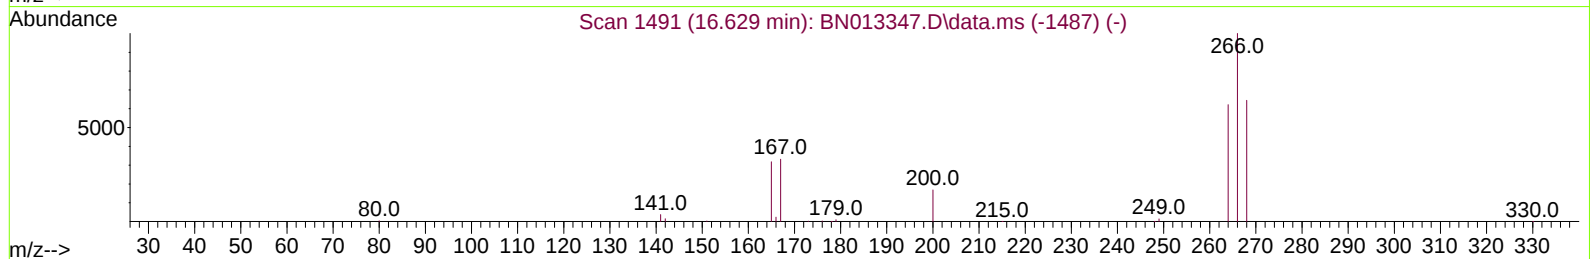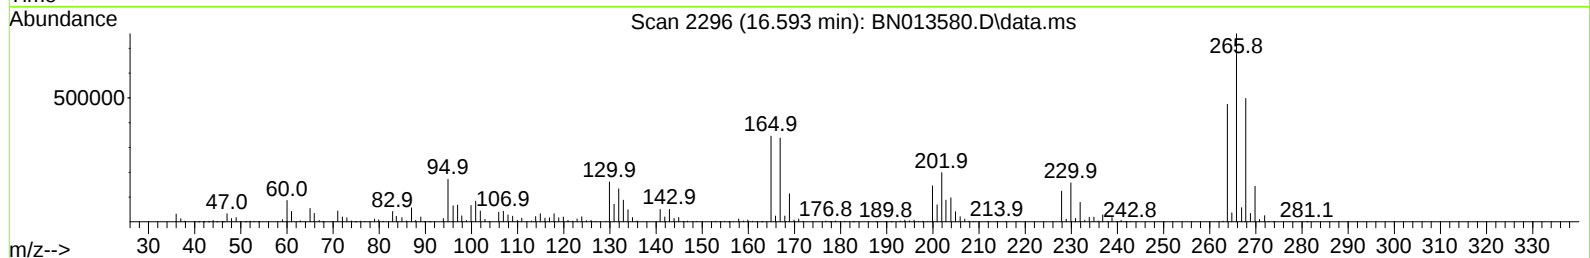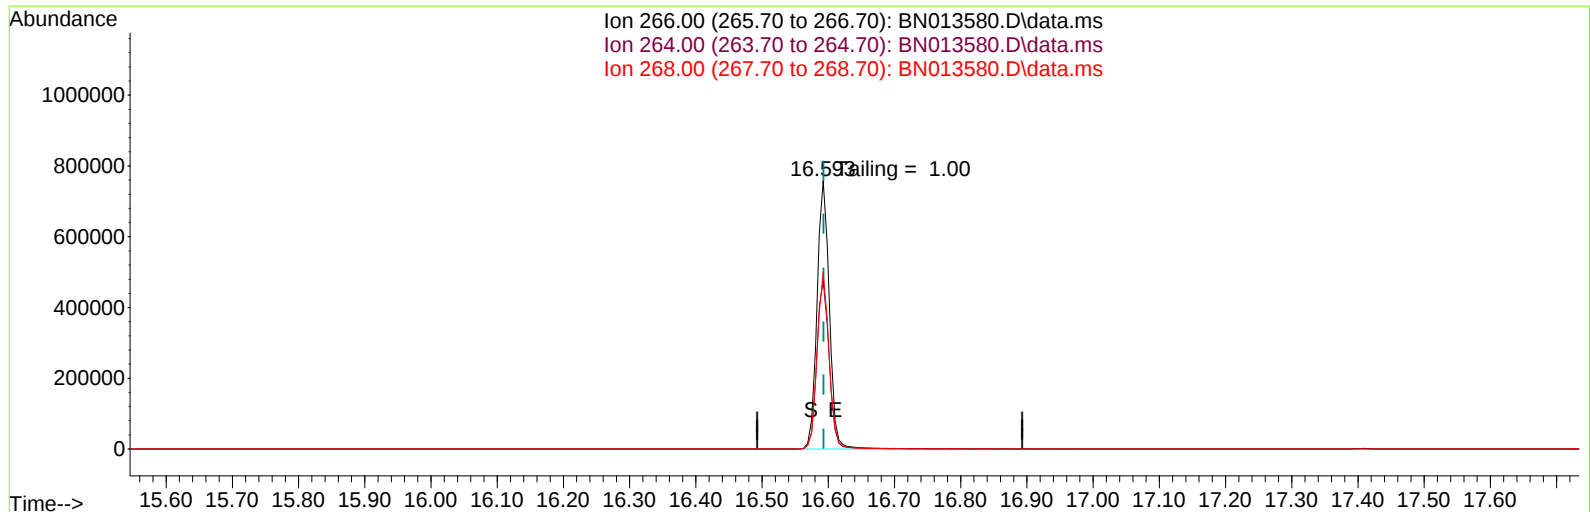

TIC: BN013580.D\data.ms

(24) Pentachlorophenol

16.593min (-0.000) 0.00 ng

response 980712

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	63.01
268.00	68.30	64.37
0.00	0.00	0.00