

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
 Data File : BN029504.D
 Acq On : 05 Feb 2024 12:45
 Operator : MA/JU
 Sample : PB158799BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB158799BS

Quant Time: Feb 05 13:14:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 01:51:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.890	152	5379	0.400	ng	0.00
7) Naphthalene-d8	10.690	136	14412	0.400	ng	0.00
13) Acenaphthene-d10	14.532	164	6125	0.400	ng	0.00
19) Phenanthrene-d10	17.280	188	10628	0.400	ng	0.00
29) Chrysene-d12	21.483	240	5736	0.400	ng	0.00
35) Perylene-d12	23.864	264	5376	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.464	112	4899	0.379	ng	0.00
5) Phenol-d6	7.060	99	5747	0.385	ng	0.00
8) Nitrobenzene-d5	9.057	82	4045	0.337	ng	0.00
11) 2-Methylnaphthalene-d10	12.280	152	8208	0.418	ng	0.00
14) 2,4,6-Tribromophenol	16.026	330	610	0.310	ng	0.00
15) 2-Fluorobiphenyl	13.164	172	9121	0.347	ng	0.00
27) Fluoranthene-d10	19.317	212	7055	0.274	ng	0.00
31) Terphenyl-d14	19.926	244	4932	0.346	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.377	88	2525	0.333	ng	# 57
3) n-Nitrosodimethylamine	3.702	42	1794	0.291	ng	# 84
6) bis(2-Chloroethyl)ether	7.327	93	4771	0.335	ng	98
9) Naphthalene	10.744	128	12603	0.307	ng	99
10) Hexachlorobutadiene	11.021	225	2261	0.290	ng	# 99
12) 2-Methylnaphthalene	12.355	142	7259	0.301	ng	99
16) Acenaphthylene	14.254	152	9400	0.323	ng	99
17) Acenaphthene	14.596	154	5980	0.306	ng	98
18) Fluorene	15.580	166	7138	0.291	ng	100
20) 4,6-Dinitro-2-methylph...	15.667	198	457	0.293	ng	# 62
21) 4-Bromophenyl-phenylether	16.486	248	1989	0.314	ng	# 68
22) Hexachlorobenzene	16.573	284	2337	0.301	ng	99
23) Atrazine	16.759	200	1318	0.293	ng	99
24) Pentachlorophenol	16.933	266	775	0.315	ng	98
25) Phenanthrene	17.317	178	9848	0.313	ng	98
26) Anthracene	17.417	178	8231	0.307	ng	100
28) Fluoranthene	19.350	202	8922	0.252	ng	100
30) Pyrene	19.712	202	9222	0.349	ng	100
32) Benzo(a)anthracene	21.465	228	5911	0.302	ng	99
33) Chrysene	21.519	228	6740	0.303	ng	100
34) Bis(2-ethylhexyl)phtha...	21.420	149	3822	0.286	ng	98
36) Indeno(1,2,3-cd)pyrene	26.329	276	6895	0.319	ng	# 89
37) Benzo(b)fluoranthene	23.142	252	6059	0.315	ng	92
38) Benzo(k)fluoranthene	23.192	252	5825	0.289	ng	# 89
39) Benzo(a)pyrene	23.759	252	5166	0.308	ng	# 89
40) Dibenzo(a,h)anthracene	26.355	278	5448	0.317	ng	97
41) Benzo(g,h,i)perylene	27.080	276	6352	0.303	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029504.D
Acq On : 05 Feb 2024 12:45
Operator : MA/JU
Sample : PB158799BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB158799BS


Quant Time: Feb 05 13:14:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 01:51:59 2024
Response via : Initial Calibration

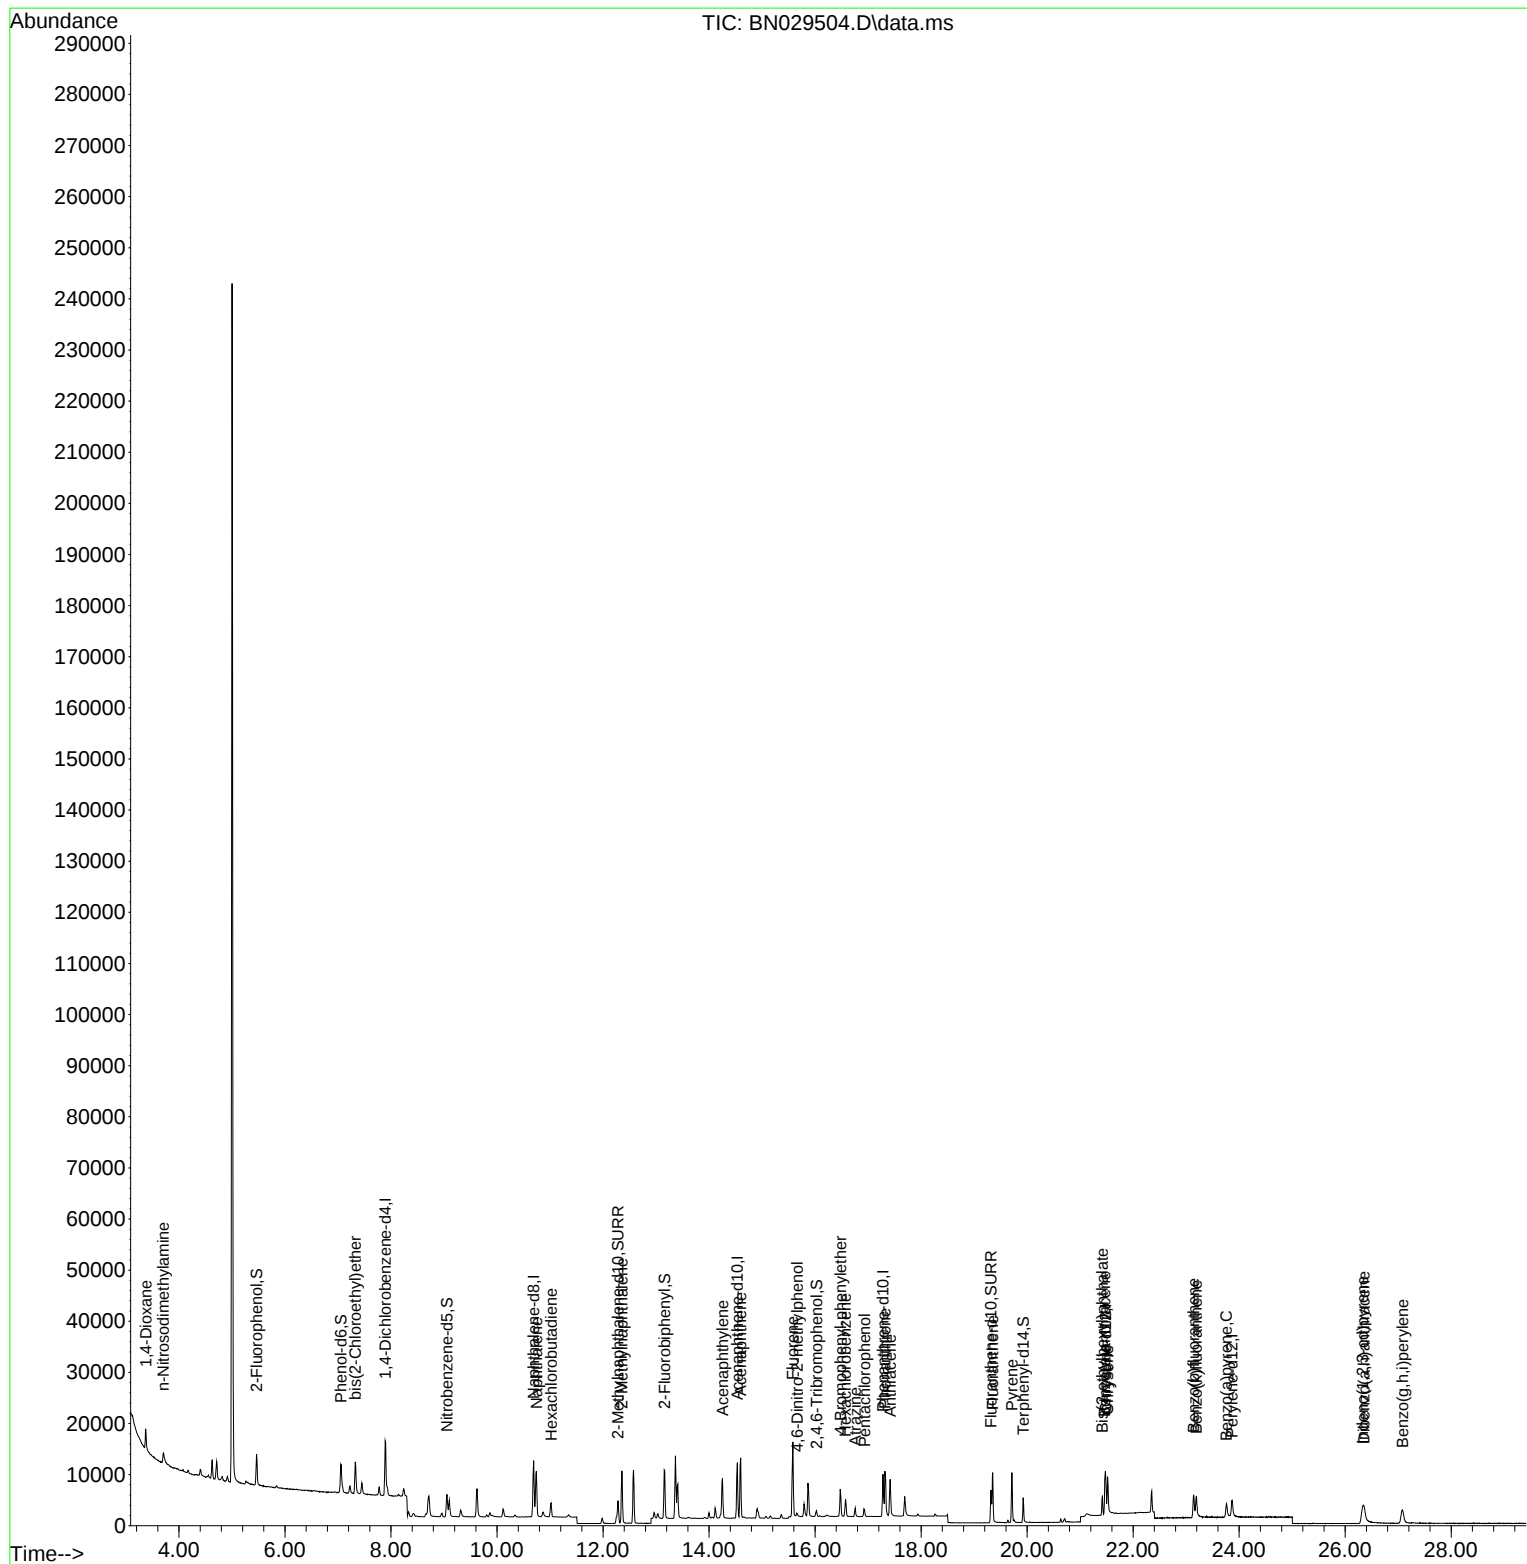





#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.890 min Scan# 668
Delta R.T. -0.008 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Instrument :
BNA_N
ClientSampleId :
PB158799BS







Tgt Ion:152 Resp: 5379
Ion Ratio Lower Upper
152 100
150 156.9 123.0 184.4
115 66.2 51.4 77.0

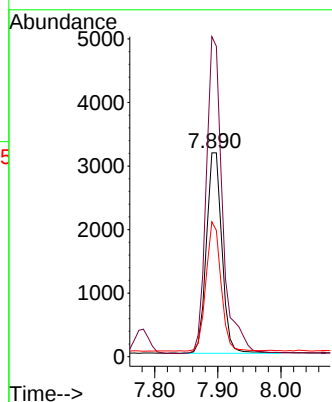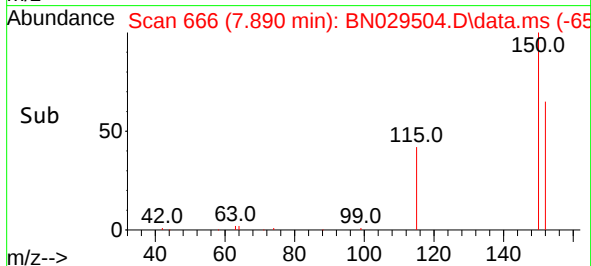

#2
1,4-Dioxane
Concen: 0.333 ng
RT: 3.377 min Scan# 41
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion: 88 Resp: 2525
Ion Ratio Lower Upper
88 100
43 89.9 23.3 34.9#
58 76.6 53.8 80.6



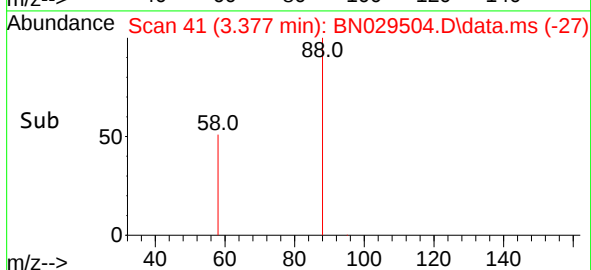
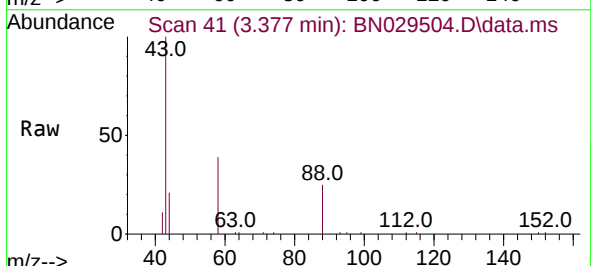


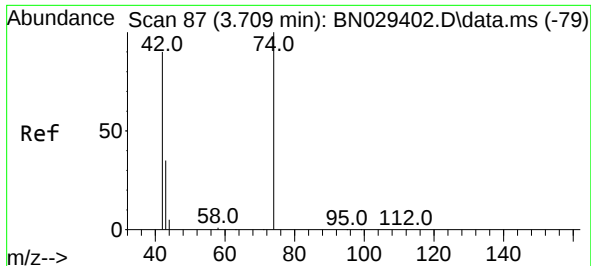

#3
 n-Nitrosodimethylamine
 Concen: 0.291 ng
 RT: 3.702 min Scan# 80
 Delta R.T. -0.007 min
 Lab File: BN029504.D
 Acq: 05 Feb 2024 12:45




Instrument :
 BNA_N
 ClientSampleId :
 PB158799BS

Tgt Ion: 42 Resp: 1794
 Ion Ratio Lower Upper
 42 100
 74 132.3 93.7 140.5
 44 4.3 13.0 19.4#

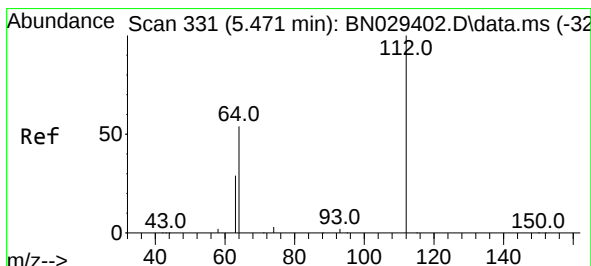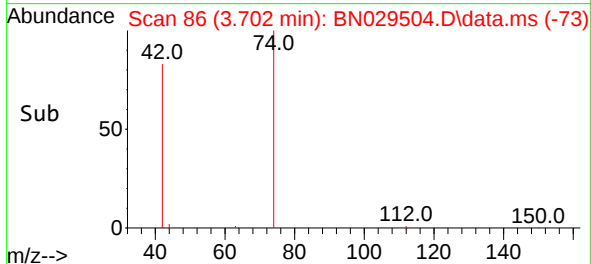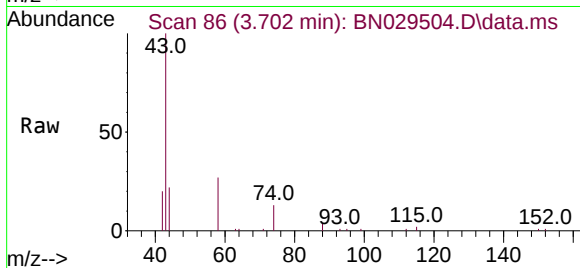

#4
 2-Fluorophenol
 Concen: 0.379 ng
 RT: 5.464 min Scan# 330
 Delta R.T. -0.000 min
 Lab File: BN029504.D
 Acq: 05 Feb 2024 12:45


Tgt Ion: 112 Resp: 4899
 Ion Ratio Lower Upper
 112 100
 64 58.5 47.2 70.8
 63 32.6 25.8 38.6

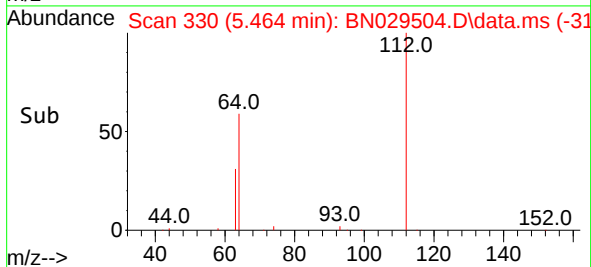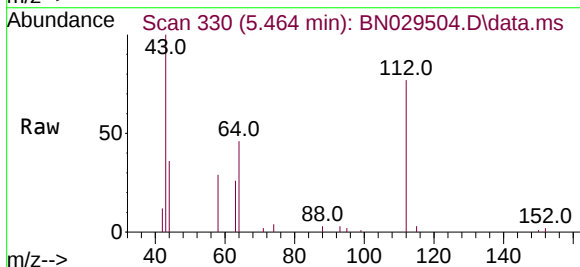





#5
Phenol-d6
Concen: 0.385 ng
RT: 7.060 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Instrument :
BNA_N
ClientSampleId :
PB158799BS



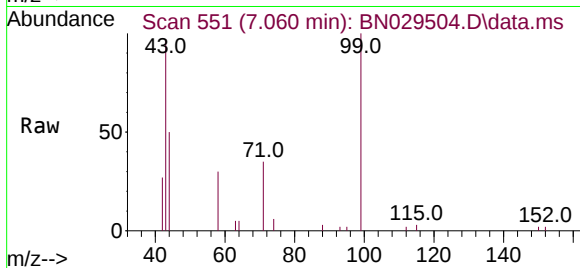


Tgt Ion:	99	Resp:	5747
Ion	Ratio	Lower	Upper
99	100		
42	20.4	16.9	25.3
71	35.7	30.0	45.0

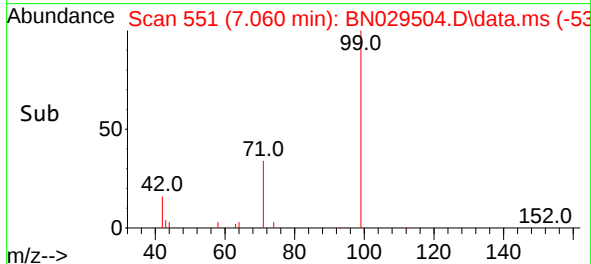

#6
bis(2-Chloroethyl)ether
Concen: 0.335 ng
RT: 7.327 min Scan# 588
Delta R.T. -0.007 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion:	93	Resp:	4771
Ion	Ratio	Lower	Upper
93	100		
63	76.6	63.1	94.7
95	33.7	27.1	40.7

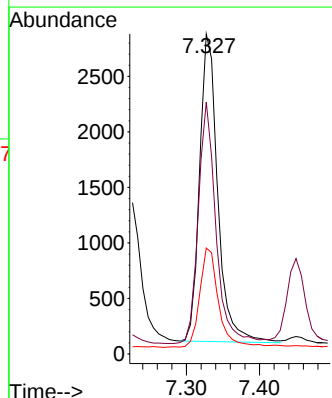
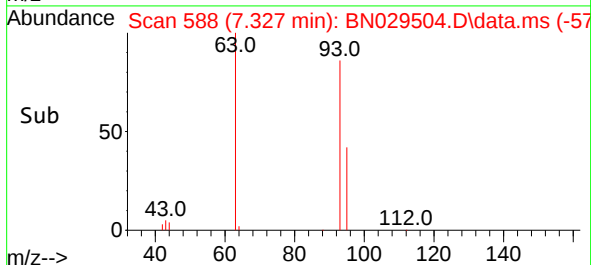
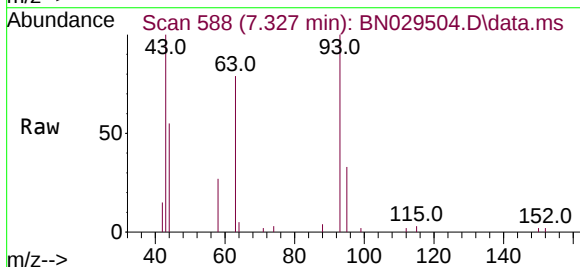




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.690 min Scan# 94
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45




Instrument :
BNA_N
ClientSampleId :
PB158799BS

Tgt Ion:136	Resp:	14412
Ion Ratio	Lower	Upper
136	100	
137	11.3	9.7 14.5
54	7.7	6.6 10.0
68	6.4	5.7 8.5

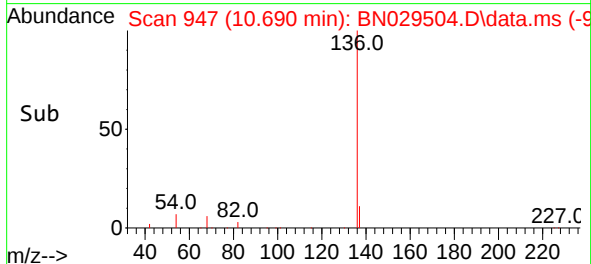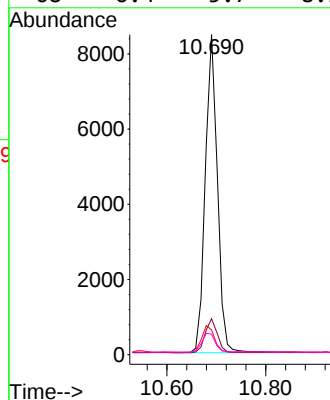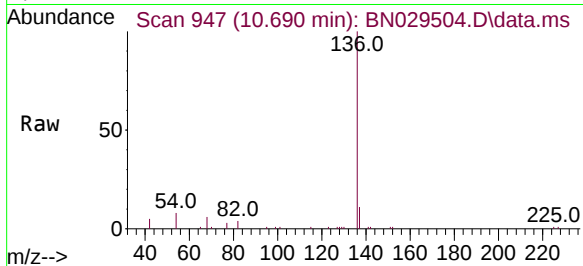

#8
Nitrobenzene-d5
Concen: 0.337 ng
RT: 9.057 min Scan# 794
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion: 82	Resp:	4045
Ion Ratio	Lower	Upper
82	100	
128	38.5	31.6 47.4
54	46.7	38.2 57.4


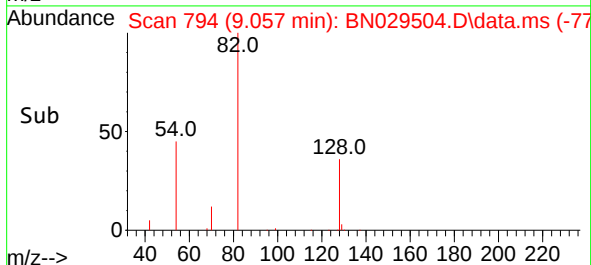
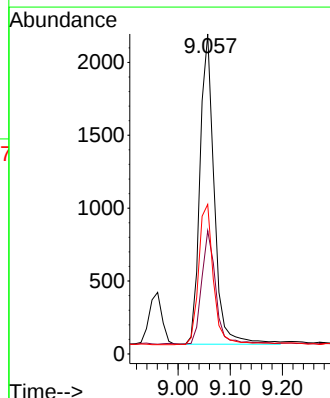
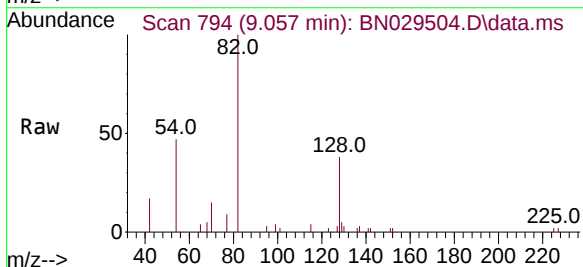




#9
Naphthalene
Concen: 0.307 ng
RT: 10.744 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45




Instrument :
BNA_N
ClientSampleId :
PB158799BS

Tgt Ion:	128	Resp:	12603
Ion Ratio	Lower	Upper	
128	100		
129	11.7	9.5	14.3
127	13.3	10.8	16.2

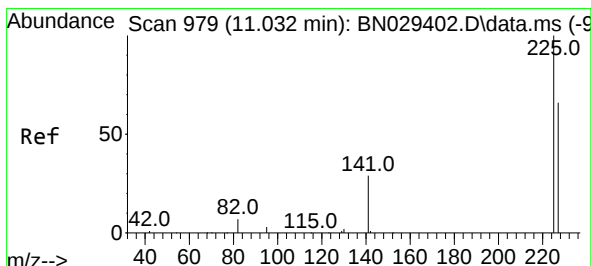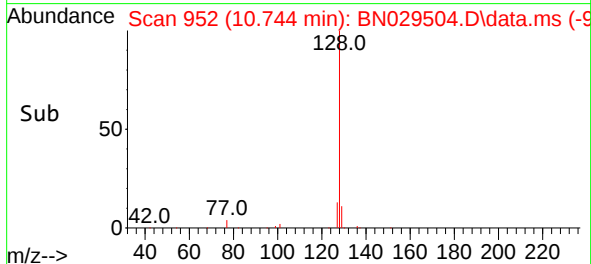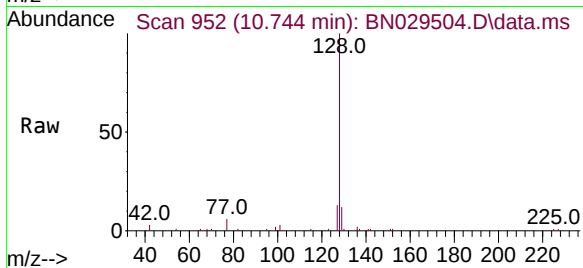

#10
Hexachlorobutadiene
Concen: 0.290 ng
RT: 11.021 min Scan# 978
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion:	225	Resp:	2261
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	64.4	51.1	76.7


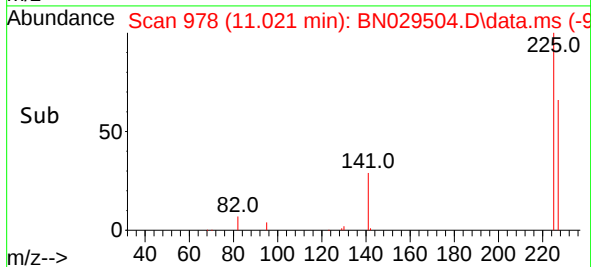

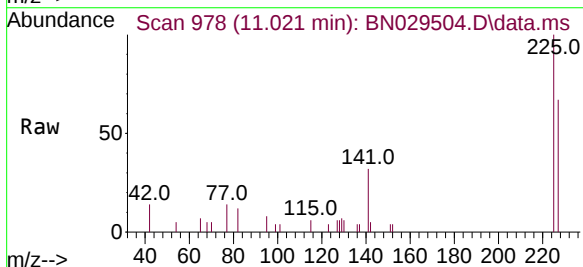




#11
2-Methylnaphthalene-d10
Concen: 0.418 ng
RT: 12.280 min Scan# 11
Delta R.T. -0.008 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45




Instrument :
BNA_N
ClientSampleId :
PB158799BS


Tgt Ion:152 Resp: 8208
Ion Ratio Lower Upper
152 100
151 15.4 17.1 25.7#

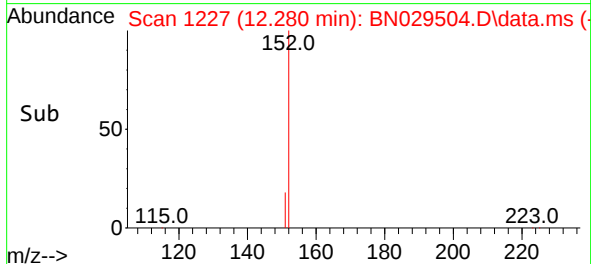

#12
2-Methylnaphthalene
Concen: 0.301 ng
RT: 12.355 min Scan# 1247
Delta R.T. -0.004 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion:142 Resp: 7259
Ion Ratio Lower Upper
142 100
141 88.1 71.9 107.9
115 42.7 33.9 50.9

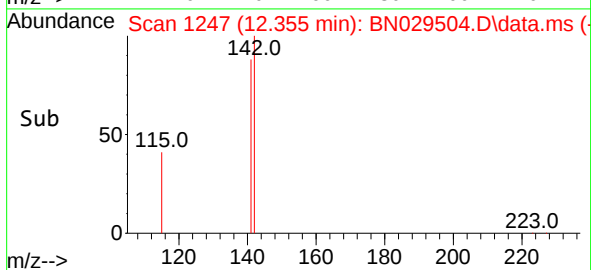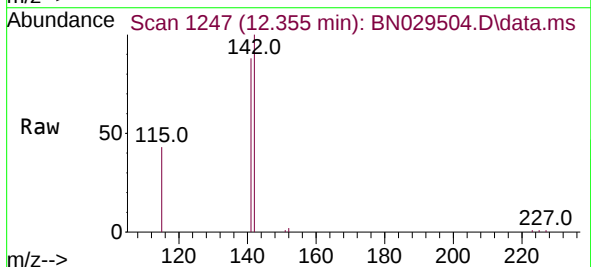



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.532 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN029504.D

Acq: 05 Feb 2024 12:45

Instrument :

BNA_N

ClientSampleId :

PB158799BS





Tgt Ion:164 Resp: 6125

Ion Ratio Lower Upper

164 100

162 105.1 82.6 123.8

160 51.9 41.5 62.3

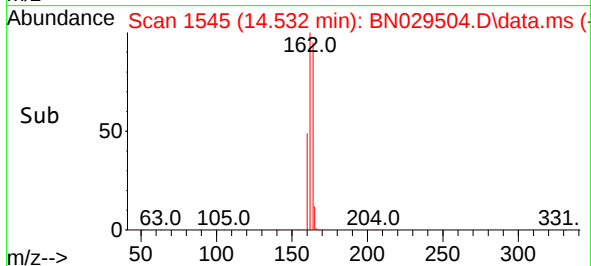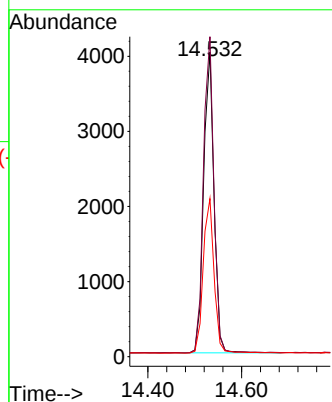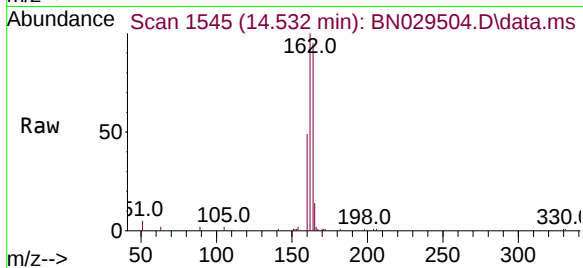

#14

2,4,6-Tribromophenol

Concen: 0.310 ng

RT: 16.026 min Scan# 1678

Delta R.T. -0.000 min

Lab File: BN029504.D

Acq: 05 Feb 2024 12:45




Tgt Ion:330 Resp: 610

Ion Ratio Lower Upper

330 100

332 95.2 76.0 114.0

141 61.5 43.4 65.2

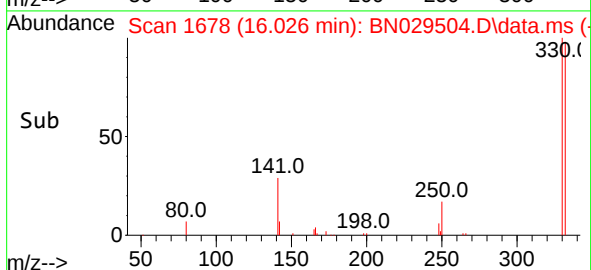
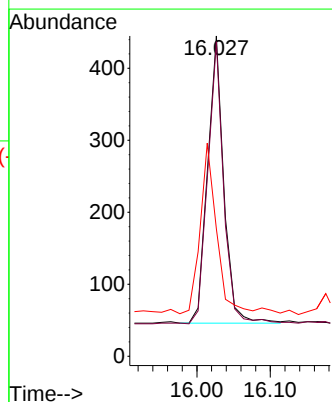
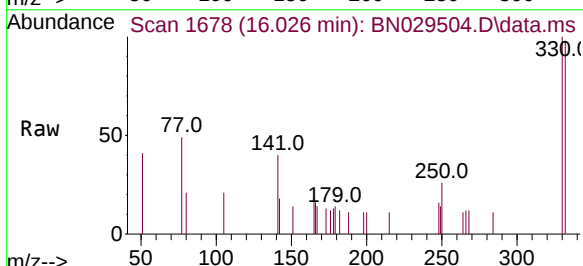




#15
2-Fluorobiphenyl
Concen: 0.347 ng
RT: 13.164 min Scan# 1418
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45




Instrument :
BNA_N
ClientSampleId :
PB158799BS


Tgt Ion:172 Resp: 9121
Ion Ratio Lower Upper
172 100
171 33.6 28.0 42.0
170 22.9 18.7 28.1

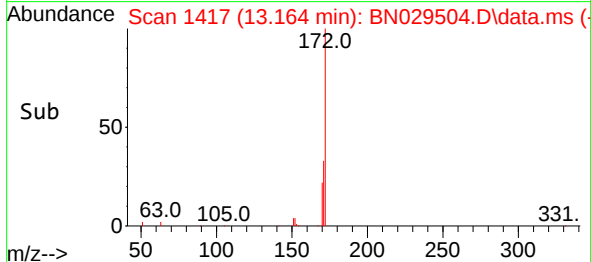

#16
Acenaphthylene
Concen: 0.323 ng
RT: 14.254 min Scan# 1519
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion:152 Resp: 9400
Ion Ratio Lower Upper
152 100
151 19.3 15.9 23.9
153 13.3 10.5 15.7


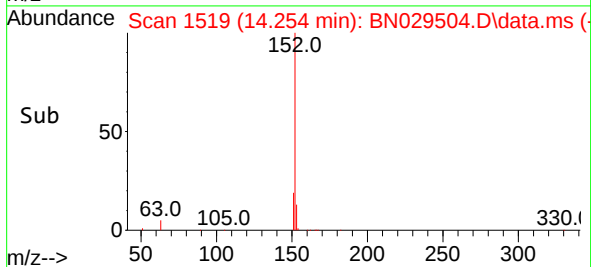

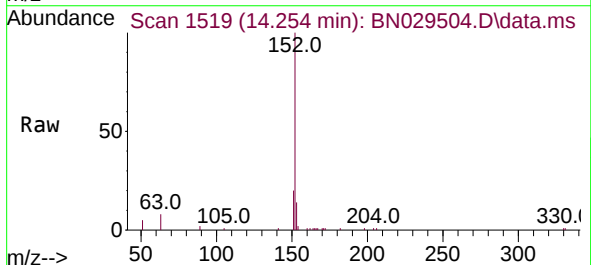


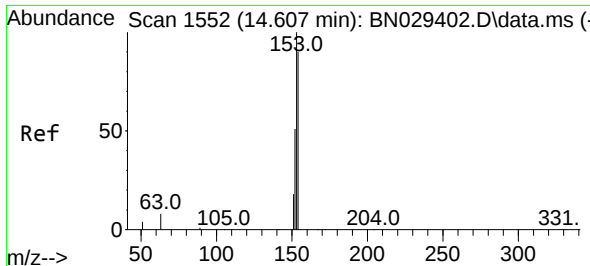

#17
Acenaphthene
Concen: 0.306 ng
RT: 14.596 min Scan# 1551
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45




Instrument :
BNA_N
ClientSampleId :
PB158799BS


Tgt Ion:154 Resp: 5980
Ion Ratio Lower Upper
154 100
153 114.1 93.6 140.4
152 60.7 48.6 73.0

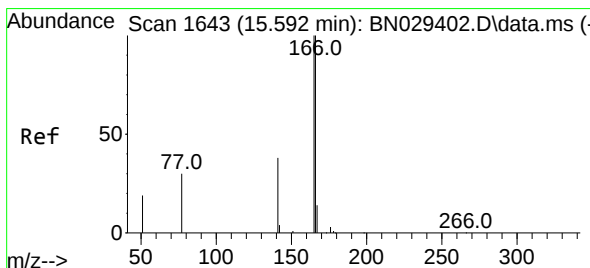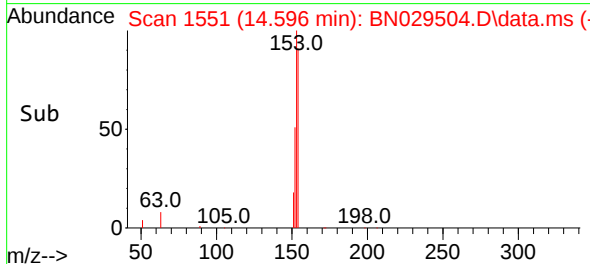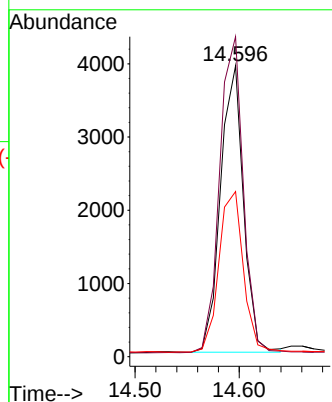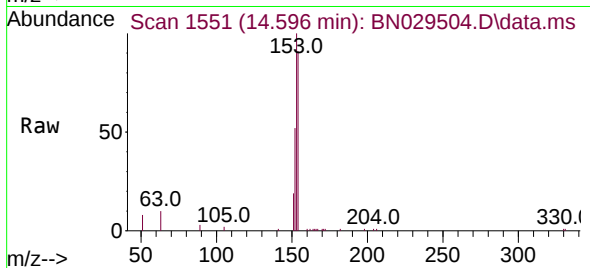

#18
Fluorene
Concen: 0.291 ng
RT: 15.580 min Scan# 1642
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion:166 Resp: 7138
Ion Ratio Lower Upper
166 100
165 100.0 79.9 119.9
167 13.7 11.3 16.9

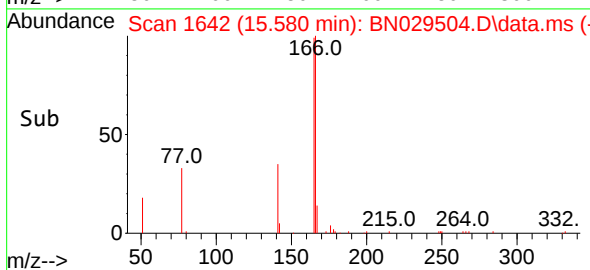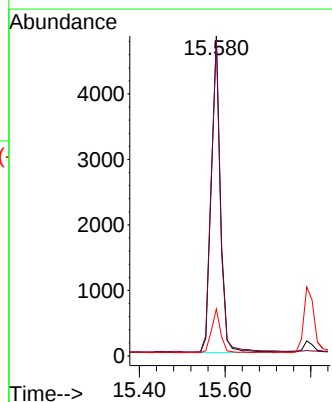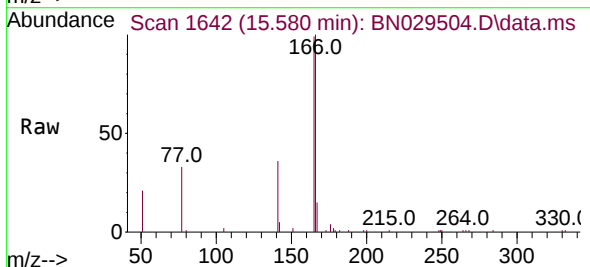

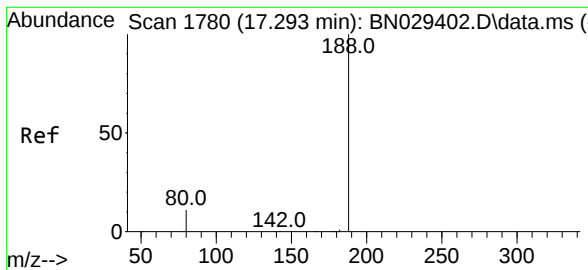

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.280 min Scan# 1779

Delta R.T. -0.000 min

Lab File: BN029504.D

Acq: 05 Feb 2024 12:45

Instrument :

BNA_N

ClientSampleId :

PB158799BS





Tgt Ion:188 Resp: 10628

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 13.3 10.0 15.0

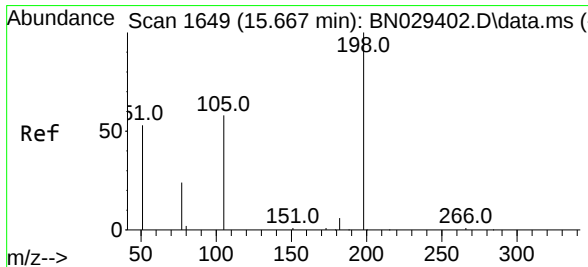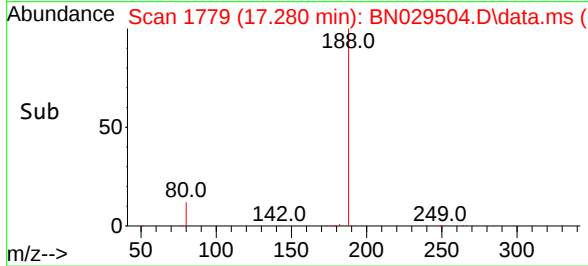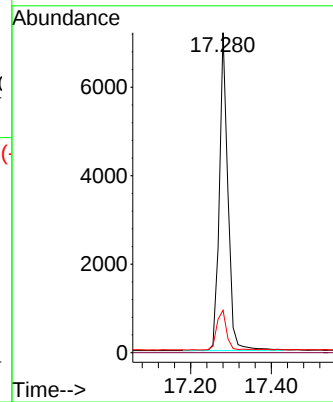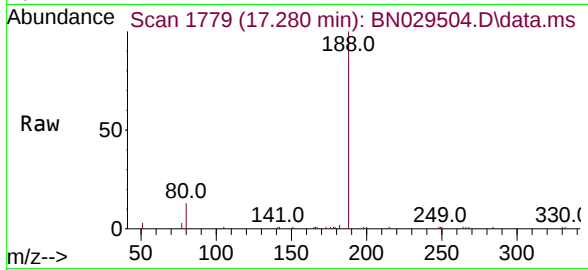

#20

4,6-Dinitro-2-methylphenol

Concen: 0.293 ng

RT: 15.667 min Scan# 1649

Delta R.T. -0.000 min

Lab File: BN029504.D

Acq: 05 Feb 2024 12:45




Tgt Ion:198 Resp: 457

Ion Ratio Lower Upper

198 100

51 83.4 111.0 166.6#

105 61.6 67.0 100.6#


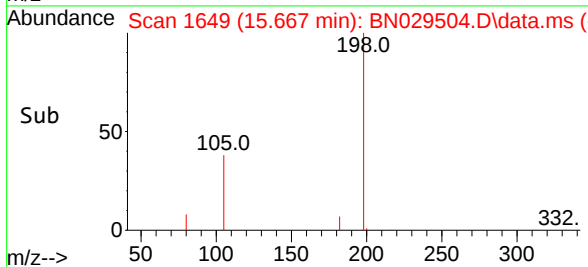
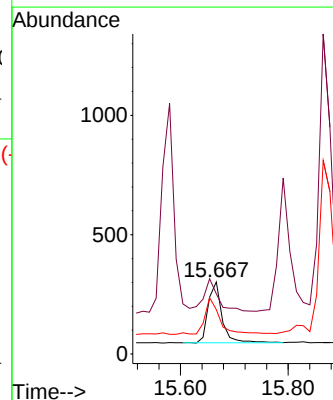
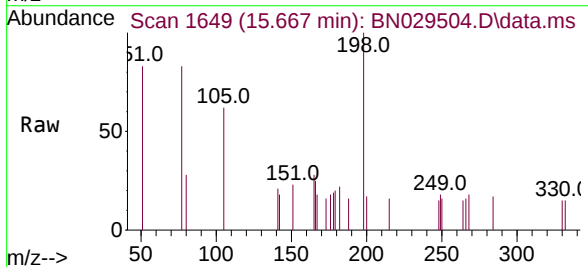




#21
4-Bromophenyl-phenylether
Concen: 0.314 ng
RT: 16.486 min Scan# 1715
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45




Instrument :
BNA_N
ClientSampleId :
PB158799BS


Tgt Ion:248 Resp: 1989
Ion Ratio Lower Upper
248 100
250 104.6 75.0 112.4
141 44.7 77.0 115.6#

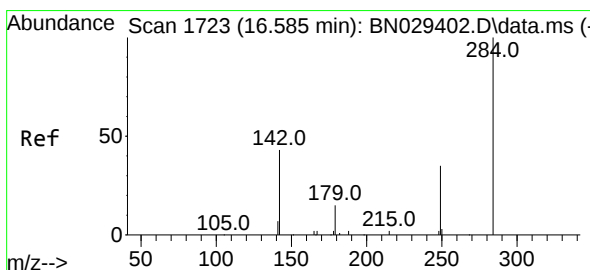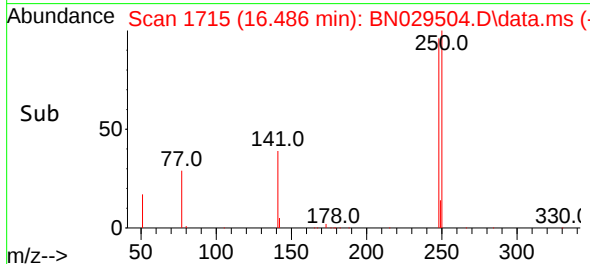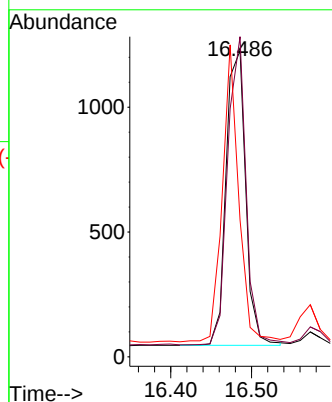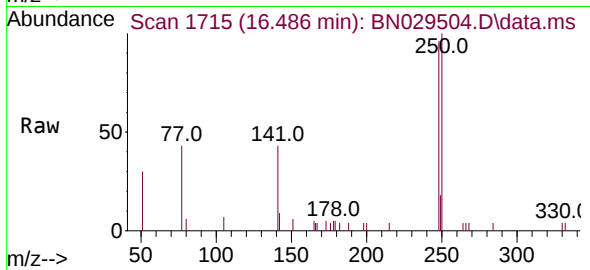

#22
Hexachlorobenzene
Concen: 0.301 ng
RT: 16.573 min Scan# 1722
Delta R.T. -0.013 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion:284 Resp: 2337
Ion Ratio Lower Upper
284 100
142 49.4 39.4 59.2
249 34.3 26.9 40.3


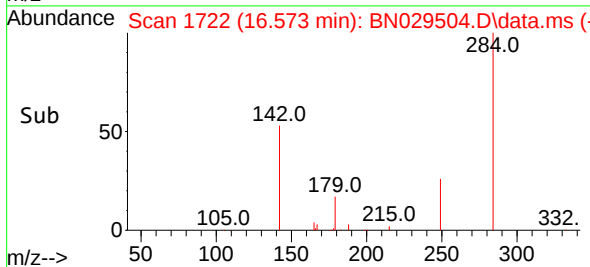
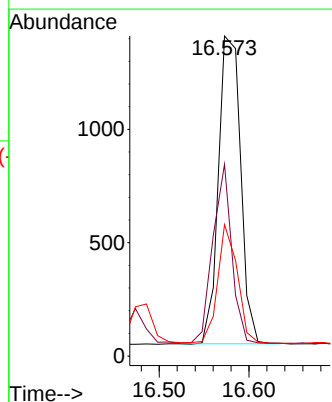
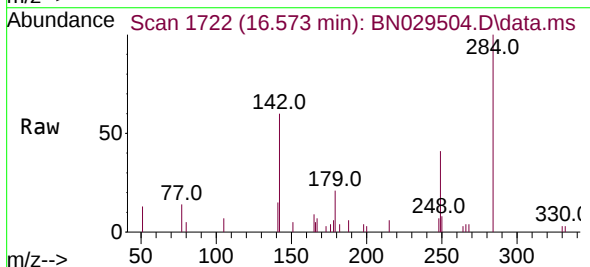


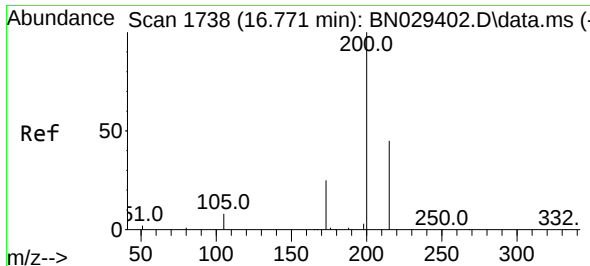

#23
Atrazine
Concen: 0.293 ng
RT: 16.759 min Scan# 1737
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45




Instrument :
BNA_N
ClientSampleId :
PB158799BS


Tgt Ion:200 Resp: 1318
Ion Ratio Lower Upper
200 100
173 28.0 23.4 35.0
215 47.7 38.4 57.6

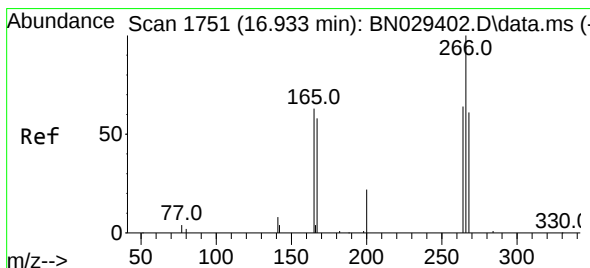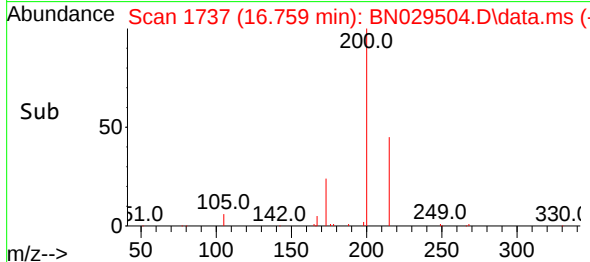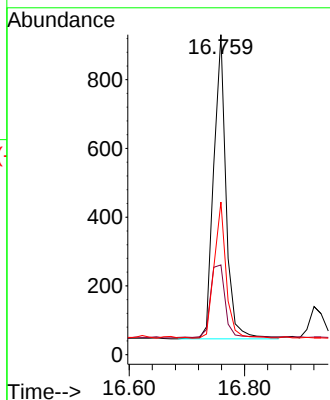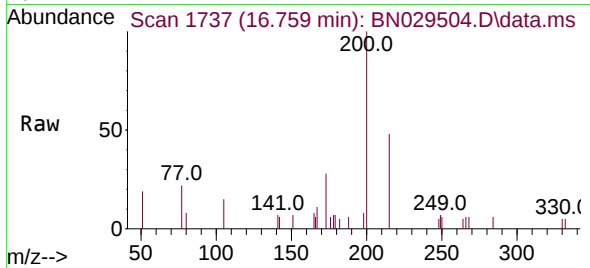

#24
Pentachlorophenol
Concen: 0.315 ng
RT: 16.933 min Scan# 1751
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion:266 Resp: 775
Ion Ratio Lower Upper
266 100
264 61.2 50.8 76.2
268 64.8 51.5 77.3


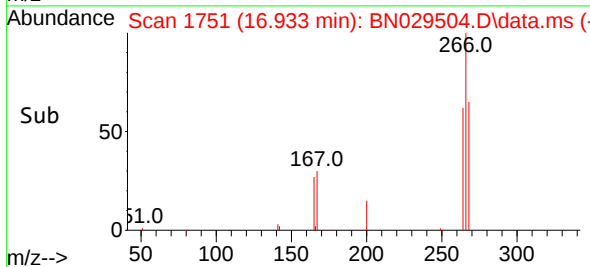
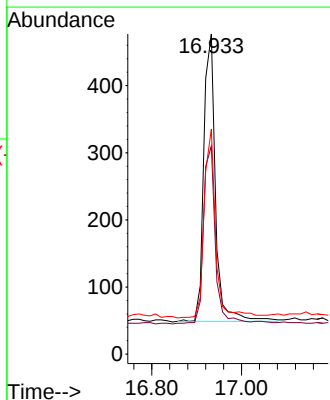
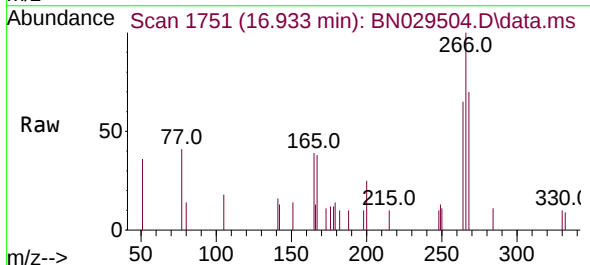


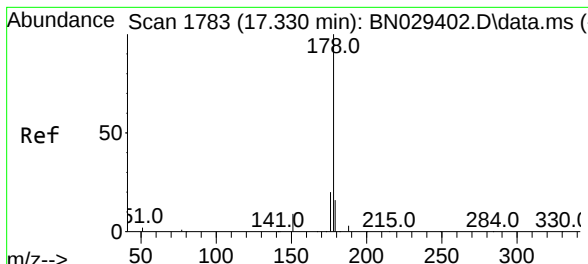

#25
 Phenanthrene
 Concen: 0.313 ng
 RT: 17.317 min Scan# 1790
 Delta R.T. -0.013 min
 Lab File: BN029504.D
 Acq: 05 Feb 2024 12:45




Instrument :
 BNA_N
 ClientSampleId :
 PB158799BS

Tgt Ion:	178	Resp:	9848
Ion	Ratio	Lower	Upper
178	100		
176	19.1	15.8	23.6
179	16.6	12.6	19.0

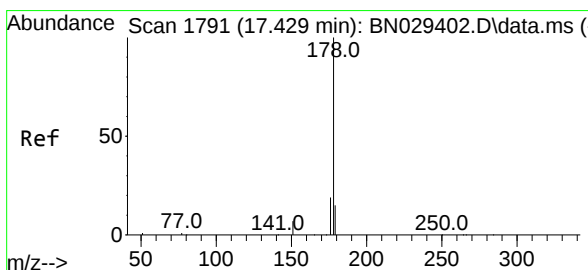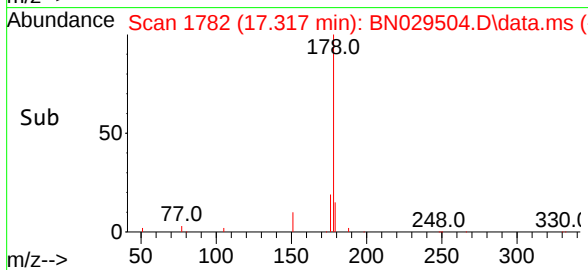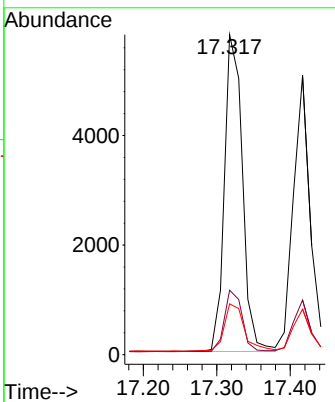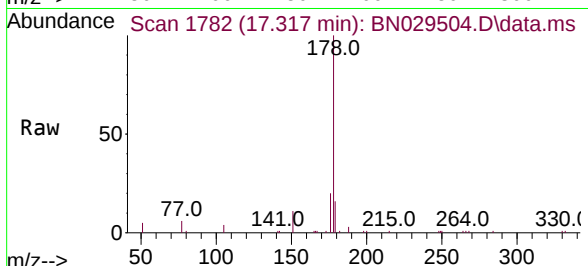

#26
 Anthracene
 Concen: 0.307 ng
 RT: 17.417 min Scan# 1790
 Delta R.T. -0.000 min
 Lab File: BN029504.D
 Acq: 05 Feb 2024 12:45

Tgt Ion:	178	Resp:	8231
Ion	Ratio	Lower	Upper
178	100		
176	18.6	15.0	22.4
179	15.0	12.3	18.5


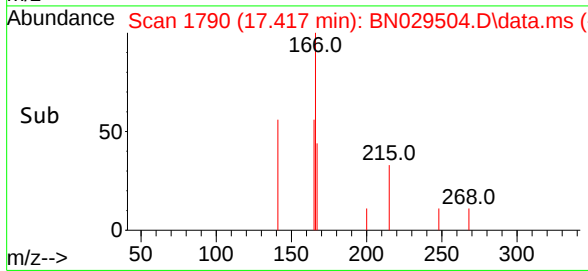
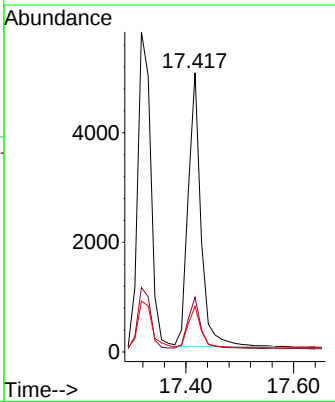
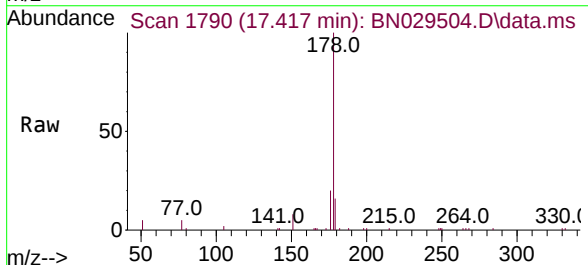




#27
Fluoranthene-d10
Concen: 0.274 ng
RT: 19.317 min Scan# 2052
Delta R.T. -0.005 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45




Instrument :
BNA_N
ClientSampleId :
PB158799BS


Tgt Ion:212 Resp: 7055
Ion Ratio Lower Upper
212 100
106 17.2 13.2 19.8
104 10.1 7.7 11.5

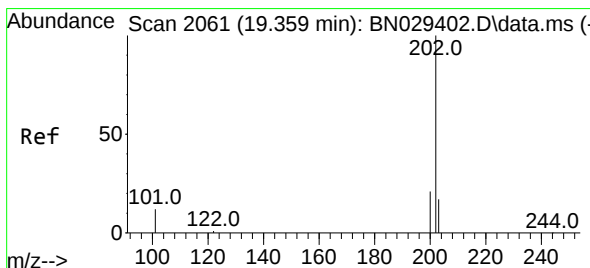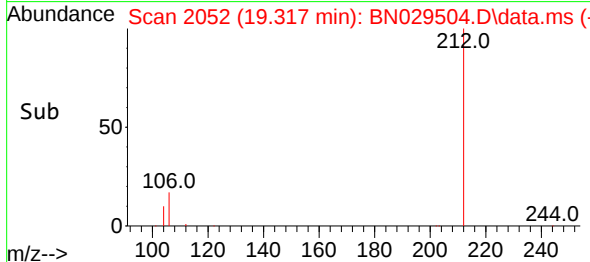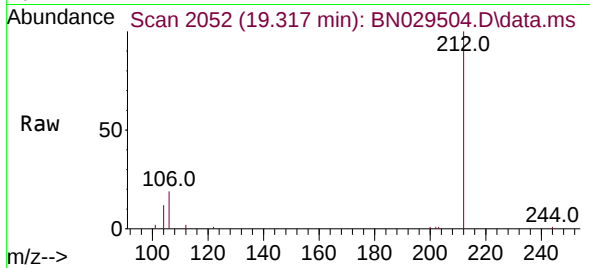

#28
Fluoranthene
Concen: 0.252 ng
RT: 19.350 min Scan# 2059
Delta R.T. -0.005 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion:202 Resp: 8922
Ion Ratio Lower Upper
202 100
101 13.3 10.5 15.7
203 17.0 13.5 20.3


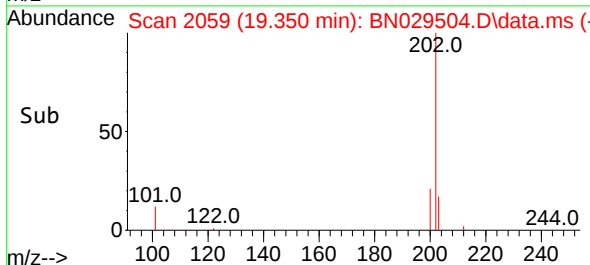
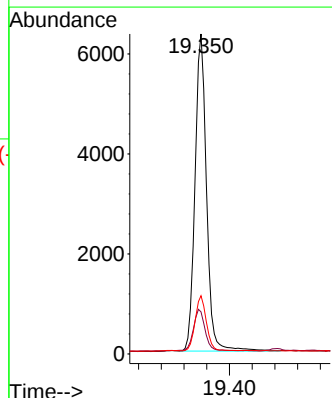
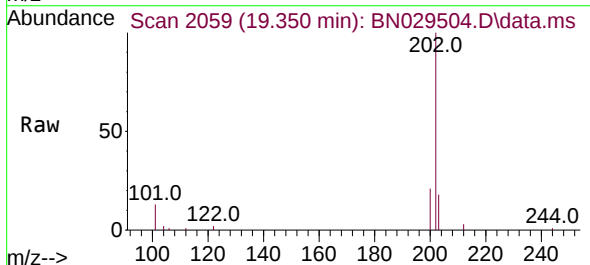




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.483 min Scan# 2469
Delta R.T. -0.009 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45




Instrument :
BNA_N
ClientSampleId :
PB158799BS

Tgt Ion:240 Resp: 5736
Ion Ratio Lower Upper
240 100
120 17.6 16.7 25.1
236 29.0 23.9 35.9

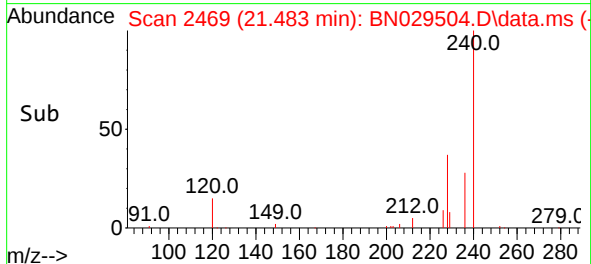

#30
Pyrene
Concen: 0.349 ng
RT: 19.712 min Scan# 2137
Delta R.T. -0.005 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion:202 Resp: 9222
Ion Ratio Lower Upper
202 100
200 20.8 16.6 25.0
203 17.5 14.2 21.4


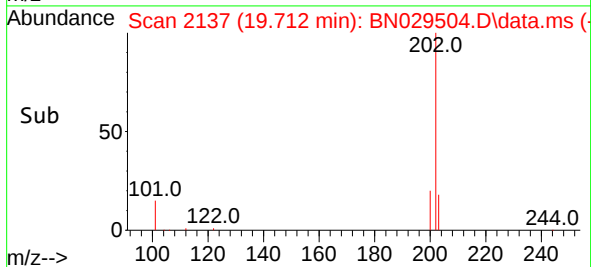

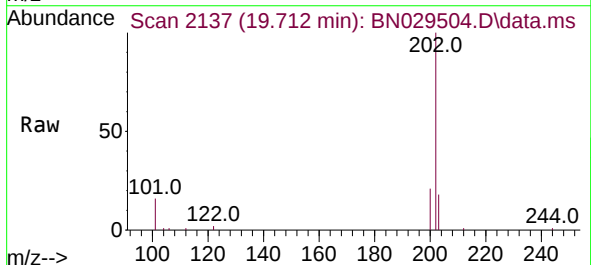




#31
 Terphenyl-d14
 Concen: 0.346 ng
 RT: 19.926 min Scan# 2183
 Delta R.T. -0.005 min
 Lab File: BN029504.D
 Acq: 05 Feb 2024 12:45




Instrument :
 BNA_N
 ClientSampleId :
 PB158799BS

Tgt Ion:244 Resp: 4932
 Ion Ratio Lower Upper
 244 100
 212 10.5 8.2 12.4
 122 20.2 15.6 23.4

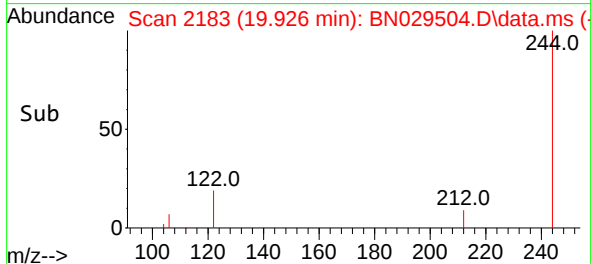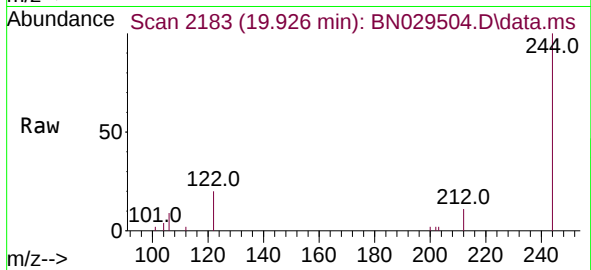

#32
 Benzo(a)anthracene
 Concen: 0.302 ng
 RT: 21.465 min Scan# 2467
 Delta R.T. -0.009 min
 Lab File: BN029504.D
 Acq: 05 Feb 2024 12:45


Tgt Ion:228 Resp: 5911
 Ion Ratio Lower Upper
 228 100
 226 29.0 22.2 33.4
 229 20.4 16.5 24.7

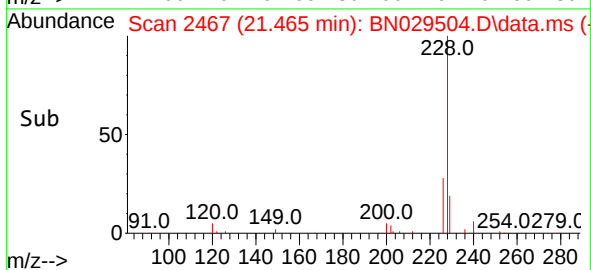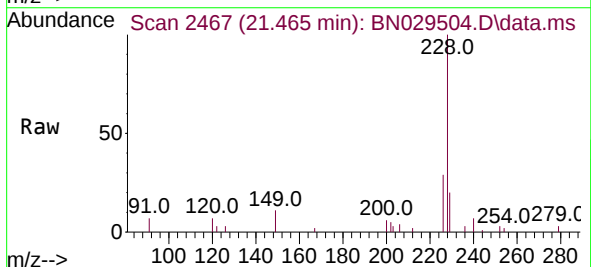






#33
Chrysene
Concen: 0.303 ng
RT: 21.519 min Scan# 2473
Delta R.T. -0.009 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45


Instrument :
BNA_N
ClientSampleId :
PB158799BS

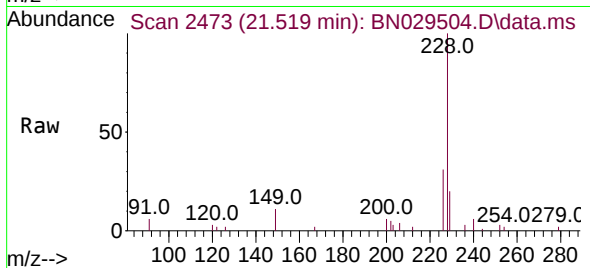



Tgt Ion:228 Resp: 6740
Ion Ratio Lower Upper
228 100
226 31.1 24.9 37.3
229 19.9 15.9 23.9

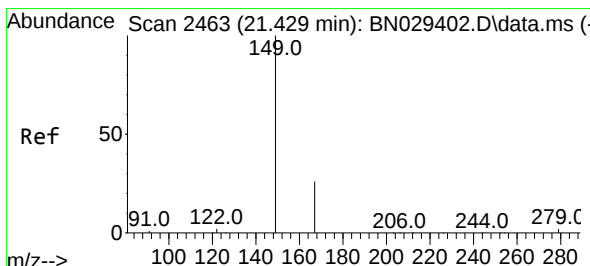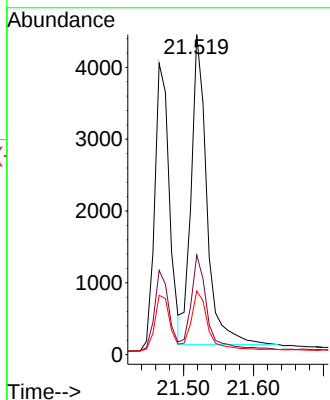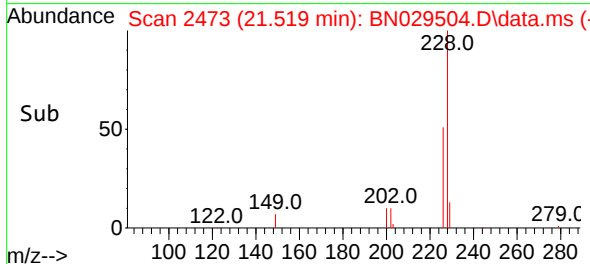

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.286 ng
RT: 21.420 min Scan# 2462
Delta R.T. -0.000 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

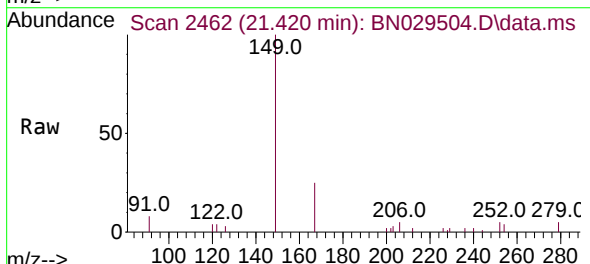

Tgt Ion:149 Resp: 3822
Ion Ratio Lower Upper
149 100
167 23.8 20.1 30.1
279 2.8 2.5 3.7

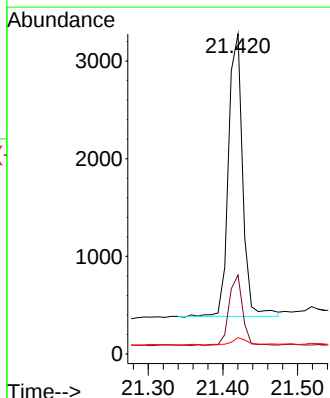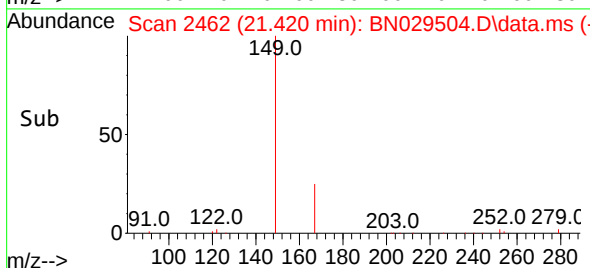



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.864 min Scan# 3078

Delta R.T. -0.006 min

Lab File: BN029504.D

Acq: 05 Feb 2024 12:45

Instrument :

BNA_N

ClientSampleId :

PB158799BS





Tgt Ion:264 Resp: 5376

Ion Ratio Lower Upper

264 100

260 26.6 21.2 31.8

265 53.1 41.5 62.3

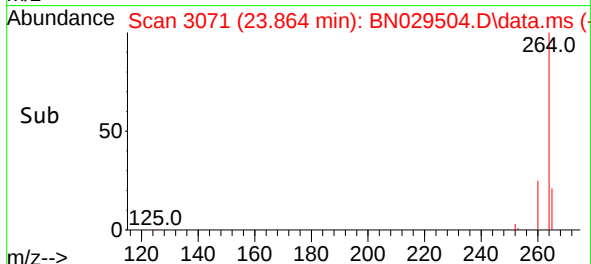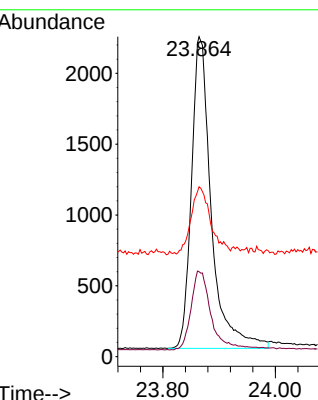

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.319 ng

RT: 26.329 min Scan# 3914

Delta R.T. -0.006 min

Lab File: BN029504.D

Acq: 05 Feb 2024 12:45




Tgt Ion:276 Resp: 6895

Ion Ratio Lower Upper

276 100

138 32.3 20.5 30.7#

277 25.2 17.0 25.4


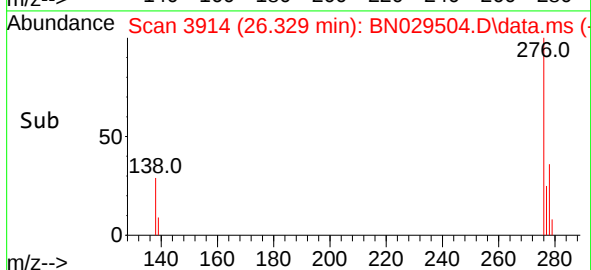
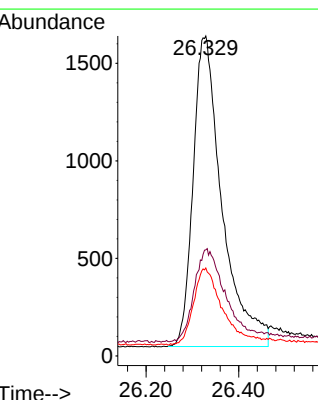
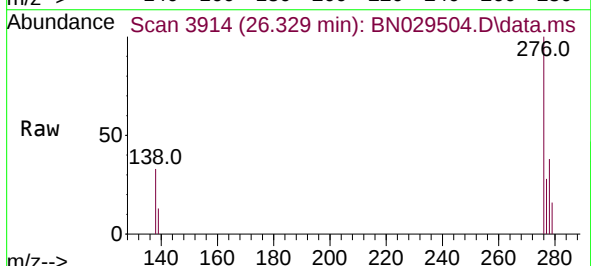




#37
Benzo(b)fluoranthene
Concen: 0.315 ng
RT: 23.142 min Scan# 2824
Delta R.T. -0.006 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45




Instrument :
BNA_N
ClientSampleId :
PB158799BS

Tgt Ion:252 Resp: 6059
Ion Ratio Lower Upper
252 100
253 32.5 21.7 32.5
125 18.2 13.3 19.9

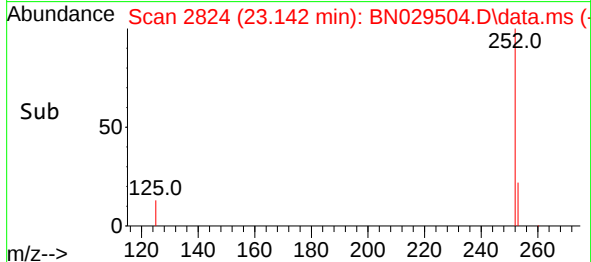

#38
Benzo(k)fluoranthene
Concen: 0.289 ng
RT: 23.192 min Scan# 2841
Delta R.T. -0.006 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Tgt Ion:252 Resp: 5825
Ion Ratio Lower Upper
252 100
253 33.8 21.8 32.8#
125 21.4 13.9 20.9#

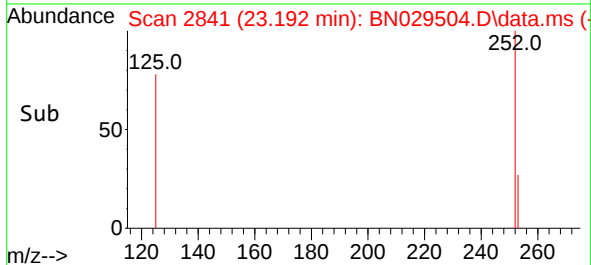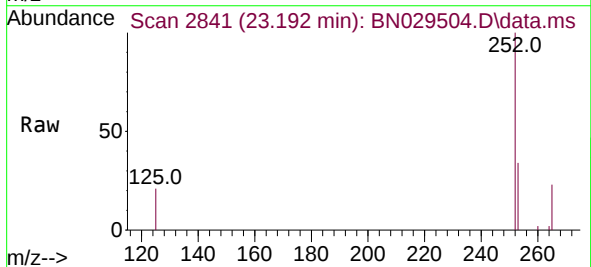



#39

Benzo(a)pyrene

Concen: 0.308 ng

RT: 23.759 min Scan# 3041

Delta R.T. -0.006 min

Lab File: BN029504.D


Acq: 05 Feb 2024 12:45

Instrument :



BNA_N

ClientSampleId :

PB158799BS



Tgt Ion:	252	Resp:	5166
Ion Ratio	Lower	Upper	
252	100		
253	39.0	24.9	37.3#
125	24.0	16.6	25.0



#40

Dibenzo(a,h)anthracene

Concen: 0.317 ng




RT: 26.355 min Scan# 3923

Delta R.T. -0.009 min

Lab File: BN029504.D

Acq: 05 Feb 2024 12:45


Tgt Ion:	278	Resp:	5448
Ion Ratio	Lower	Upper	
278	100		
139	27.4	20.4	30.6
279	33.0	25.0	37.6

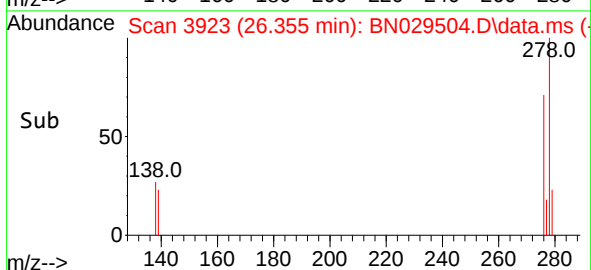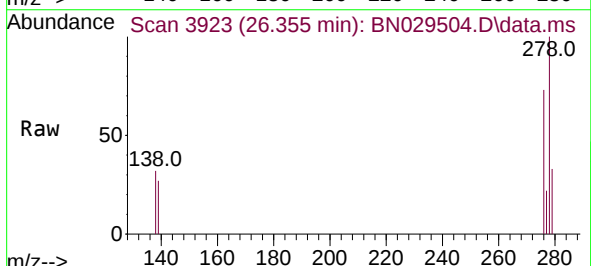



#41
Benzo(g,h,i)perylene
Concen: 0.303 ng
RT: 27.080 min Scan# 41
Delta R.T. -0.003 min
Lab File: BN029504.D
Acq: 05 Feb 2024 12:45

Instrument :
BNA_N
ClientSampleId :
PB158799BS

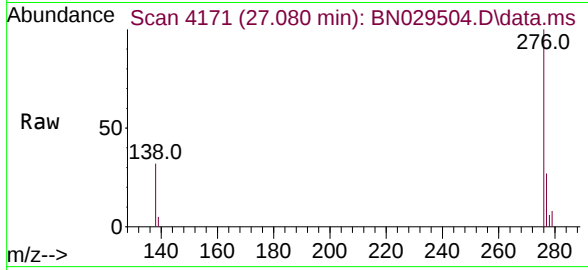

Tgt Ion: 276 Resp: 6352
Ion Ratio Lower Upper
276 100
277 26.8 19.4 29.2
138 32.1 23.5 35.3

