
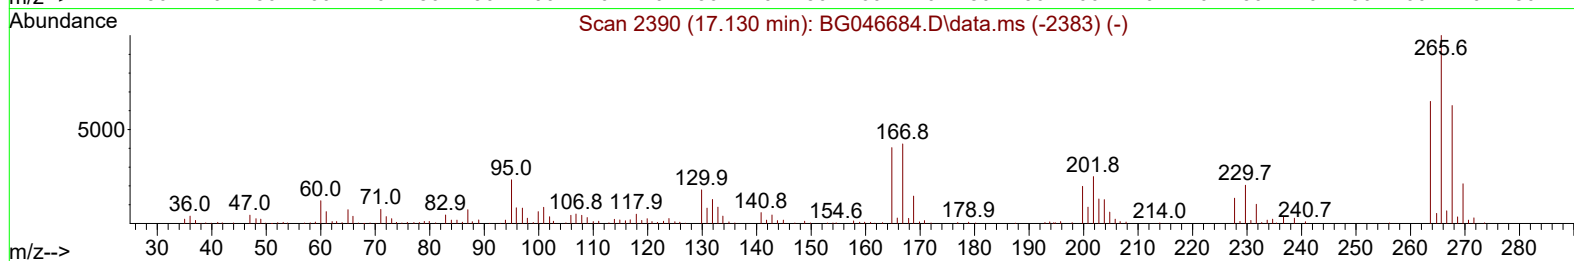
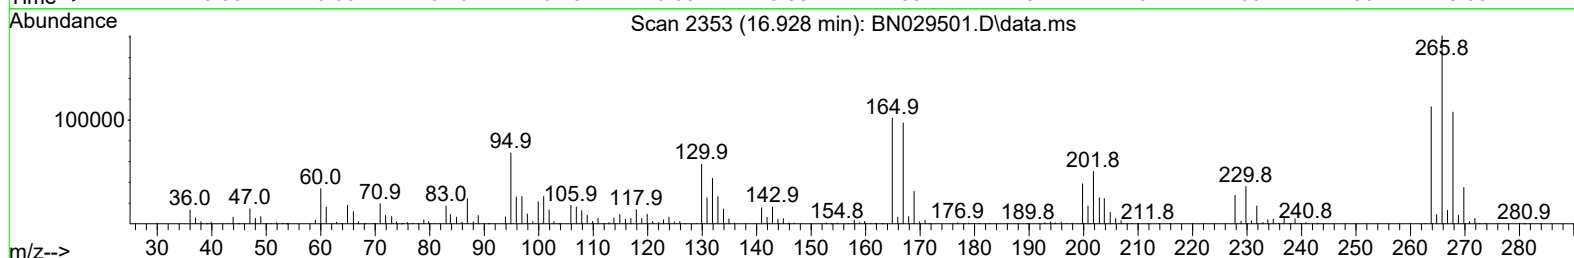


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029501.D
Acq On : 05 Feb 2024 10:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 16:08:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 03:38:30 2024
Response via : Initial Calibration

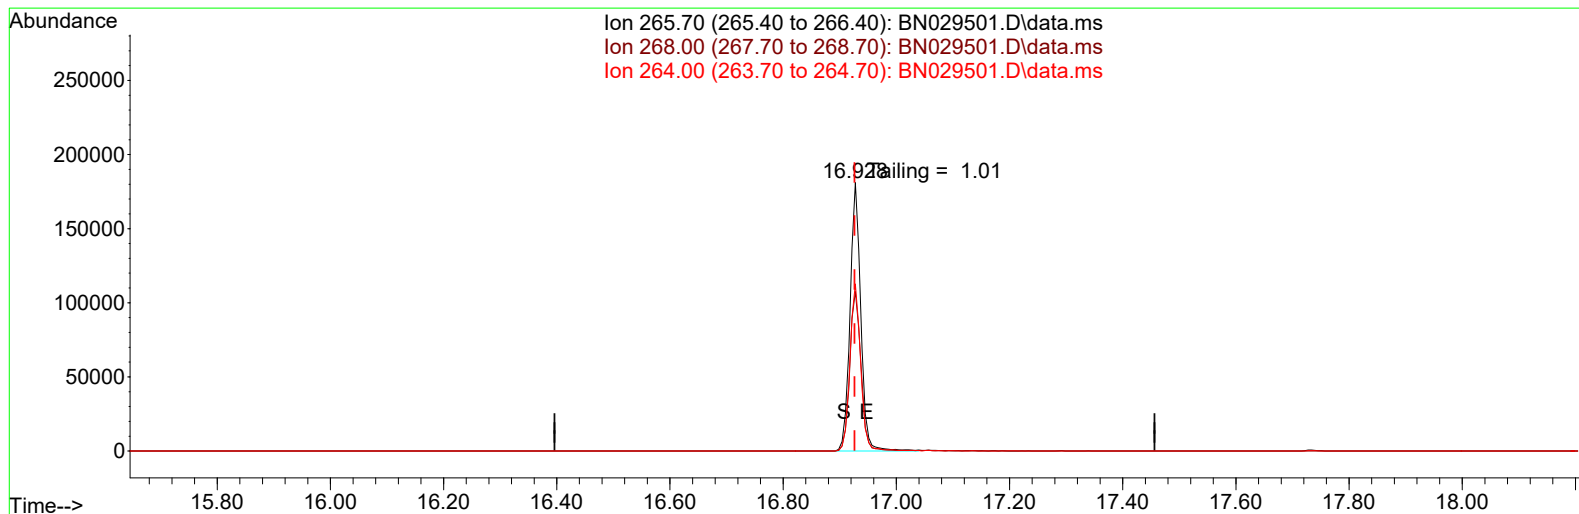

TIC: BN029501.D\data.ms

(70) Pentachlorophenol (C)




16.928min (+ 0.002) 16499.10 ng

response 239151

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.42
264.00	61.60	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029501.D
Acq On : 05 Feb 2024 10:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 16:08:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 03:38:30 2024
Response via : Initial Calibration

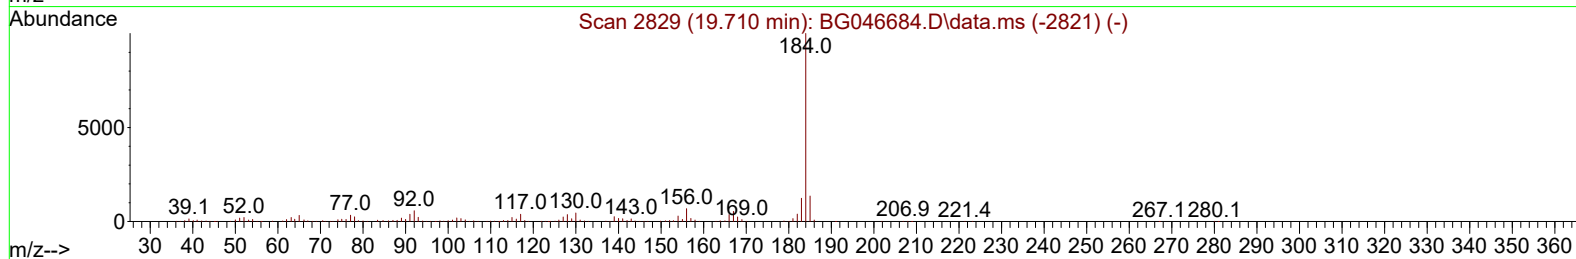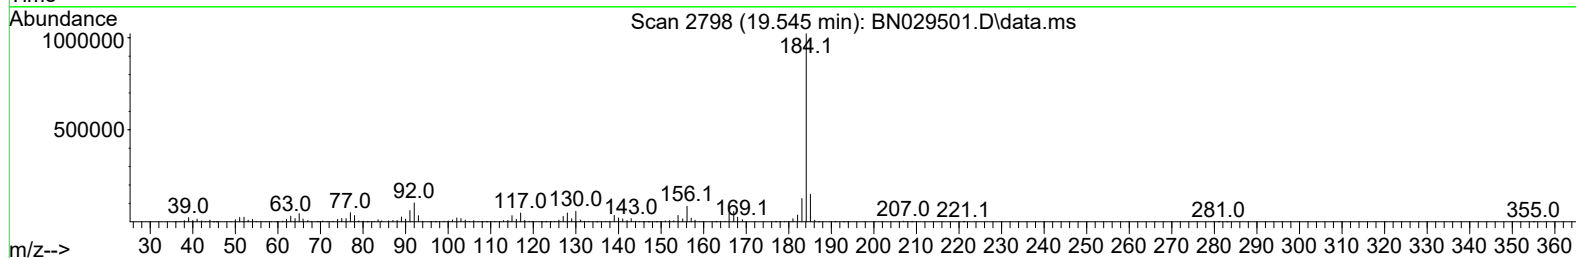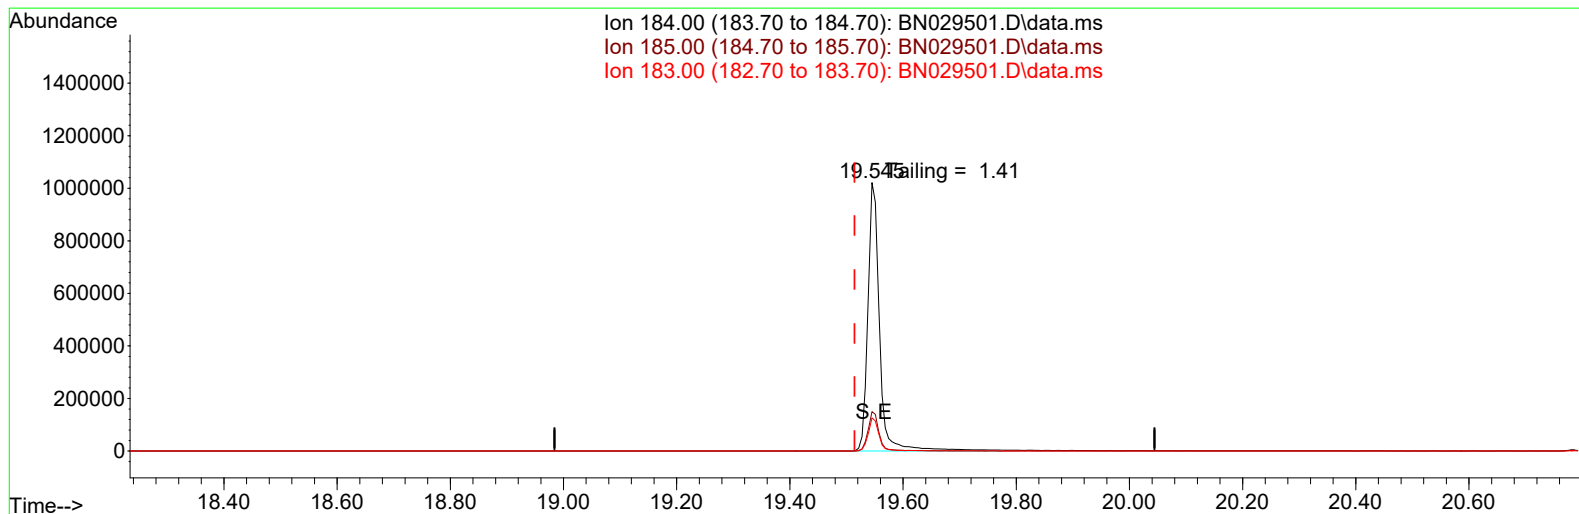

TIC: BN029501.D\data.ms

(77) Benzidine

19.545min (+ 0.031) 0.00 ng

response 1470767

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	12.34
0.00	0.00	0.00