
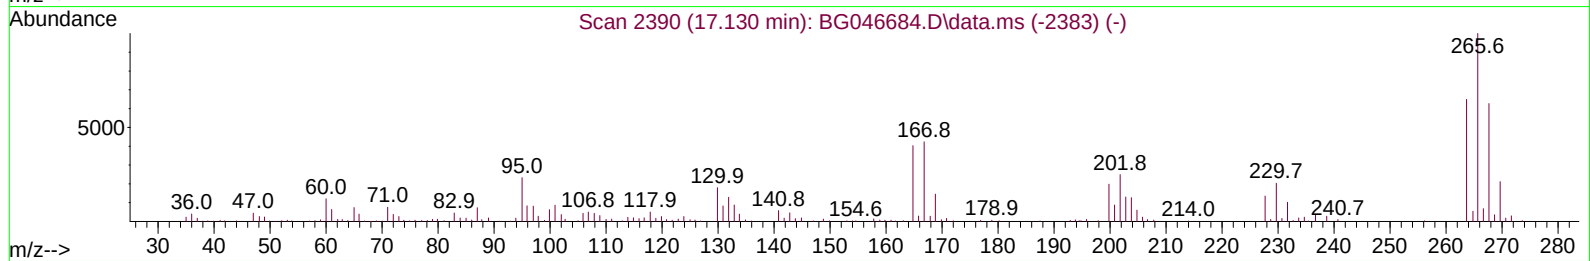
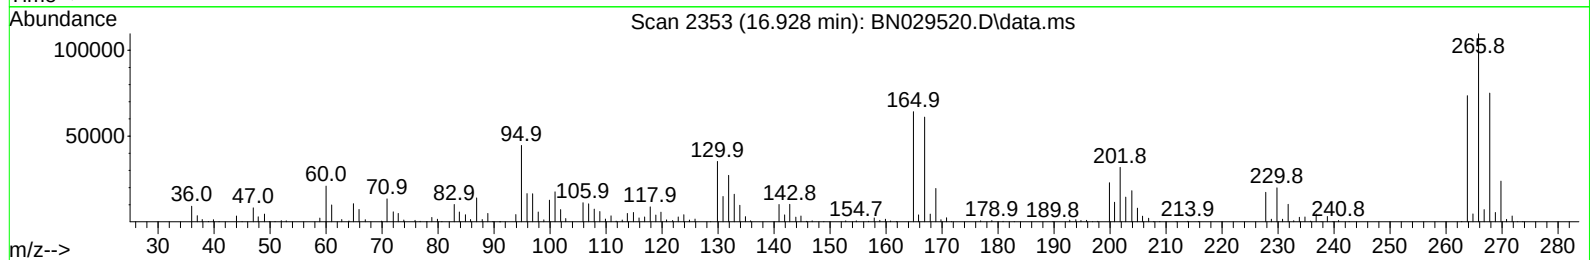


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029520.D
Acq On : 05 Feb 2024 22:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 05:26:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 03:38:30 2024
Response via : Initial Calibration

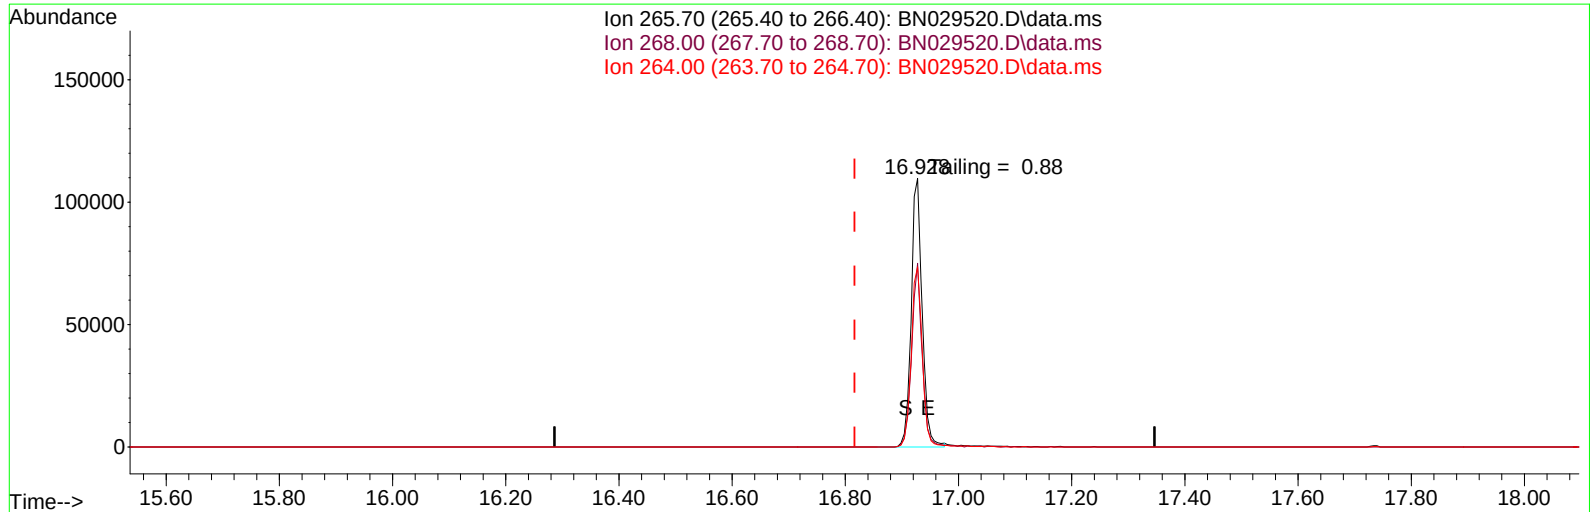

TIC: BN029520.D\data.ms

(70) Pentachlorophenol (C)




16.928min (+ 0.112) 16138.11 ng

response 147798

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.42
264.00	61.60	67.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029520.D
Acq On : 05 Feb 2024 22:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 05:26:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 03:38:30 2024
Response via : Initial Calibration

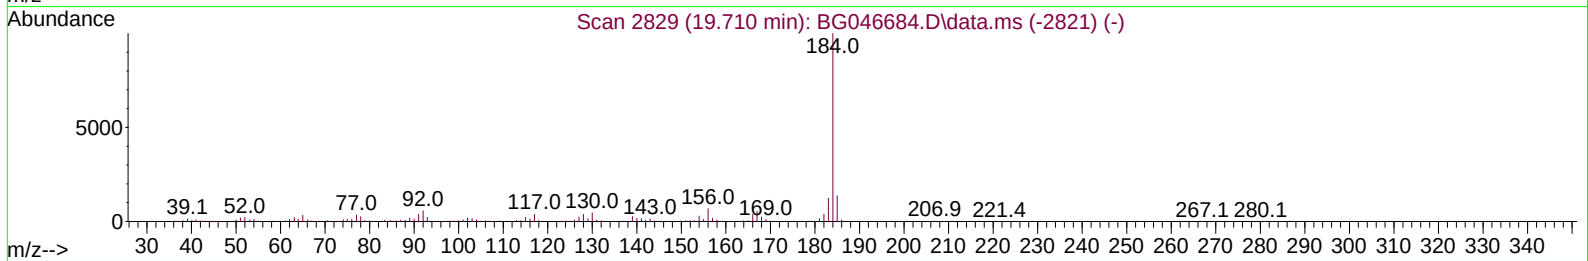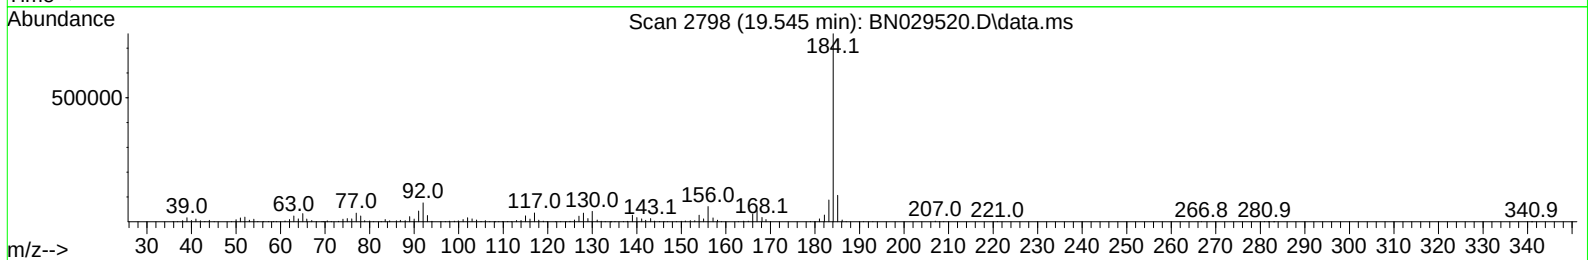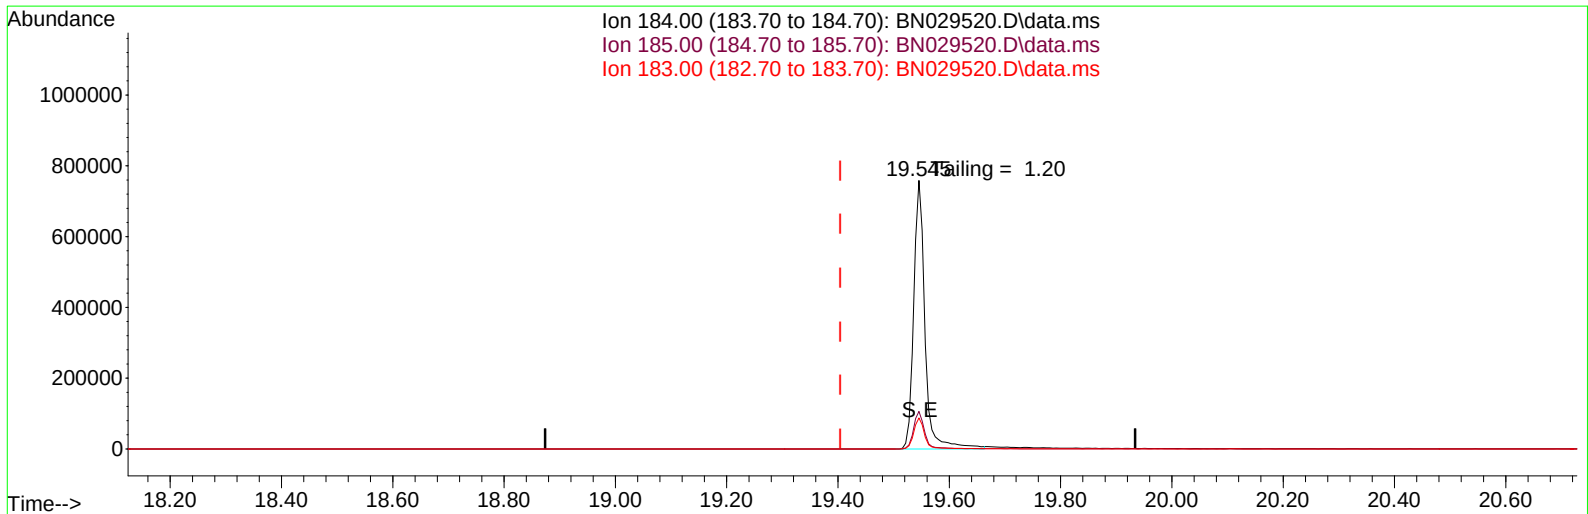

TIC: BN029520.D\data.ms

(77) Benzidine

19.545min (+ 0.141) 0.00 ng

response 1084015

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	11.58
0.00	0.00	0.00