

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
 Data File : BN029513.D
 Acq On : 05 Feb 2024 18:10
 Operator : MA/JU
 Sample : P1343-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-195-GW-585-587

Quant Time: Feb 06 04:21:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 01:51:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.890	152	4120	0.400	ng	0.00
7) Naphthalene-d8	10.690	136	11029	0.400	ng	0.00
13) Acenaphthene-d10	14.532	164	4857	0.400	ng	0.00
19) Phenanthrene-d10	17.280	188	8902	0.400	ng	0.00
29) Chrysene-d12	21.483	240	6031	0.400	ng	0.00
35) Perylene-d12	23.864	264	6120	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.464	112	1822	0.184	ng	0.00
5) Phenol-d6	7.060	99	1106	0.097	ng	0.00
8) Nitrobenzene-d5	9.057	82	3218	0.350	ng	0.00
11) 2-Methylnaphthalene-d10	12.284	152	5641	0.376	ng	0.00
14) 2,4,6-Tribromophenol	16.027	330	532	0.341	ng	0.00
15) 2-Fluorobiphenyl	13.164	172	8906	0.427	ng	0.00
27) Fluoranthene-d10	19.317	212	8629	0.400	ng	0.00
31) Terphenyl-d14	19.926	244	6118	0.409	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.369	88	336	0.058	ng	# 70
34) Bis(2-ethylhexyl)phtha...	21.411	149	583	0.042	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029513.D
Acq On : 05 Feb 2024 18:10
Operator : MA/JU
Sample : P1343-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-585-587


Quant Time: Feb 06 04:21:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 01:51:59 2024
Response via : Initial Calibration

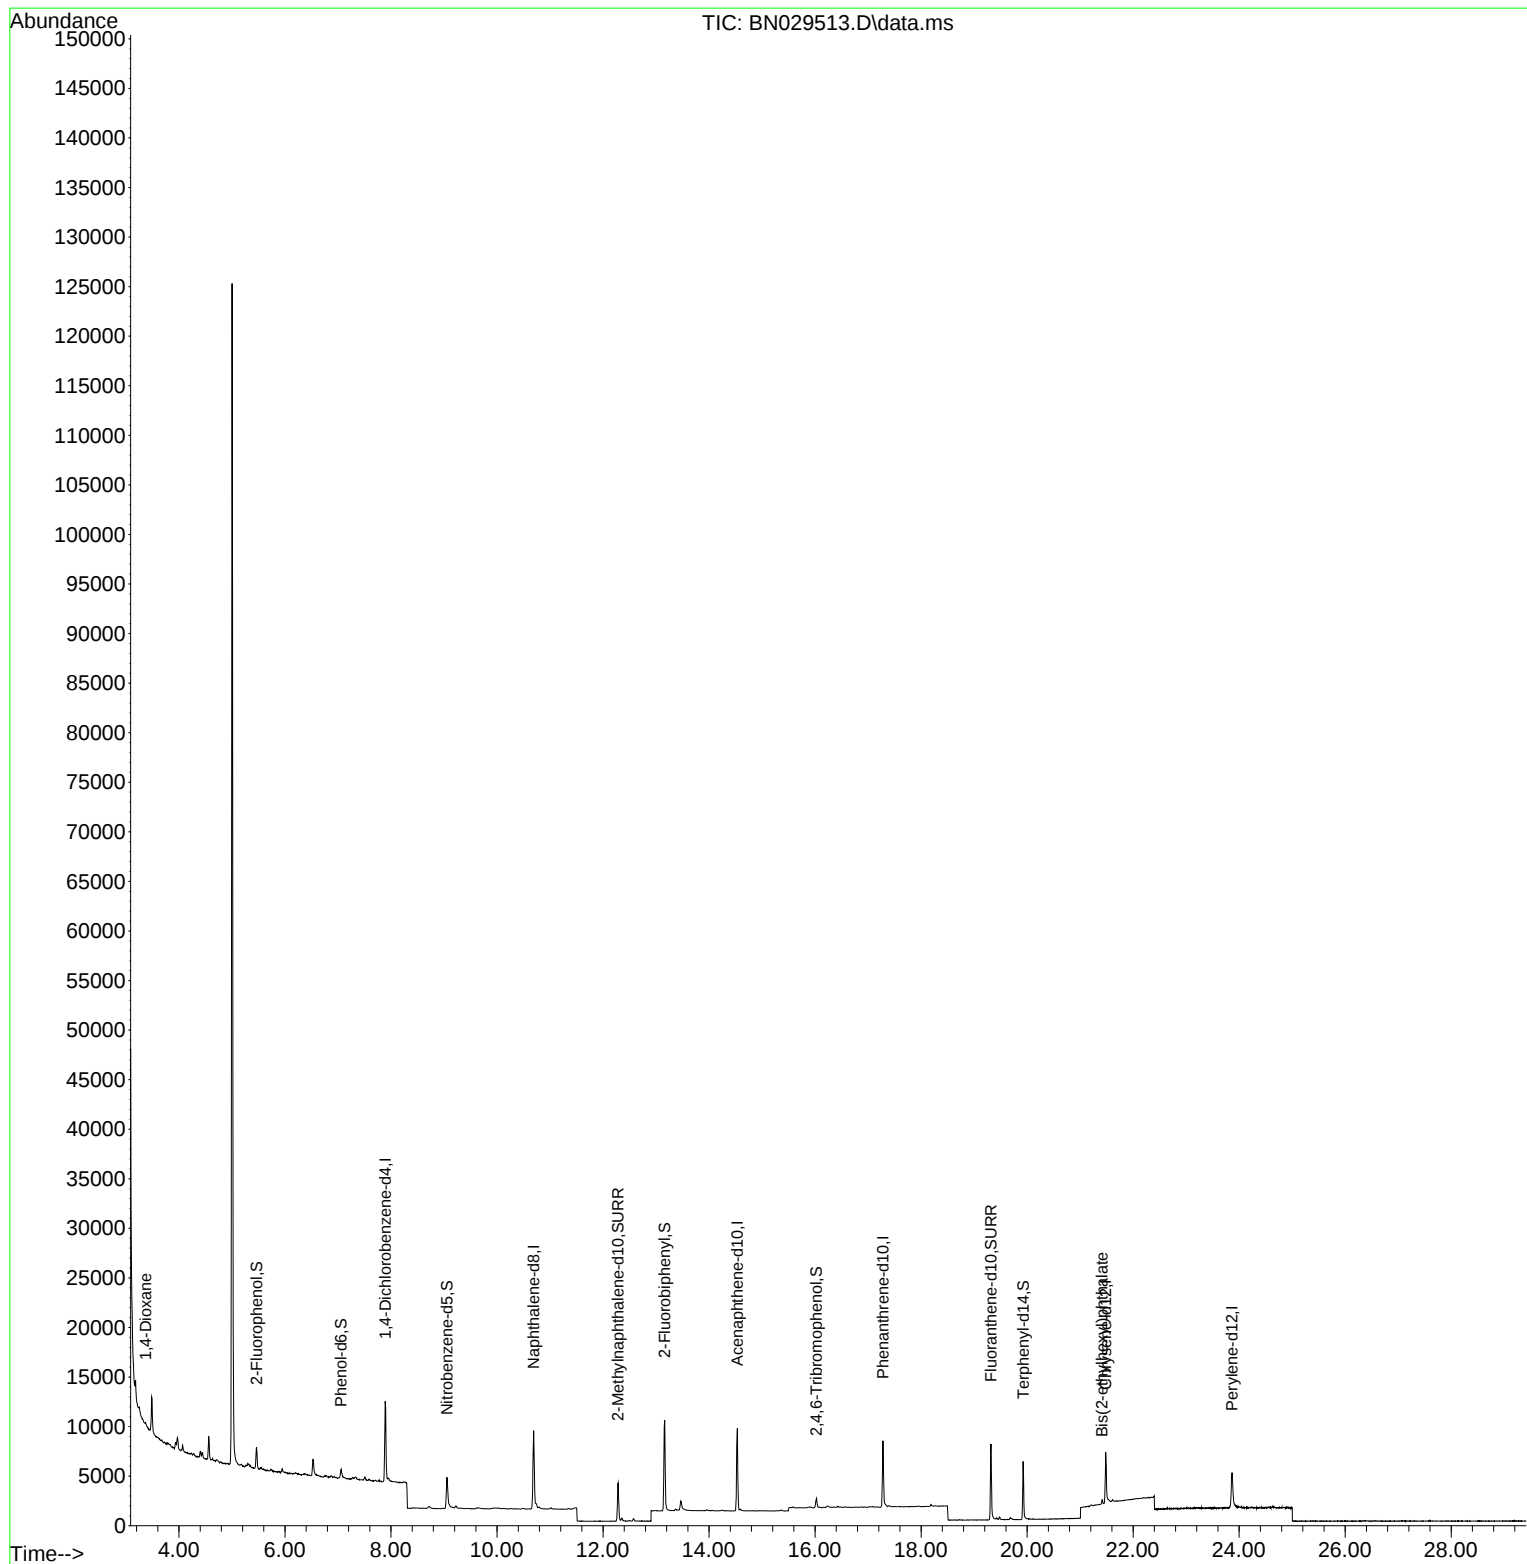






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.890 min Scan# 6
 Delta R.T. -0.008 min
 Lab File: BN029513.D
 Acq: 05 Feb 2024 18:10


Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-195-GW-585-587

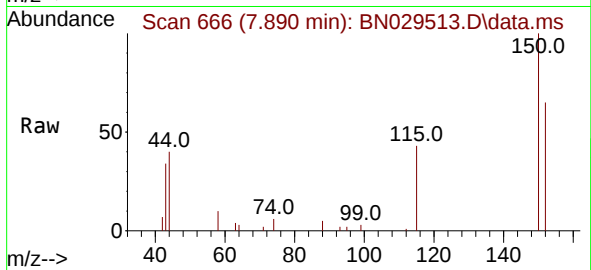



Tgt Ion:152 Resp: 4120
 Ion Ratio Lower Upper
 152 100
 150 154.6 123.0 184.4
 115 66.6 51.4 77.0

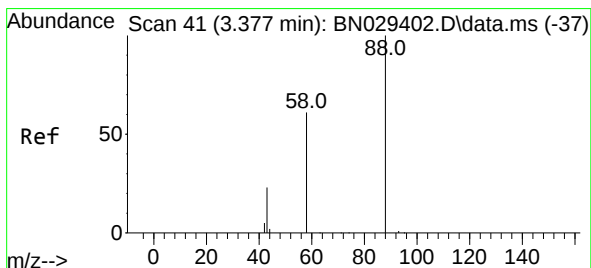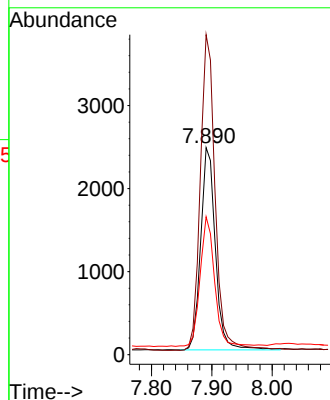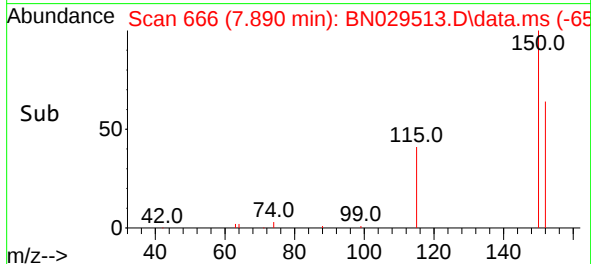


#2
 1,4-Dioxane
 Concen: 0.058 ng
 RT: 3.369 min Scan# 40
 Delta R.T. -0.007 min
 Lab File: BN029513.D
 Acq: 05 Feb 2024 18:10

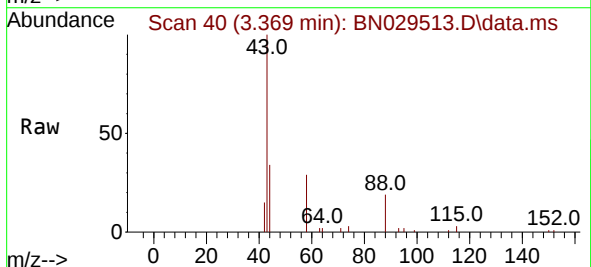

Tgt Ion: 88 Resp: 336
 Ion Ratio Lower Upper
 88 100
 43 0.0 23.3 34.9#
 58 82.7 53.8 80.6#



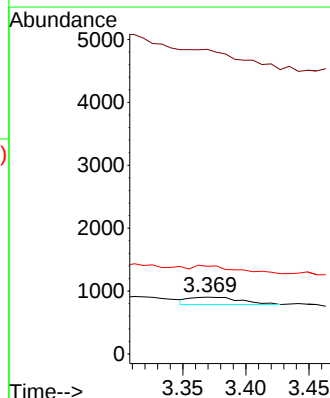
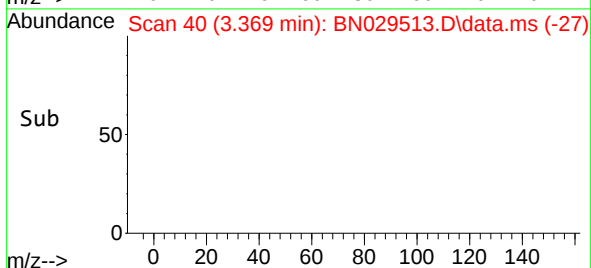




#4
2-Fluorophenol
Concen: 0.184 ng
RT: 5.464 min Scan# 311
Delta R.T. -0.000 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10




Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-585-587


Tgt Ion:112 Resp: 1822
Ion Ratio Lower Upper
112 100
64 54.6 47.2 70.8
63 30.9 25.8 38.6

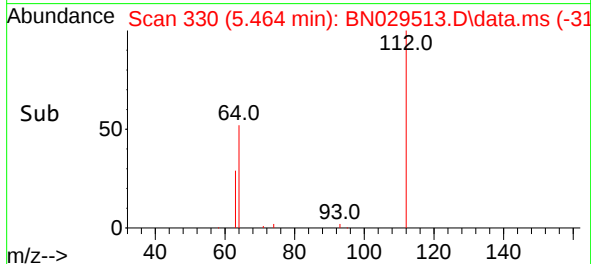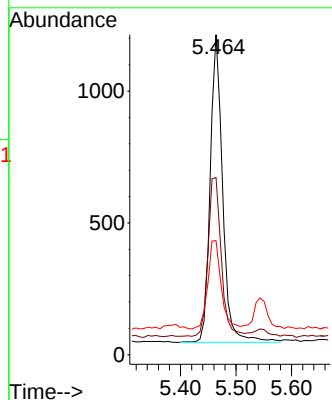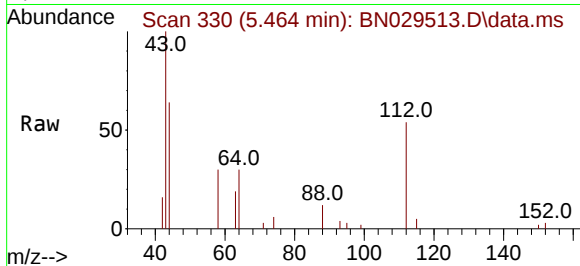

#5
Phenol-d6
Concen: 0.097 ng
RT: 7.060 min Scan# 551
Delta R.T. -0.000 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10

Tgt Ion: 99 Resp: 1106
Ion Ratio Lower Upper
99 100
42 24.4 16.9 25.3
71 44.7 30.0 45.0


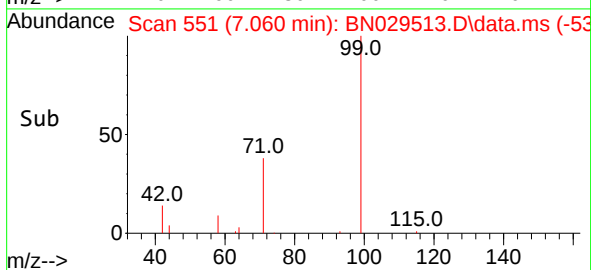
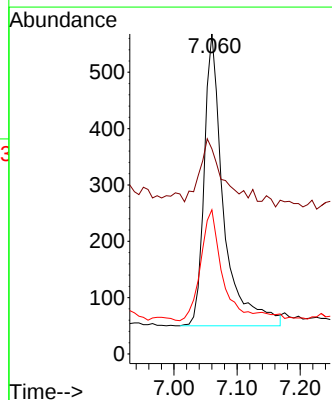
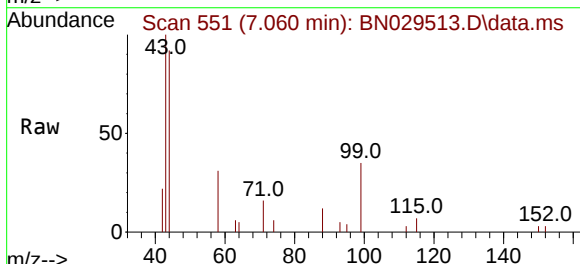




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.690 min Scan# 94
Delta R.T. -0.000 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10




Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-585-587


Tgt Ion:	136	Resp:	11029
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.7	14.5
54	8.6	6.6	10.0
68	7.3	5.7	8.5

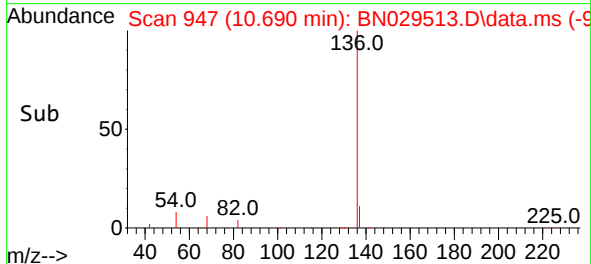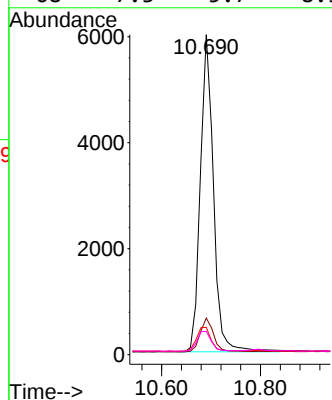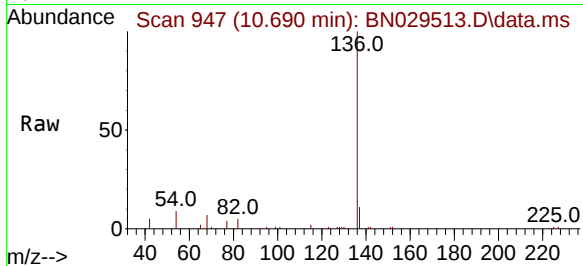

#8
Nitrobenzene-d5
Concen: 0.350 ng
RT: 9.057 min Scan# 794
Delta R.T. -0.000 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10

Tgt Ion:	82	Resp:	3218
Ion	Ratio	Lower	Upper
82	100		
128	38.7	31.6	47.4
54	49.7	38.2	57.4


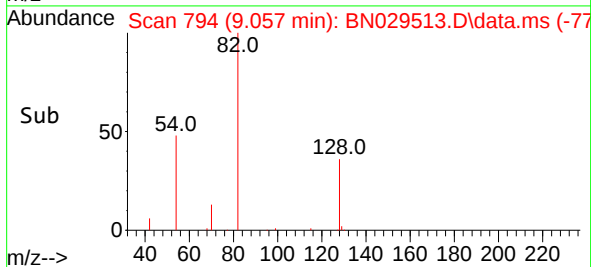
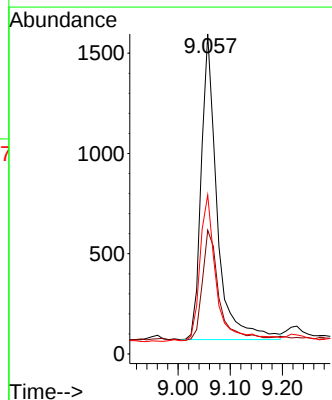
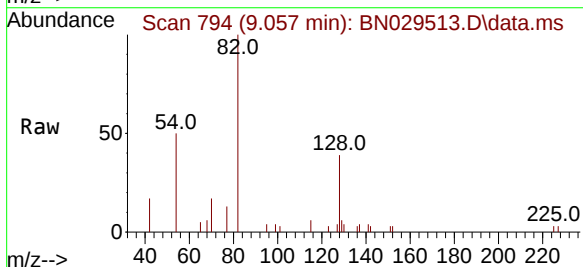


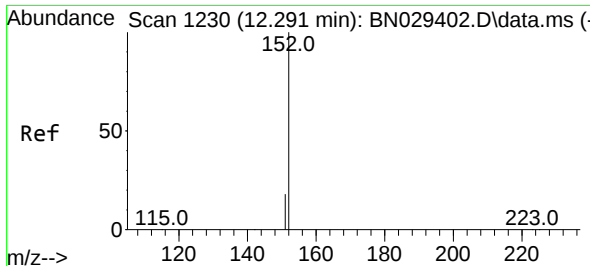

#11
2-Methylnaphthalene-d10
Concen: 0.376 ng
RT: 12.284 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10




Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-585-587


Tgt Ion:152 Resp: 5641
Ion Ratio Lower Upper
152 100
151 21.0 17.1 25.7

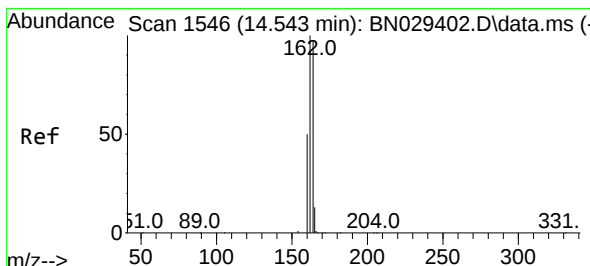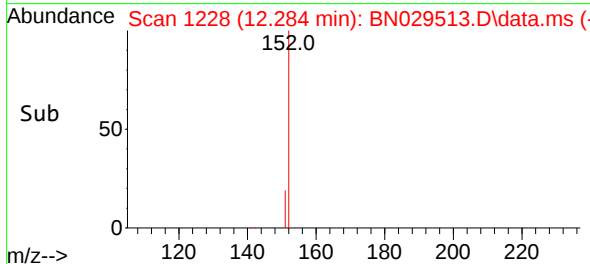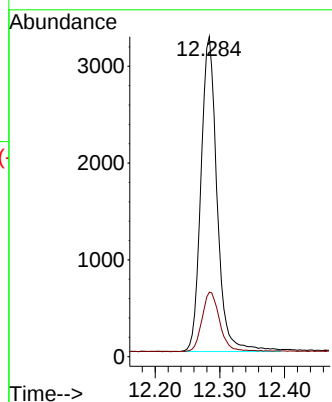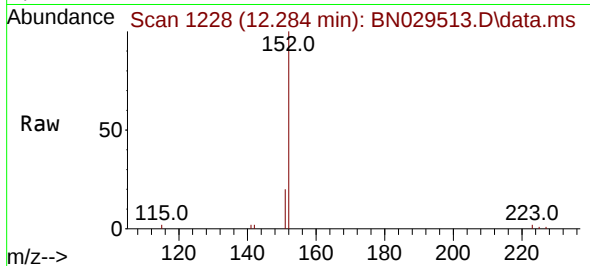

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.532 min Scan# 1545
Delta R.T. -0.000 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10


Tgt Ion:164 Resp: 4857
Ion Ratio Lower Upper
164 100
162 103.8 82.6 123.8
160 51.9 41.5 62.3

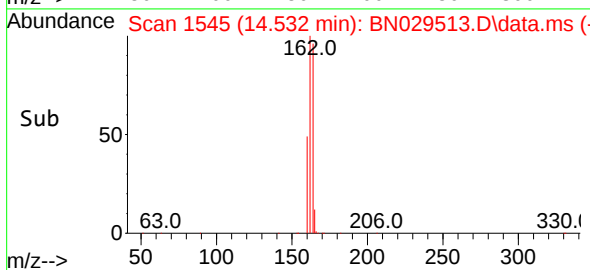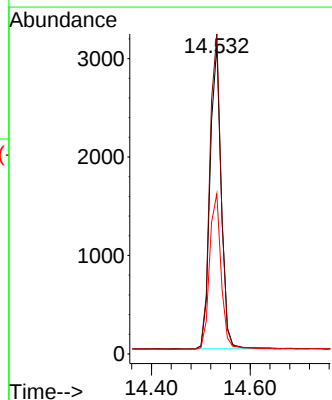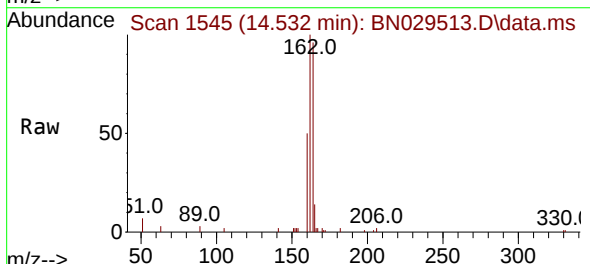






#14
2,4,6-Tribromophenol
Concen: 0.341 ng
RT: 16.027 min Scan# 1
Delta R.T. -0.000 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10

Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-585-587



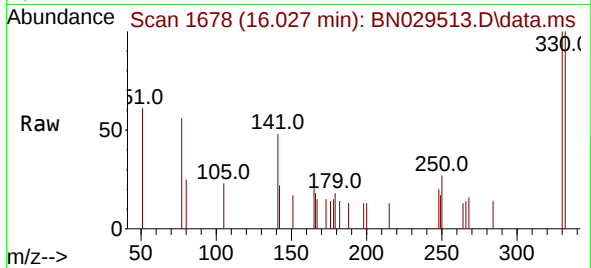



Tgt Ion:330 Resp: 532
Ion Ratio Lower Upper
330 100
332 97.2 76.0 114.0
141 62.2 43.4 65.2

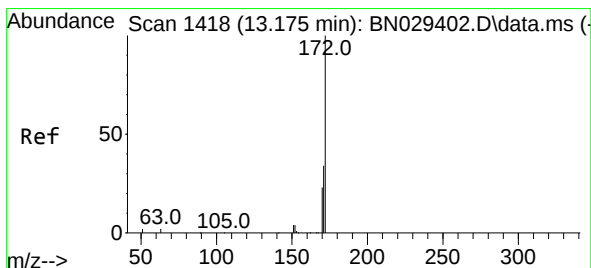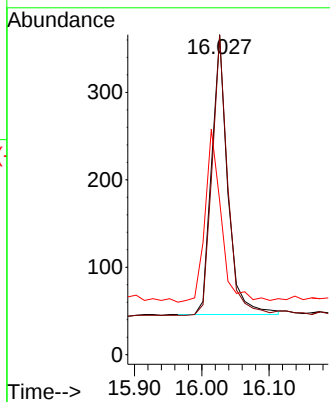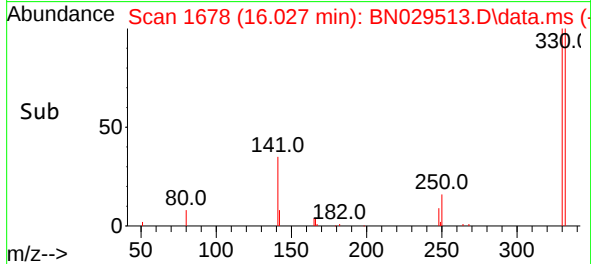

#15
2-Fluorobiphenyl
Concen: 0.427 ng
RT: 13.164 min Scan# 1417
Delta R.T. -0.000 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10

Tgt Ion:172 Resp: 8906
Ion Ratio Lower Upper
172 100
171 33.5 28.0 42.0
170 23.0 18.7 28.1


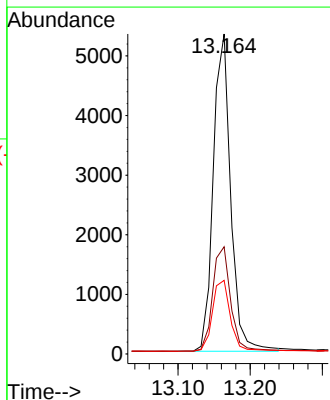
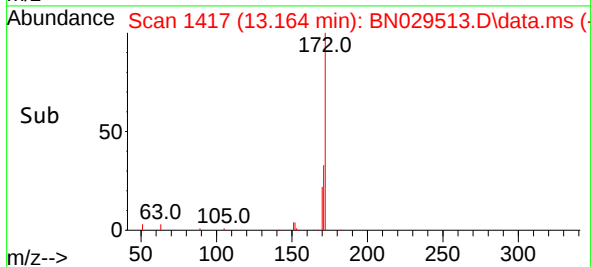
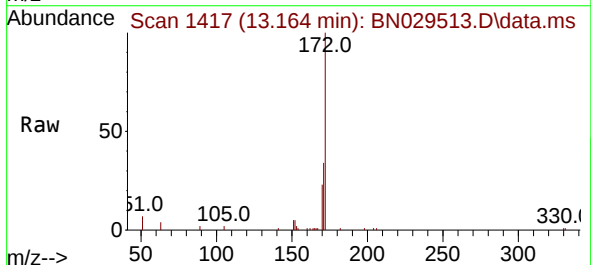




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.280 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10




Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-585-587


Tgt Ion:188 Resp: 8902
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.1 10.0 15.0

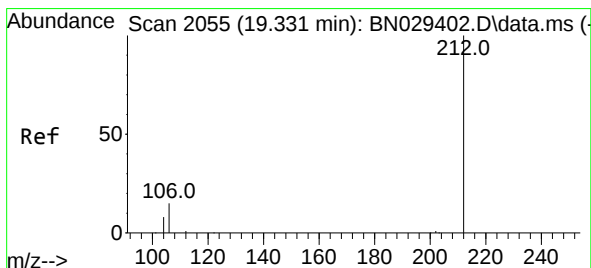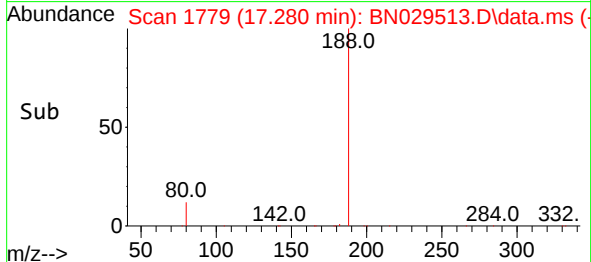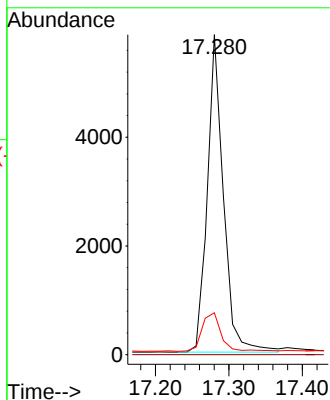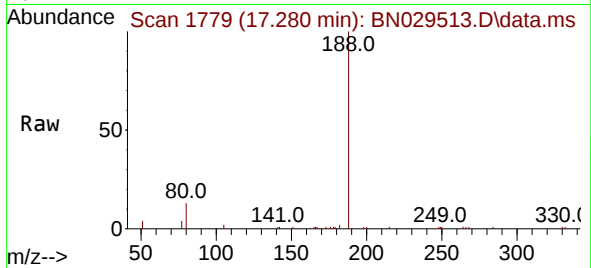

#27
Fluoranthene-d10
Concen: 0.400 ng
RT: 19.317 min Scan# 2052
Delta R.T. -0.005 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10

Tgt Ion:212 Resp: 8629
Ion Ratio Lower Upper
212 100
106 17.2 13.2 19.8
104 10.4 7.7 11.5


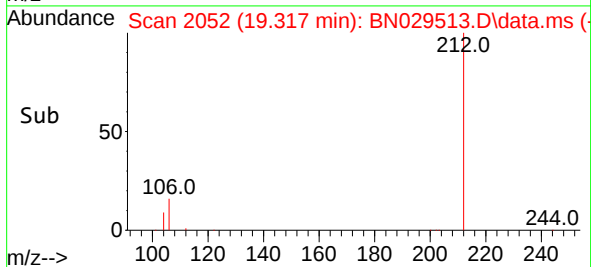
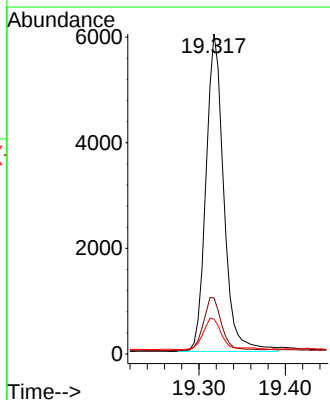
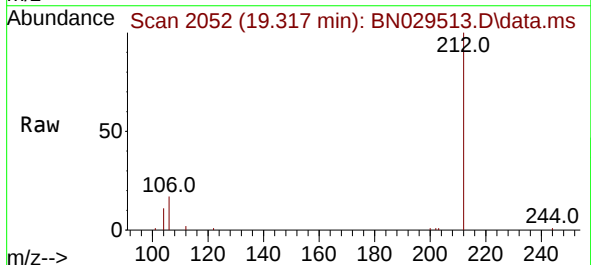




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.483 min Scan# 2469
Delta R.T. -0.009 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10




Instrument :
BNA_N
ClientSampleId :
BP-VPB-195-GW-585-587


Tgt Ion:240 Resp: 6031
Ion Ratio Lower Upper
240 100
120 17.8 16.7 25.1
236 29.0 23.9 35.9

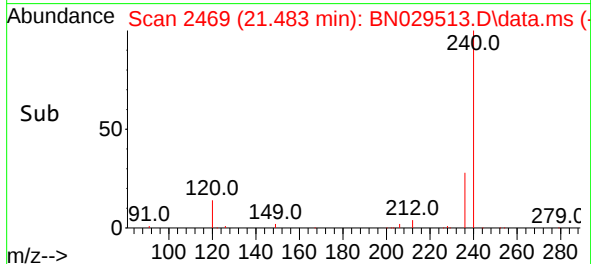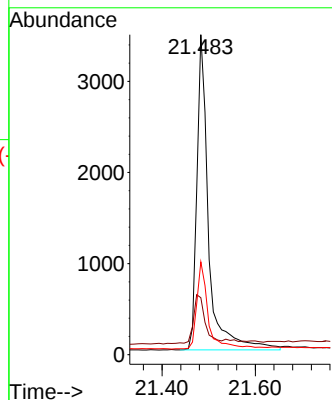

#31
Terphenyl-d14
Concen: 0.409 ng
RT: 19.926 min Scan# 2183
Delta R.T. -0.005 min
Lab File: BN029513.D
Acq: 05 Feb 2024 18:10

Tgt Ion:244 Resp: 6118
Ion Ratio Lower Upper
244 100
212 10.3 8.2 12.4
122 19.0 15.6 23.4


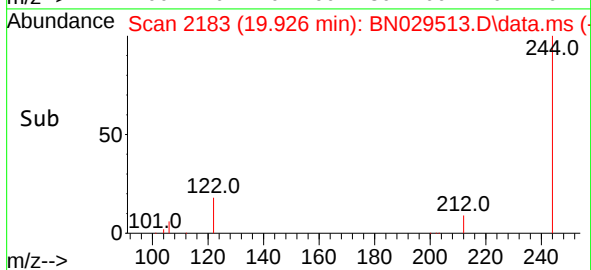
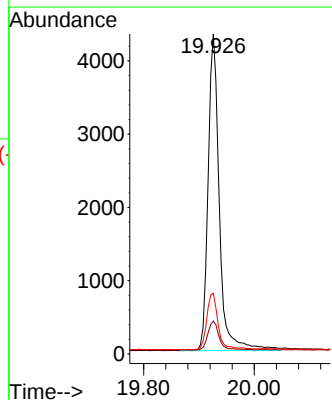
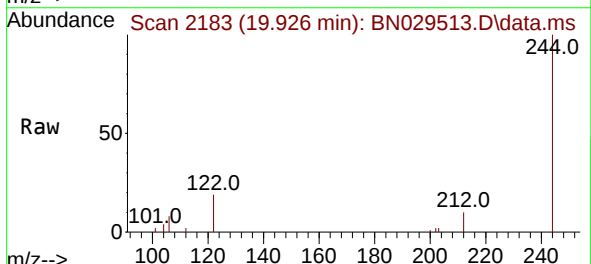


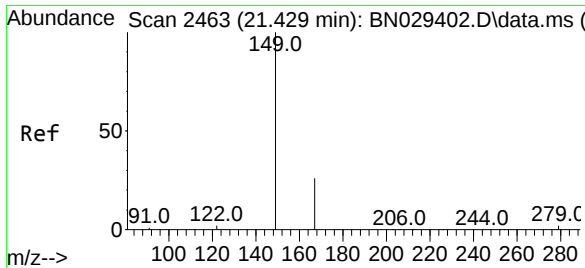

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.042 ng
 RT: 21.411 min Scan# 2461
 Delta R.T. -0.009 min
 Lab File: BN029513.D
 Acq: 05 Feb 2024 18:10

Instrument :
 BNA_N
 ClientSampleId :
 BP-VPB-195-GW-585-587

Tgt Ion:149 Resp: 583
 Ion Ratio Lower Upper
 149 100
 167 23.0 20.1 30.1
 279 5.5 2.5 3.7#

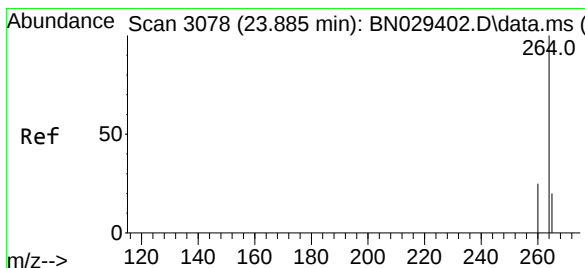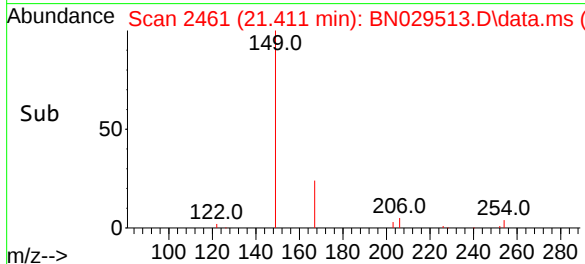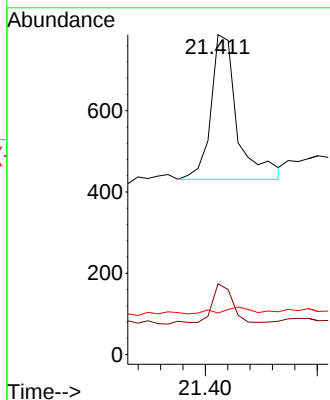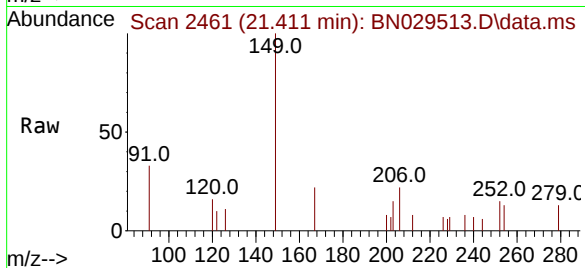

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.864 min Scan# 3071
 Delta R.T. -0.006 min
 Lab File: BN029513.D
 Acq: 05 Feb 2024 18:10

Tgt Ion:264 Resp: 6120
 Ion Ratio Lower Upper
 264 100
 260 27.3 21.2 31.8
 265 53.0 41.5 62.3

