
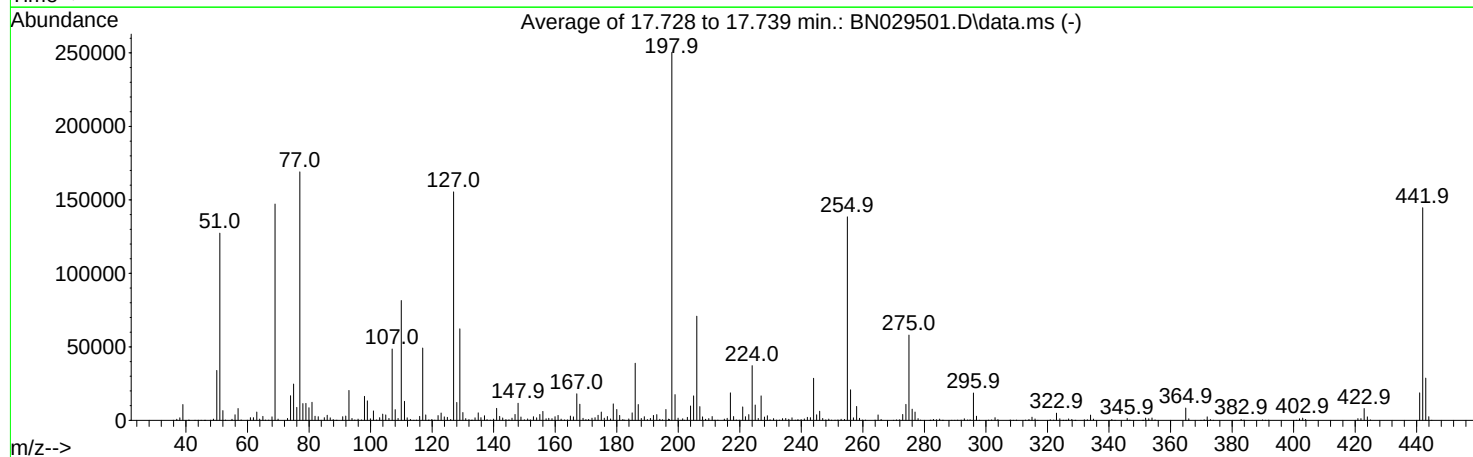


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029501.D
Acq On : 05 Feb 2024 10:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 01:51:59 2024

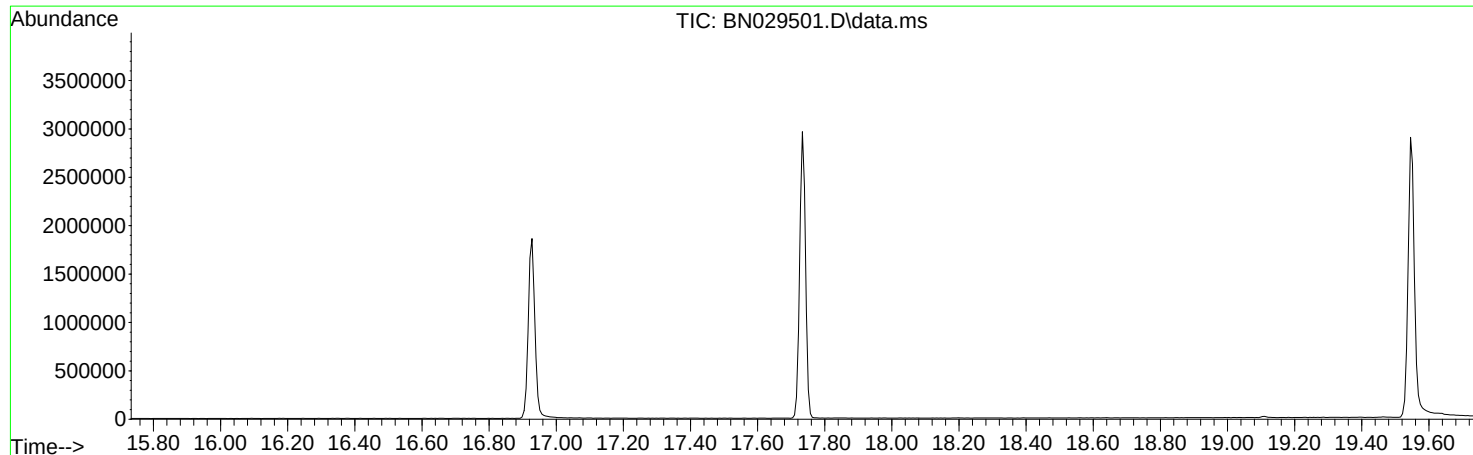




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.9	127357	PASS
68	69	0.00	2	1.7	2453	PASS
69	198	0.00	100	58.8	147141	PASS
70	69	0.00	2	0.6	863	PASS
127	198	10	80	62.1	155499	PASS
197	198	0.00	2	0.4	899	PASS
198	198	100	100	100.0	250283	PASS
199	198	5	9	7.0	17496	PASS
275	198	10	60	23.2	58021	PASS
365	198	1	100	3.3	8373	PASS
441	198	0.01	100	7.5	18766	PASS
442	442	50	100	100.0	144672	PASS
443	442	15	24	19.8	28701	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029501.D
Acq On : 05 Feb 2024 10:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 06 16:08:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 03:38:30 2024
Response via : Initial Calibration

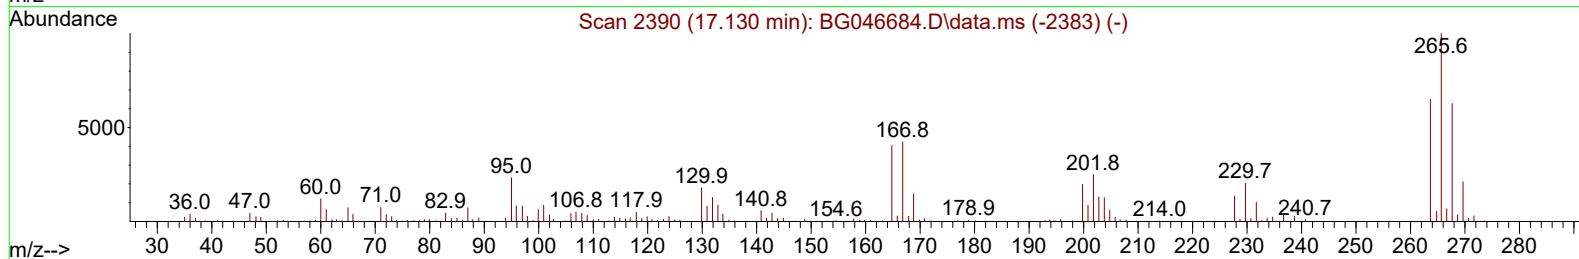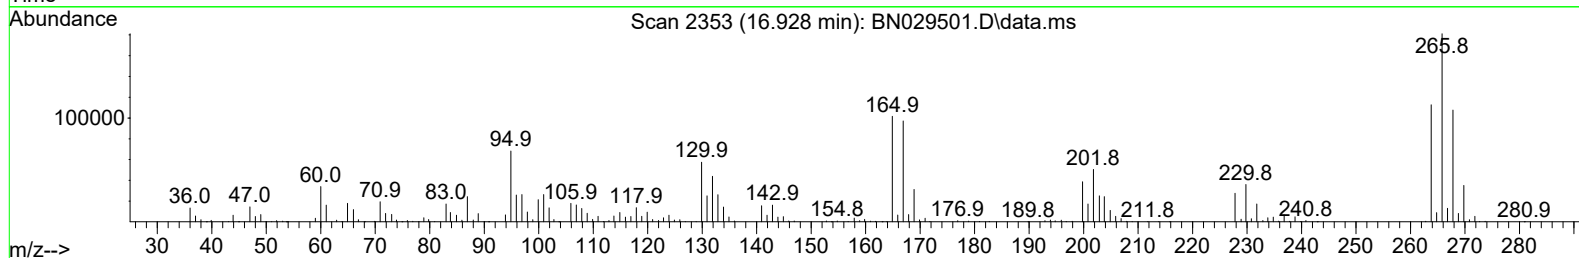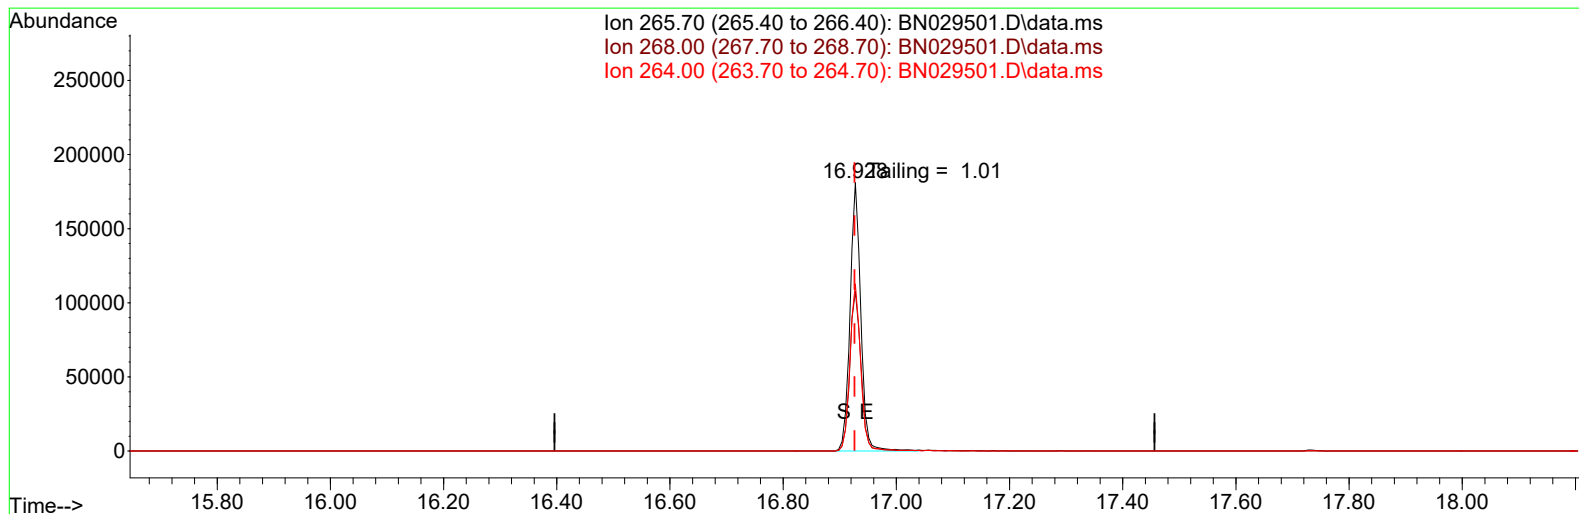

TIC: BN029501.D\data.ms

(70) Pentachlorophenol (C)

16.928min (+ 0.002) 16499.10 ng




response 239151

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.42
264.00	61.60	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029501.D
Acq On : 05 Feb 2024 10:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 06 16:08:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 03:38:30 2024
Response via : Initial Calibration

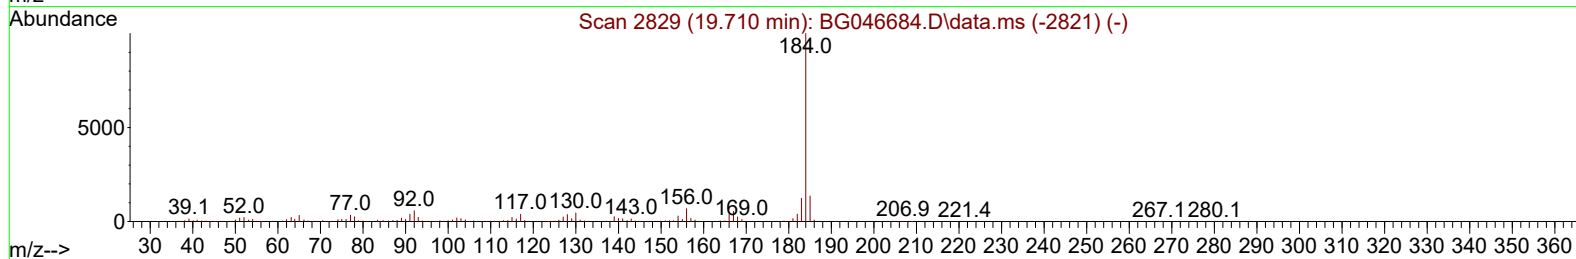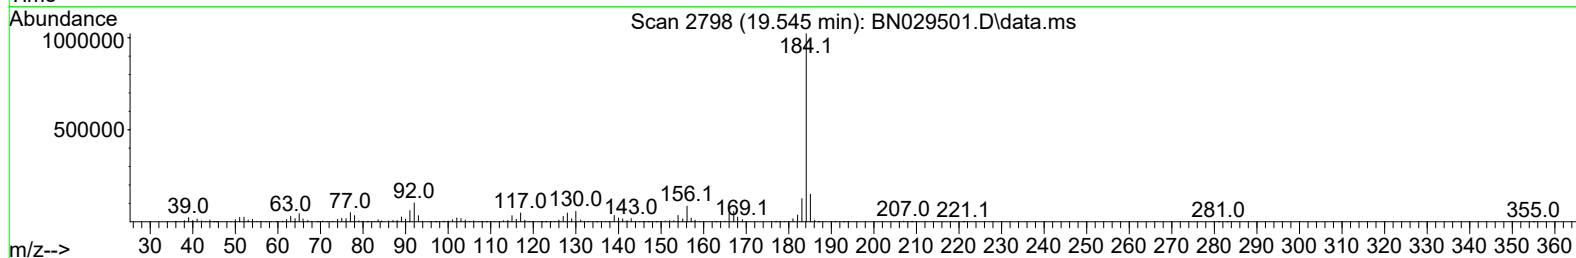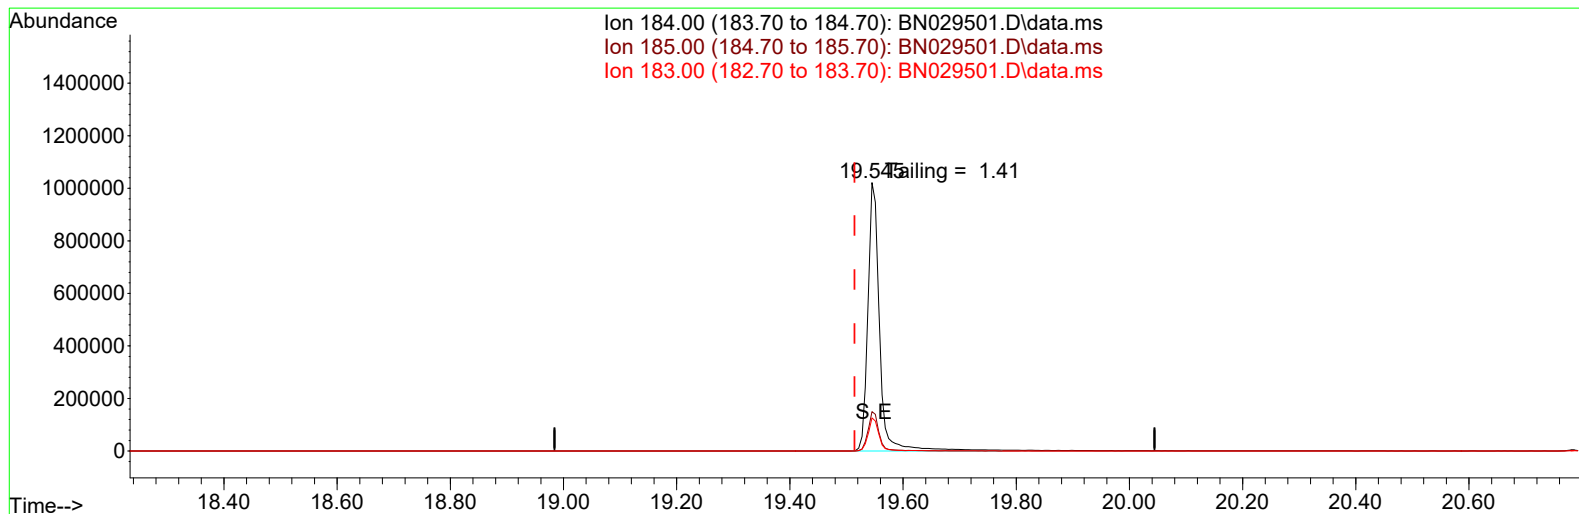

TIC: BN029501.D\data.ms

(77) Benzidine

19.545min (+ 0.031) 0.00 ng

response 1470767

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	12.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/6/2024	BNA_N	<u>BN029501.D</u>
Compound Name	Response	Retention Time
DDT	708904	20.78
DDD	8023	20.392
DDE	297	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8320	717224	1.16

Instrument :
BNA_N
ClientSampleId :
DFTPP