


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029520.D
Acq On : 05 Feb 2024 22:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 01:51:59 2024

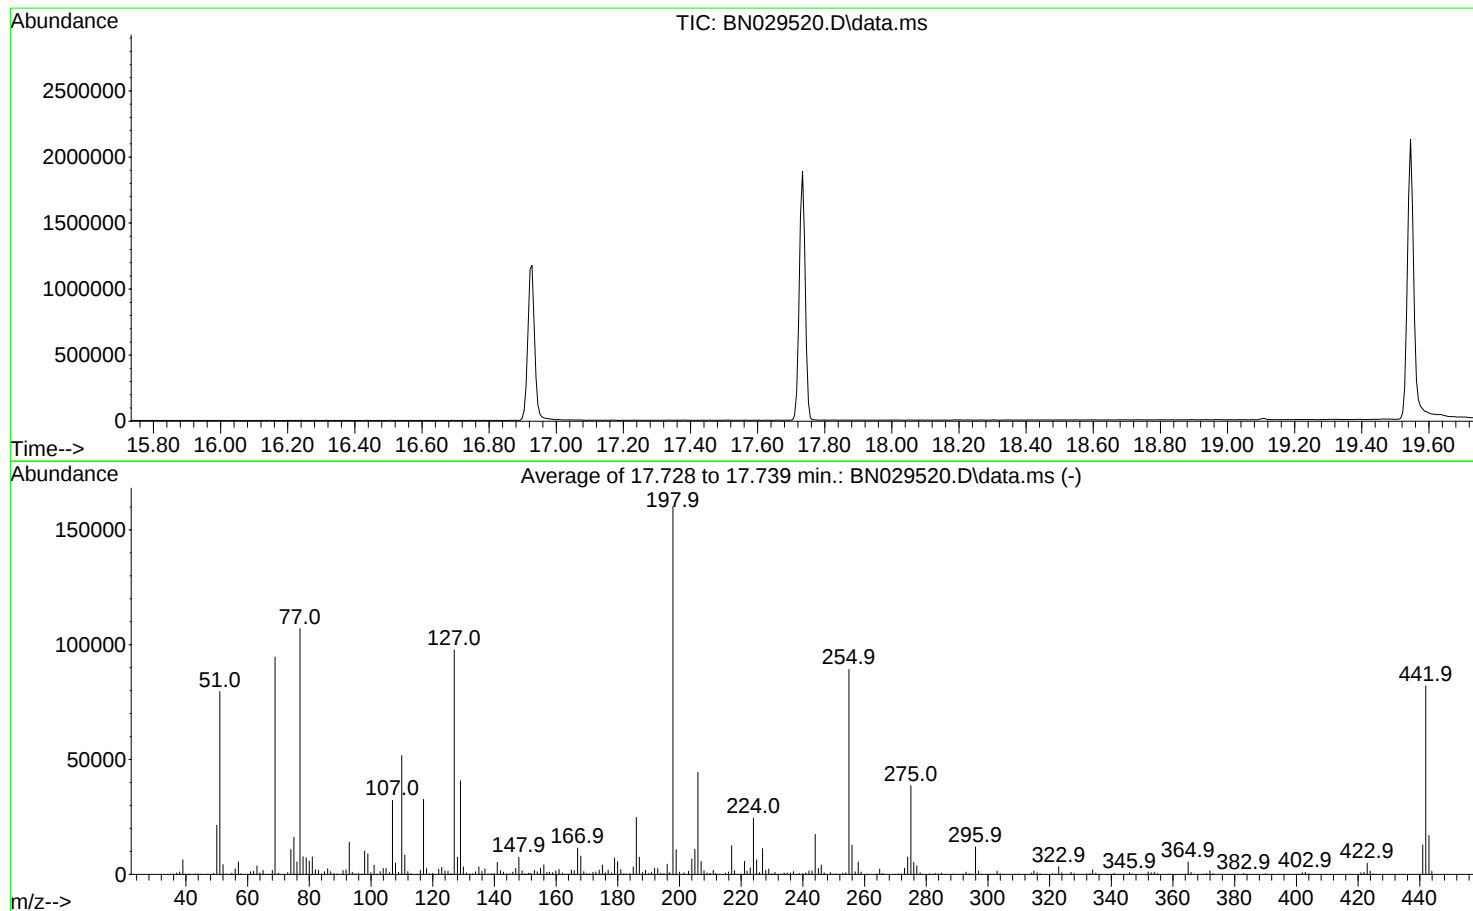




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.7	79576	PASS
68	69	0.00	2	1.9	1754	PASS
69	198	0.00	100	59.1	94648	PASS
70	69	0.00	2	0.6	576	PASS
127	198	10	80	61.0	97792	PASS
197	198	0.00	2	0.4	672	PASS
198	198	100	100	100.0	160192	PASS
199	198	5	9	6.7	10666	PASS
275	198	10	60	24.1	38683	PASS
365	198	1	100	3.3	5355	PASS
441	198	0.01	100	8.0	12827	PASS
442	442	50	100	100.0	82115	PASS
443	442	15	24	20.7	16966	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029520.D
Acq On : 05 Feb 2024 22:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 06 05:26:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 03:38:30 2024
Response via : Initial Calibration

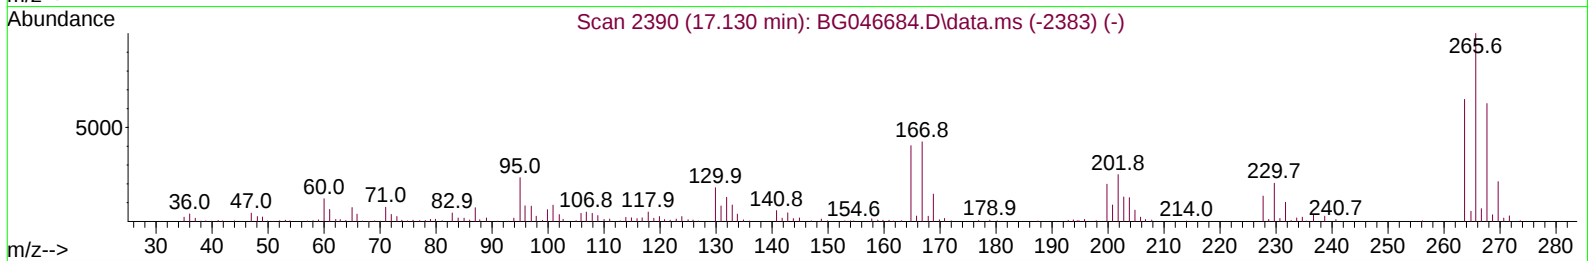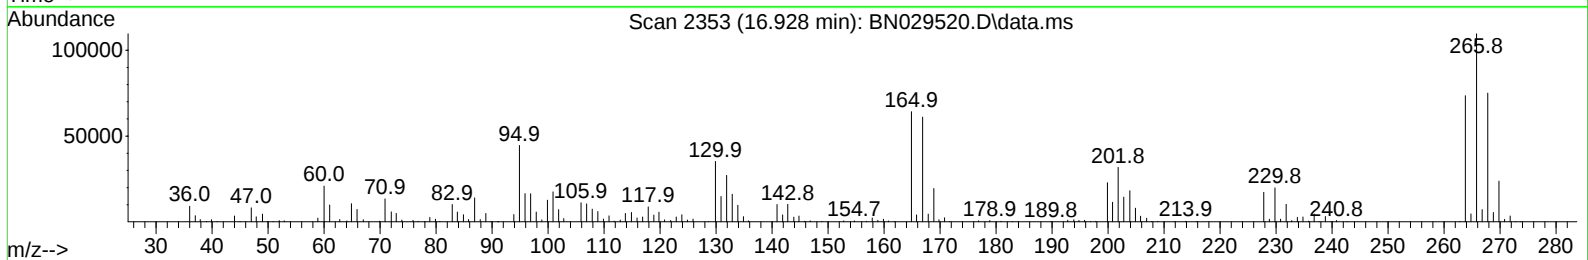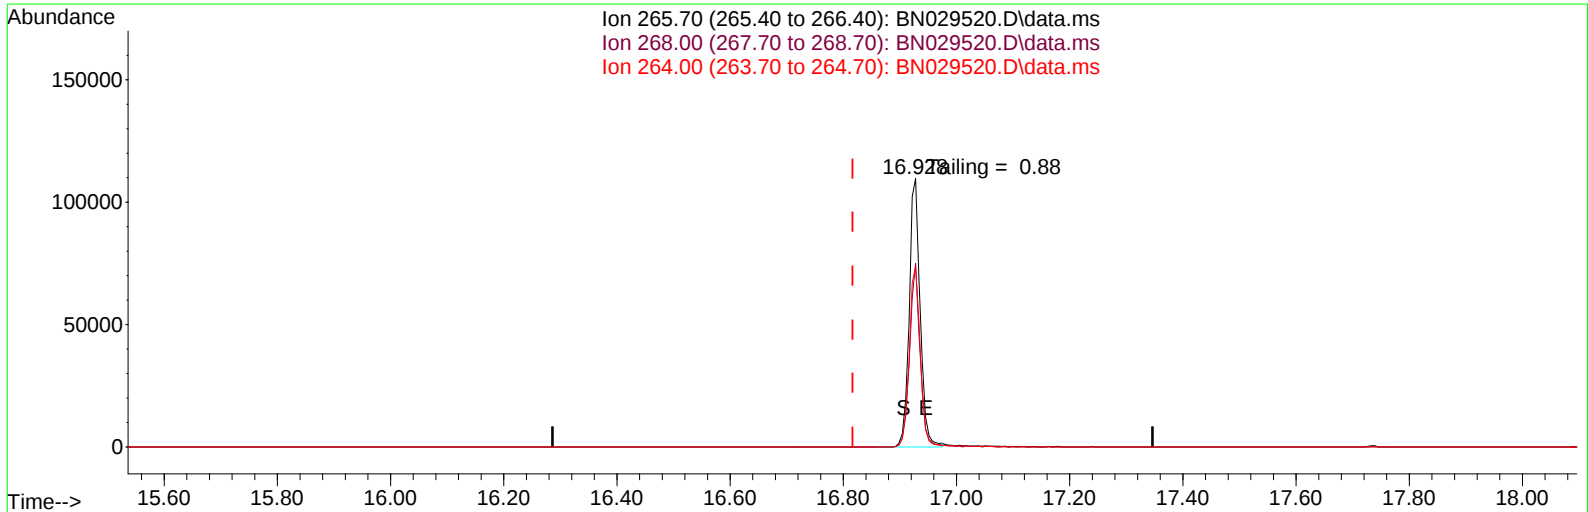

TIC: BN029520.D\data.ms

(70) Pentachlorophenol (C)

16.928min (+ 0.112) 16138.11 ng




response 147798

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.42
264.00	61.60	67.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020524\
Data File : BN029520.D
Acq On : 05 Feb 2024 22:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 06 05:26:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 03:38:30 2024
Response via : Initial Calibration

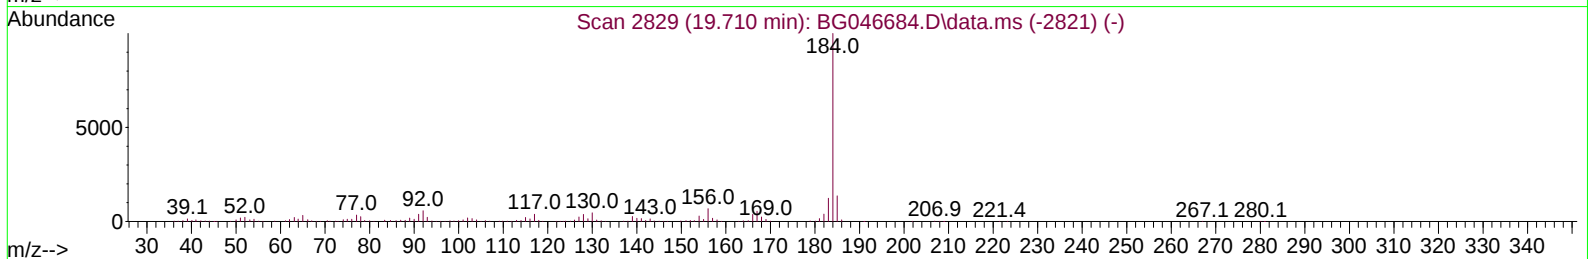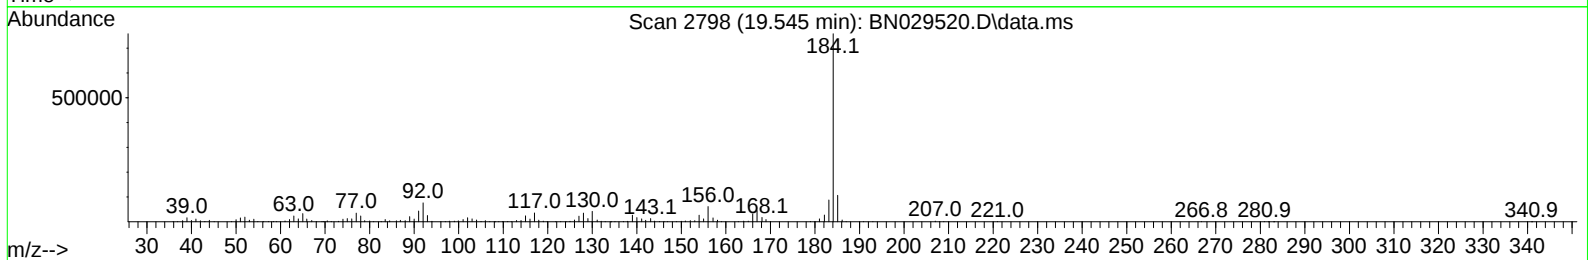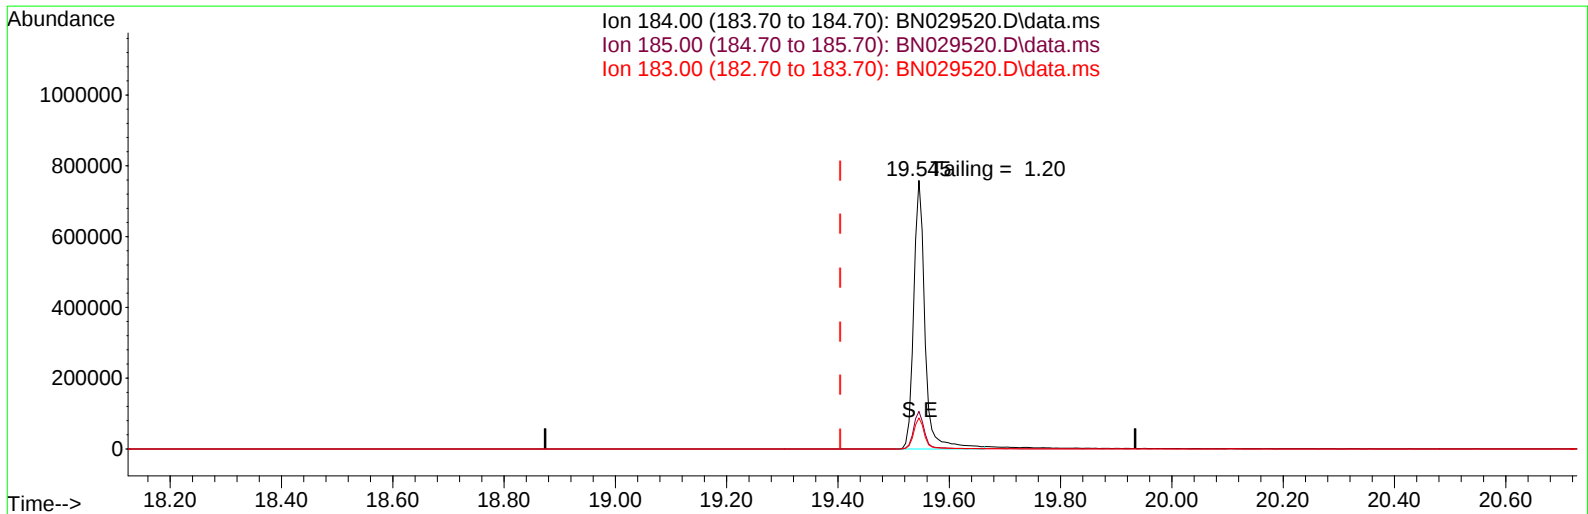

TIC: BN029520.D\data.ms

(77) Benzidine

19.545min (+ 0.141) 0.00 ng

response 1084015

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/5/2024	BNA_N	<u>BN029520.D</u>
Compound Name	Response	Retention Time
DDT	516992	20.781
DDD	6466	20.392
DDE	0	0
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6466	523458	1.24

Instrument :
BNA_N
ClientSampleId :
DFTPP