
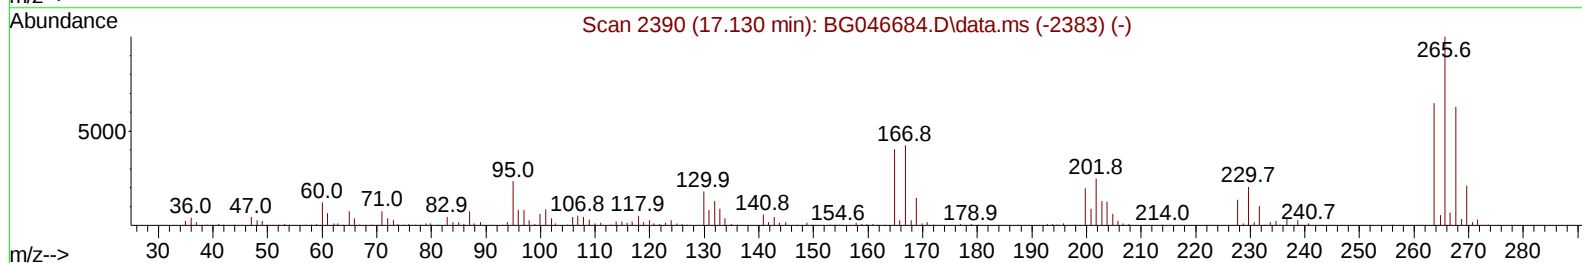
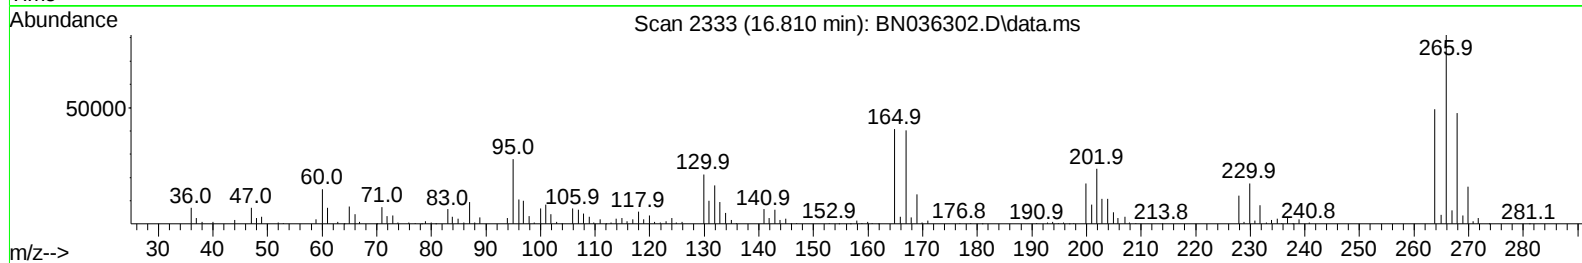


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020525\
Data File : BN036302.D
Acq On : 05 Feb 2025 18:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 03:02:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

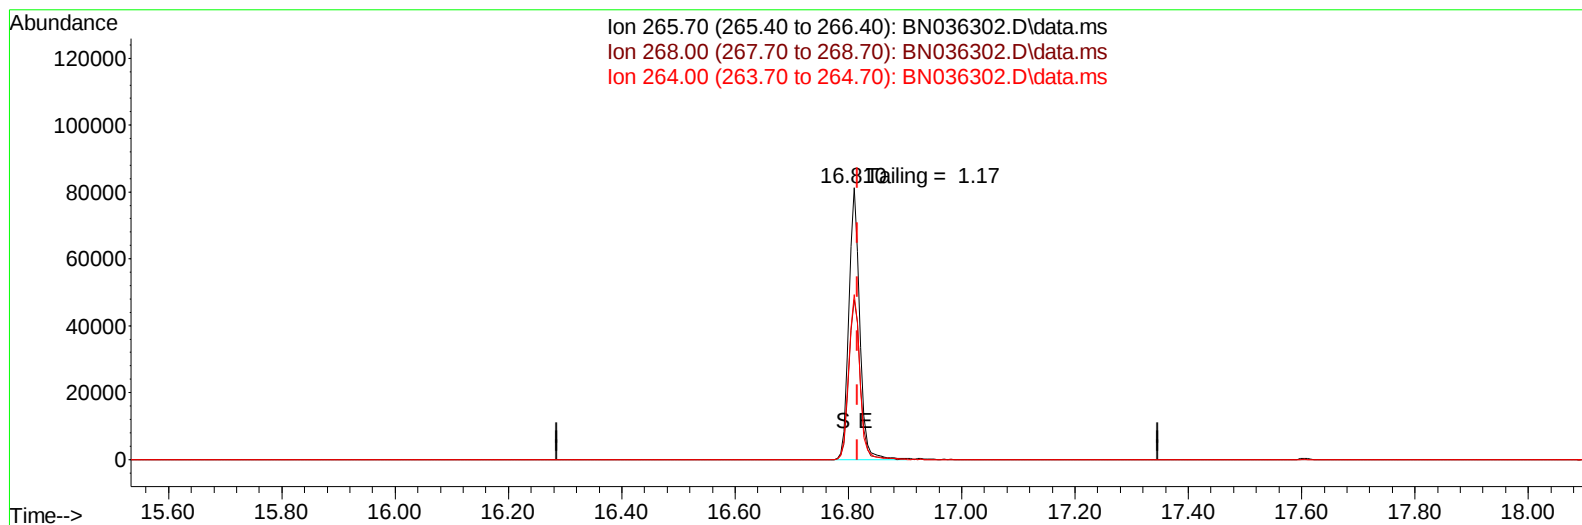




TIC: BN036302.D\data.ms

(70) Pentachlorophenol (C)**16.810min (-0.006) 17367.43 ng****response 108491**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.74
264.00	61.60	60.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020525\
Data File : BN036302.D
Acq On : 05 Feb 2025 18:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 03:02:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

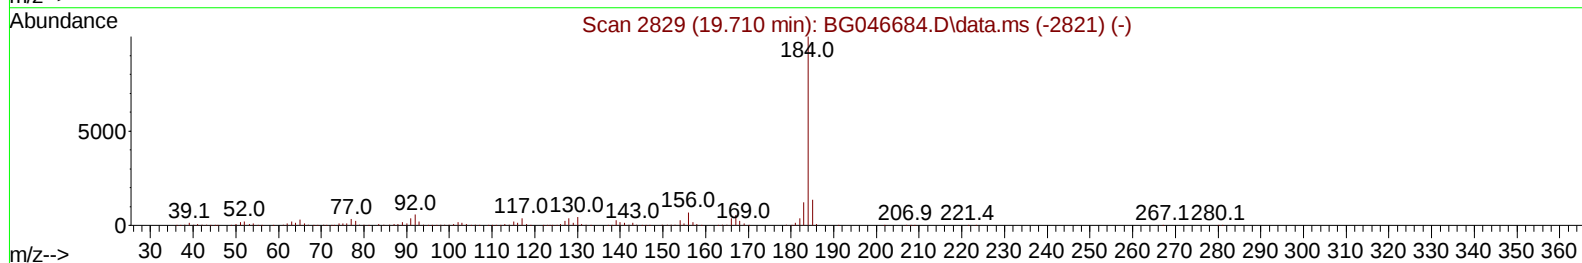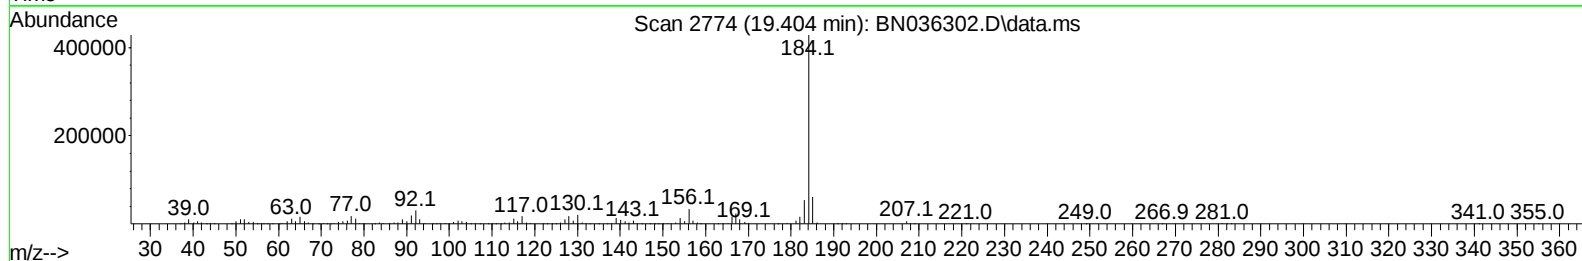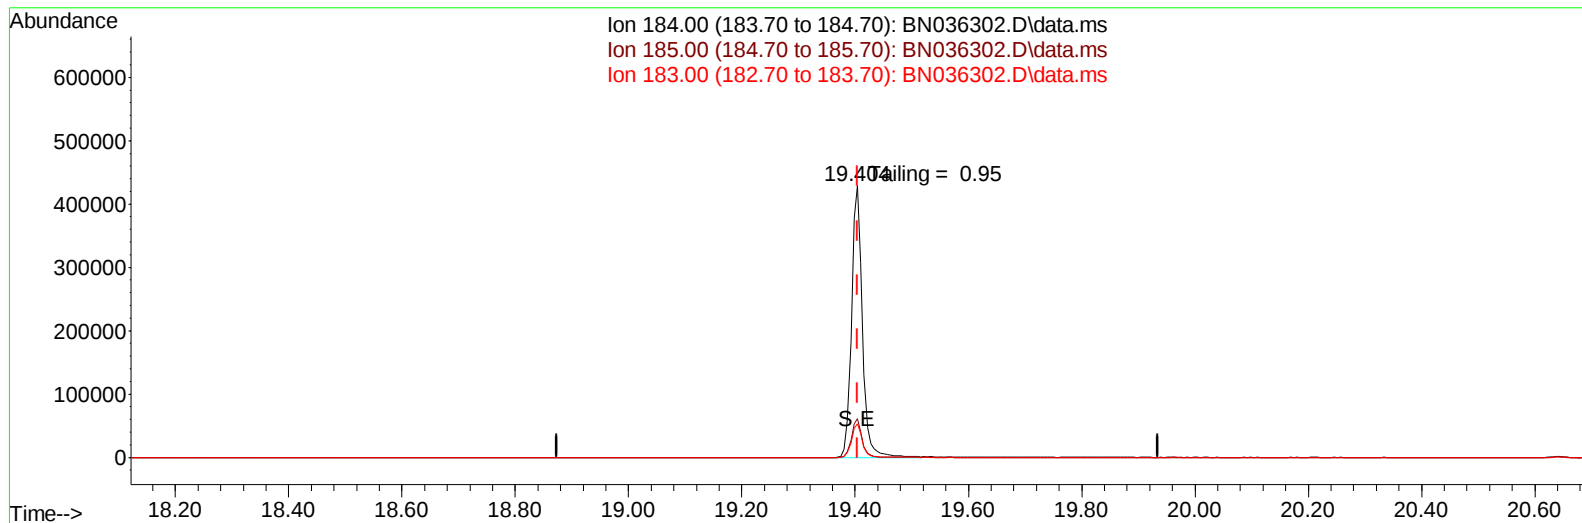

TIC: BN036302.D\data.ms

(77) Benzidine**19.404min (-0.000) 0.00 ng****response 576937**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.34
183.00	13.20	12.49
0.00	0.00	0.00