
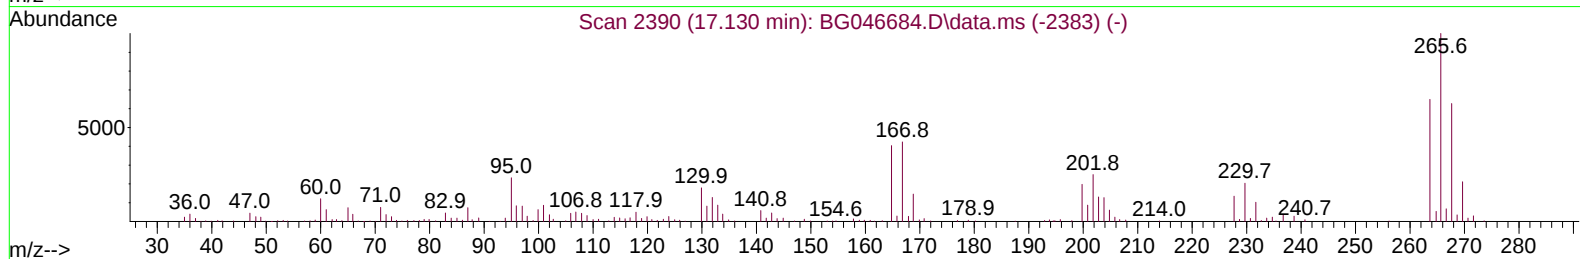
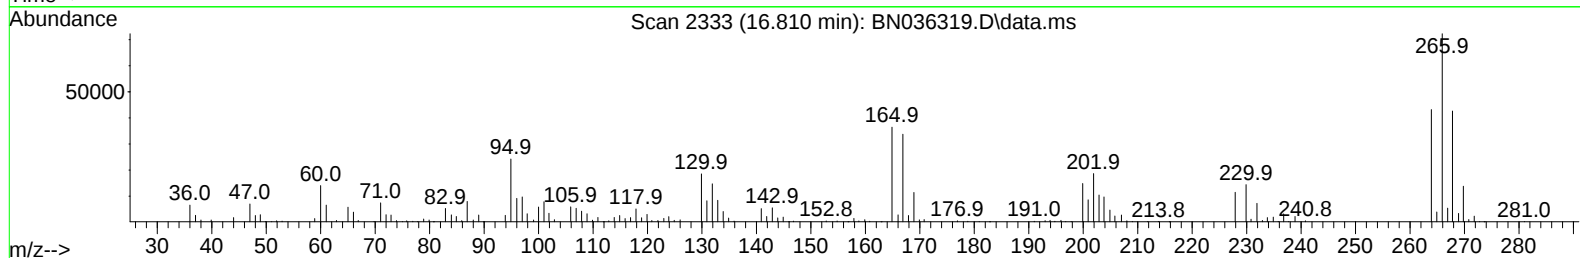


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020525\
Data File : BN036319.D
Acq On : 06 Feb 2025 05:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Feb 06 07:50:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

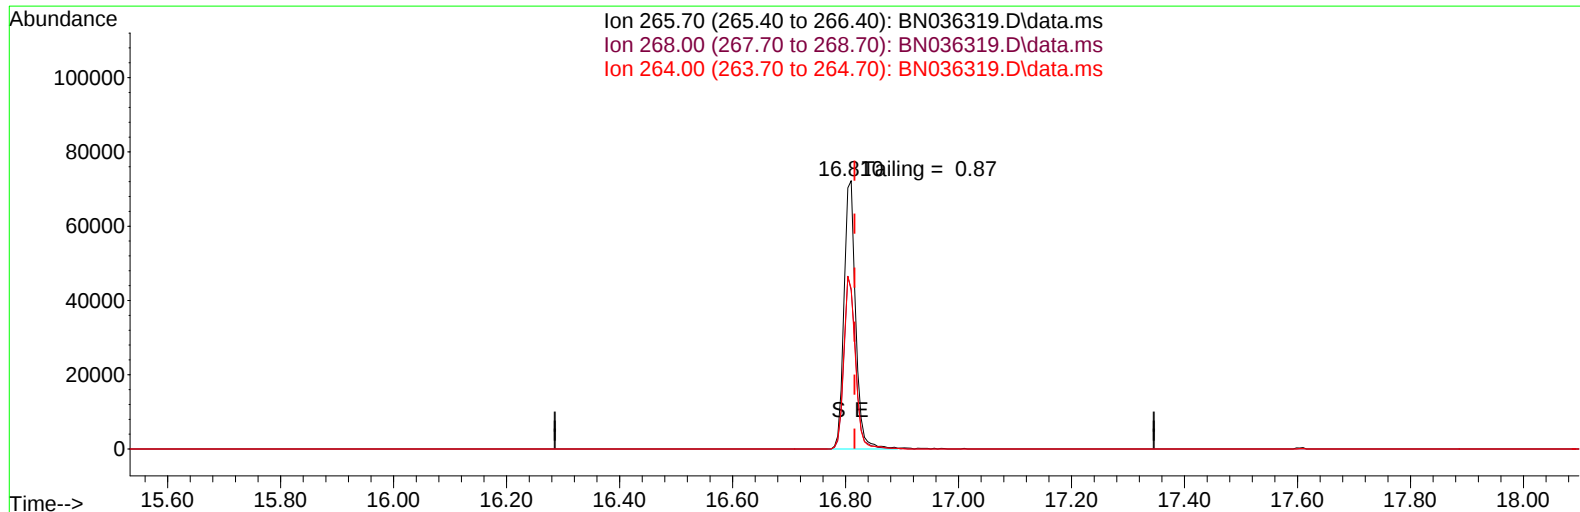

TIC: BN036319.D\data.ms

(70) Pentachlorophenol (C)




16.810min (-0.006) 17584.32 ng

response 103084

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.02
264.00	61.60	59.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020525\
Data File : BN036319.D
Acq On : 06 Feb 2025 05:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Feb 06 07:50:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

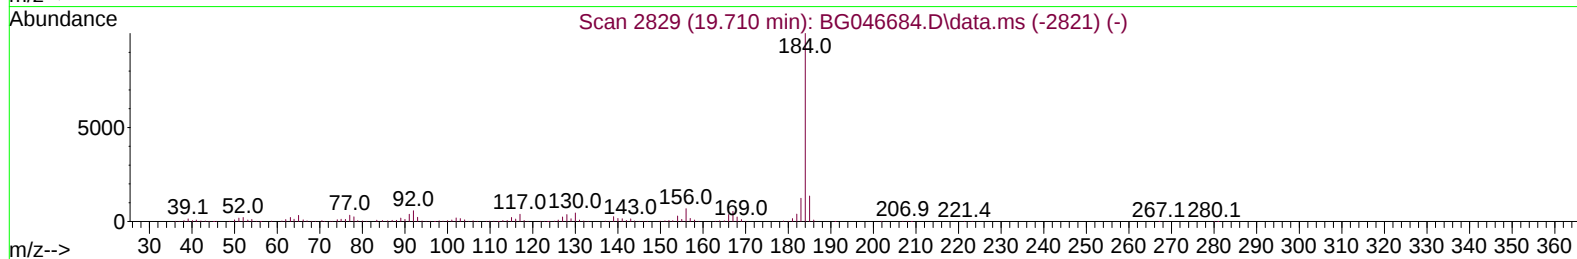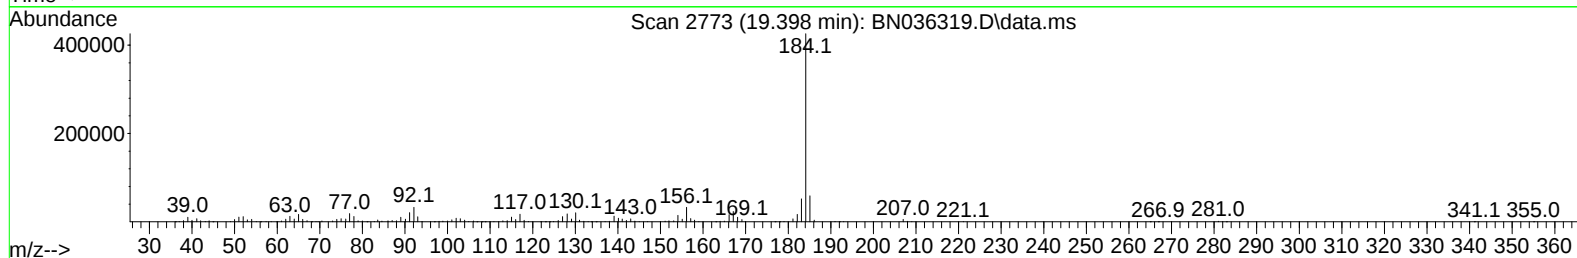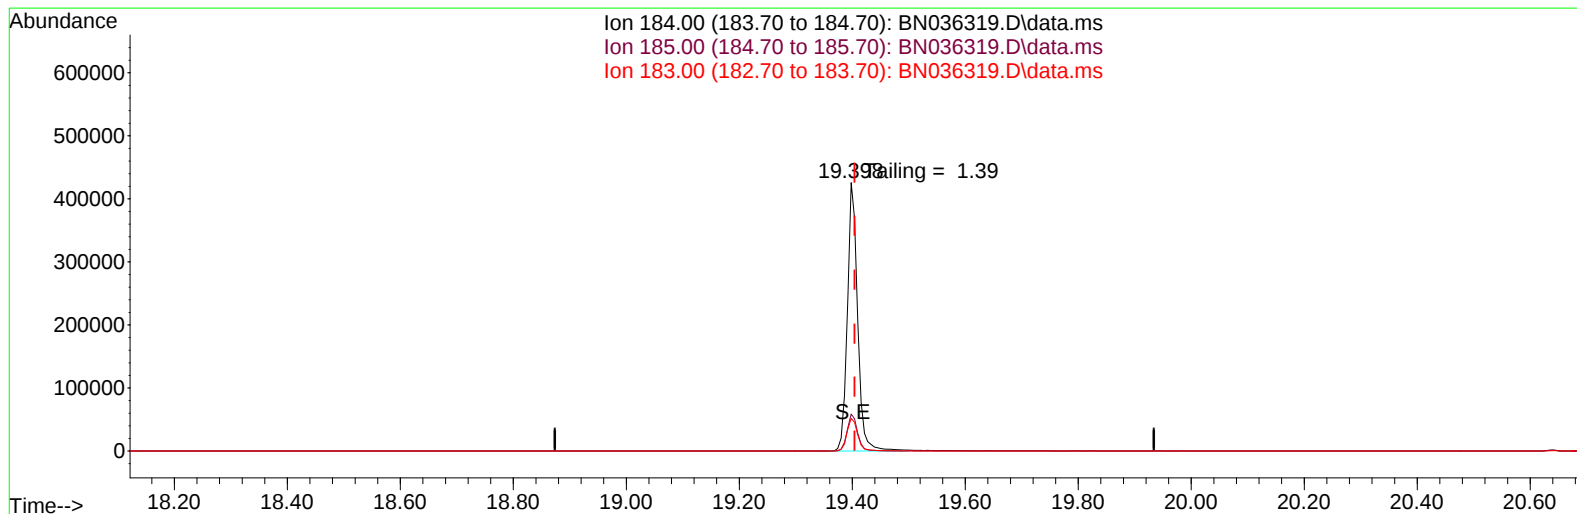

TIC: BN036319.D\data.ms

(77) Benzdine

19.398min (-0.006) 0.00 ng

response 542068

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	12.17
0.00	0.00	0.00